

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049045.D
 Acq On : 11 Jun 2022 10:39
 Operator : SY/MD
 Sample : N3249-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rBV2	248623	300879	10.97%	2.444%
2	1.906	168	176	192	rVB	73887	100369	3.66%	0.815%
3	2.565	369	381	396	rBV2	181483	308272	11.24%	2.504%
4	2.691	418	420	422	rBV2	572	249	0.01%	0.002%
5	2.983	508	511	514	rBV2	242	221	0.01%	0.002%
6	3.109	546	550	552	rBV	255	212	0.01%	0.002%
7	3.122	552	554	558	rBV	309	218	0.01%	0.002%
8	3.170	562	569	570	rBV3	1919	1489	0.05%	0.012%
9	3.353	613	626	643	rBV2	33361	67006	2.44%	0.544%
10	3.800	761	765	766	rBV2	368	222	0.01%	0.002%
11	3.868	766	786	814	rVV	584423	1381673	50.40%	11.222%
12	4.054	842	844	847	rBV2	352	202	0.01%	0.002%
13	4.147	870	873	875	rBV3	261	192	0.01%	0.002%
14	4.276	912	913	914	rBV	147	40	0.00%	0.000%
15	4.343	930	934	936	rBV2	212	149	0.01%	0.001%
16	4.443	963	965	966	rBV2	152	66	0.00%	0.001%
17	4.491	978	980	981	rBV	205	80	0.00%	0.001%
18	4.559	997	1001	1002	rBV	289	168	0.01%	0.001%
19	4.665	1007	1034	1064	rBV2	1101397	2741584	100.00%	22.267%
20	5.064	1143	1158	1180	rVB	181828	398586	14.54%	3.237%
21	5.241	1211	1213	1215	rVB2	369	118	0.00%	0.001%
22	5.314	1219	1236	1256	rVV	311106	702011	25.61%	5.702%
23	5.723	1341	1363	1379	rBV2	350176	956814	34.90%	7.771%
24	5.964	1435	1438	1443	rVB	370	279	0.01%	0.002%
25	6.041	1460	1462	1463	rBV	261	72	0.00%	0.001%
26	6.144	1492	1494	1496	rBV	235	112	0.00%	0.001%
27	6.247	1512	1526	1545	rBV	296682	566404	20.66%	4.600%
28	6.543	1605	1618	1632	rBV	81524	153891	5.61%	1.250%
29	6.691	1650	1664	1682	rBV	228972	446910	16.30%	3.630%
30	6.839	1708	1710	1712	rBV2	187	56	0.00%	0.000%
31	6.974	1745	1752	1762	rVB3	2067	3555	0.13%	0.029%
32	7.031	1767	1770	1774	rBV	381	346	0.01%	0.003%
33	7.157	1808	1809	1810	rBV	294	105	0.00%	0.001%
34	7.466	1902	1905	1908	rBV2	240	196	0.01%	0.002%
35	7.511	1917	1919	1923	rBV2	174	82	0.00%	0.001%
36	7.565	1924	1936	1954	rBV2	99228	174850	6.38%	1.420%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049045.D
 Acq On : 11 Jun 2022 10:39
 Operator : SY/MD
 Sample : N3249-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	7.771	1998	2000	2002	rVB	249	92	0.00%	0.001%
38	7.787	2002	2005	2006	rBV	546	322	0.01%	0.003%
39	7.896	2026	2039	2061	rBV	411597	712819	26.00%	5.789%
40	8.179	2116	2127	2142	rBV	71275	117905	4.30%	0.958%
41	8.401	2189	2196	2205	rVB6	3681	5827	0.21%	0.047%
42	8.552	2232	2243	2256	rBV2	53428	90221	3.29%	0.733%
43	8.633	2256	2268	2300	rBV3	301949	600904	21.92%	4.880%
44	8.851	2334	2336	2340	rBV3	318	209	0.01%	0.002%
45	8.948	2365	2366	2367	rBV	131	43	0.00%	0.000%
46	9.160	2429	2432	2436	rBV2	268	191	0.01%	0.002%
47	9.221	2446	2451	2453	rBV	330	340	0.01%	0.003%
48	9.324	2481	2483	2484	rBV	111	40	0.00%	0.000%
49	9.417	2499	2512	2540	rBV	410435	689690	25.16%	5.602%
50	9.694	2590	2598	2601	rBV2	1017	1073	0.04%	0.009%
51	9.970	2682	2684	2687	rVB	402	205	0.01%	0.002%
52	10.099	2721	2724	2728	rBV2	351	244	0.01%	0.002%
53	10.327	2792	2795	2798	rBV	329	252	0.01%	0.002%
54	10.340	2798	2799	2801	rVB	254	90	0.00%	0.001%
55	10.697	2907	2910	2912	rBV	279	184	0.01%	0.001%
56	10.755	2916	2928	2945	rVV	352947	567180	20.69%	4.607%
57	10.887	2966	2969	2970	rBV3	1183	670	0.02%	0.005%
58	11.083	3028	3030	3036	rBV3	466	474	0.02%	0.004%
59	11.186	3054	3062	3065	rBV	474	523	0.02%	0.004%
60	11.240	3075	3079	3082	rVB	320	224	0.01%	0.002%
61	11.282	3090	3092	3099	rVB2	384	233	0.01%	0.002%
62	11.813	3244	3257	3279	rBV	363116	580387	21.17%	4.714%
63	12.070	3332	3337	3340	rVB	512	481	0.02%	0.004%
64	12.086	3340	3342	3343	rBV	301	122	0.00%	0.001%
65	12.096	3343	3345	3348	rVV2	372	165	0.01%	0.001%
66	12.192	3363	3375	3392	rBV	384604	630906	23.01%	5.124%
67	12.359	3424	3427	3429	rBV2	279	204	0.01%	0.002%
68	12.478	3458	3464	3471	rBV2	425	799	0.03%	0.006%
69	12.706	3533	3535	3537	rBV	234	113	0.00%	0.001%
70	13.793	3869	3873	3876	rBV3	548	559	0.02%	0.005%
71	13.845	3886	3889	3895	rBV3	518	697	0.03%	0.006%
72	14.404	4059	4063	4065	rBV2	348	331	0.01%	0.003%




Sum of corrected areas: 12312397

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049045.D
Acq On : 11 Jun 2022 10:39
Operator : SY/MD
Sample : N3249-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

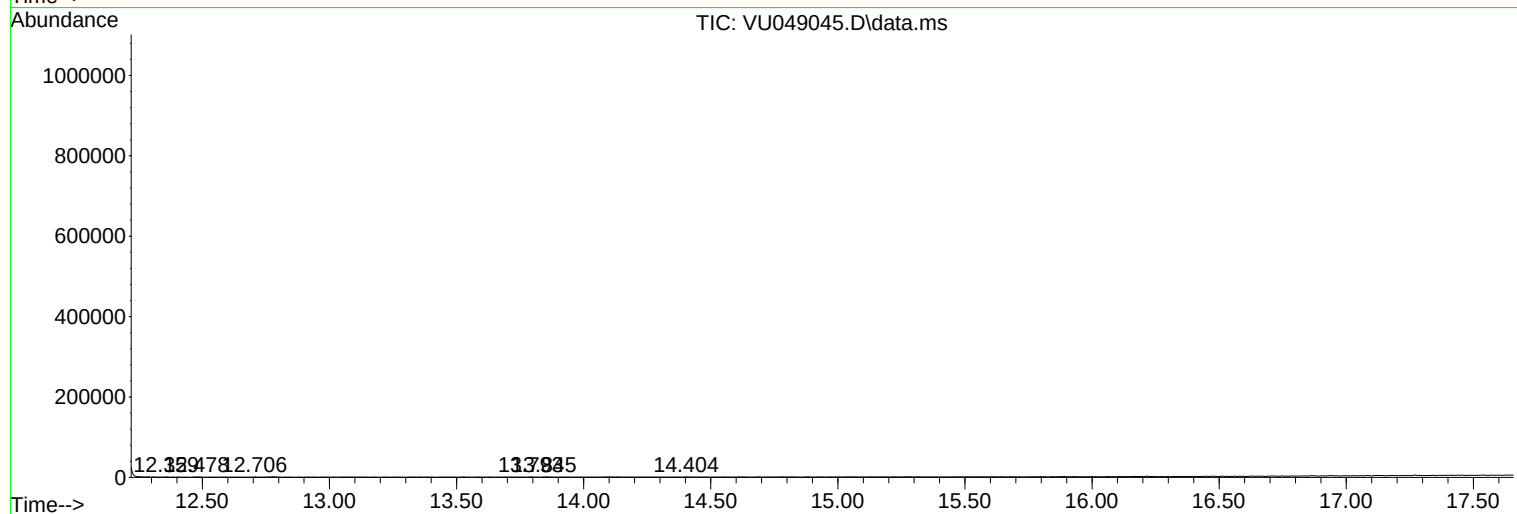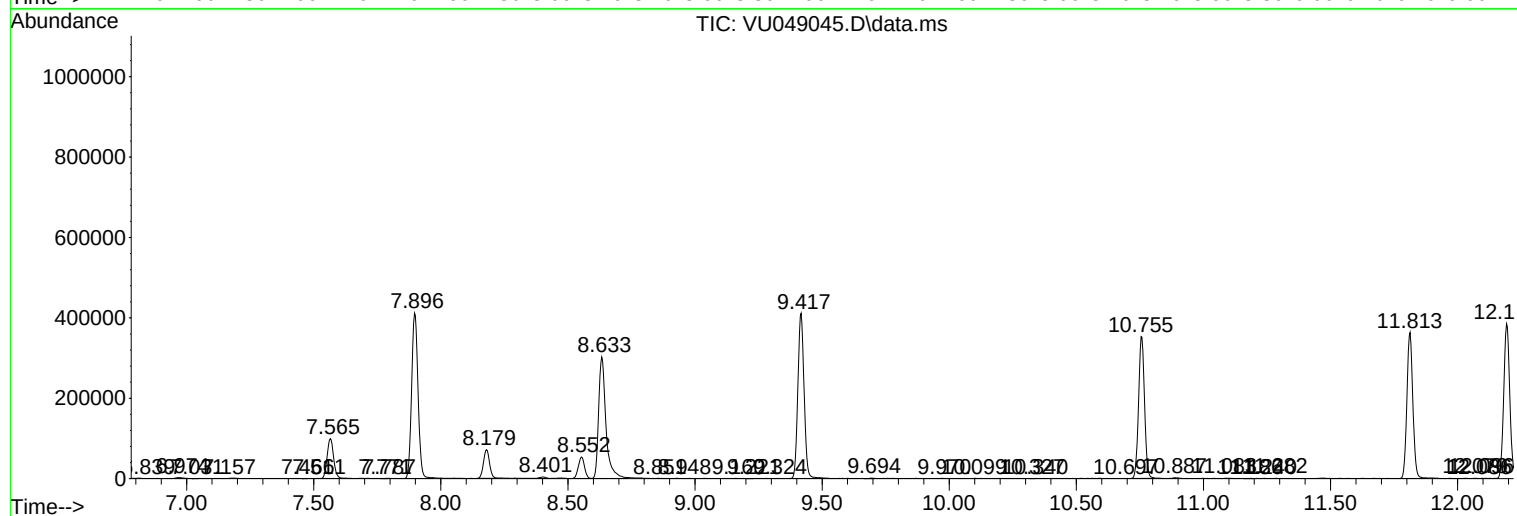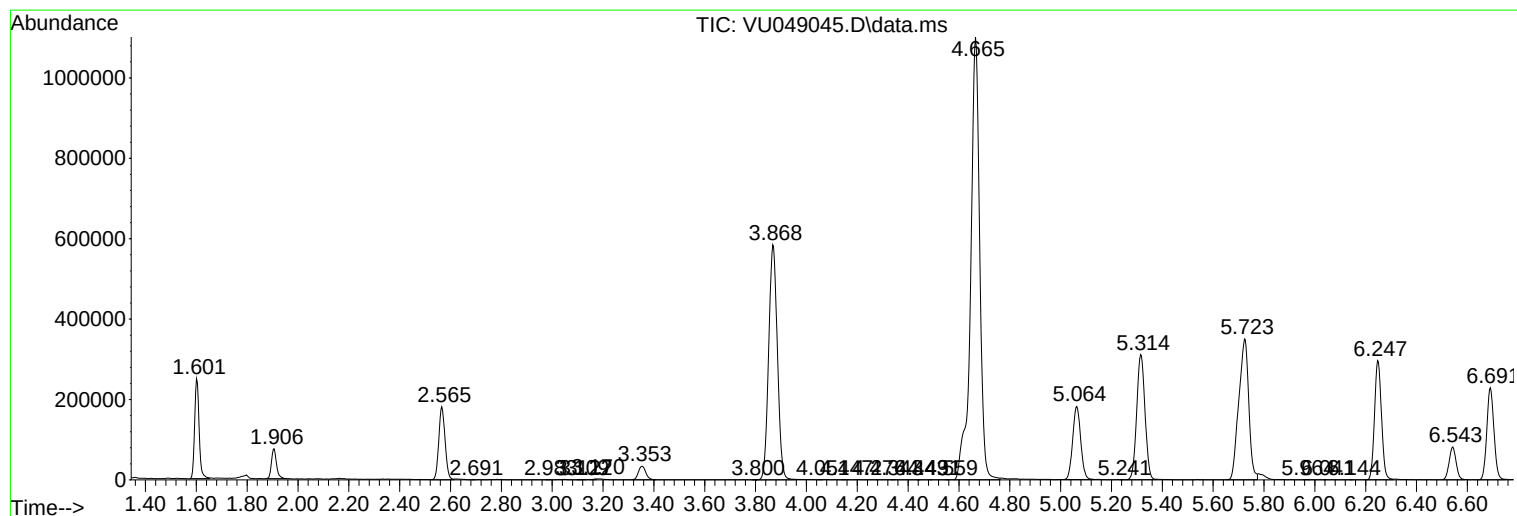

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049045.D
Acq On : 11 Jun 2022 10:39
Operator : SY/MD
Sample : N3249-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049045.D
Acq On : 11 Jun 2022 10:39
Operator : SY/MD
Sample : N3249-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc