


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU048990.D
 Acq On : 10 Jun 2022 11:20
 Operator : SY/MD
 Sample : BFB095
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB095

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis
 Last Update : Mon Jun 13 05:01:30 2022

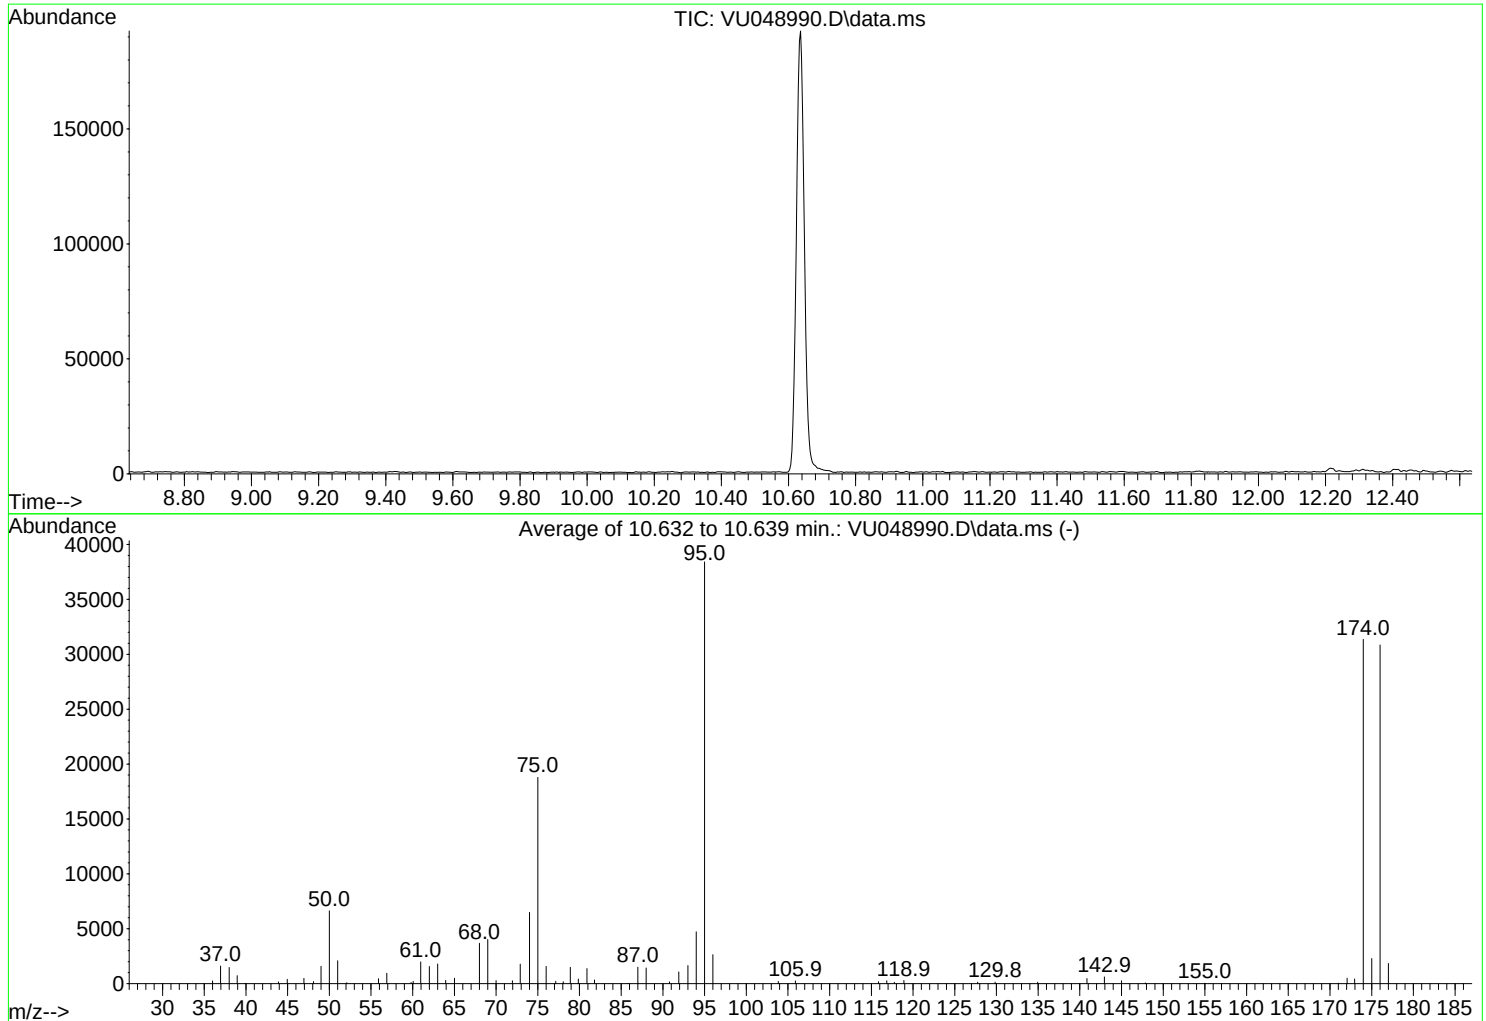

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	6634	PASS
75	95	30	80	48.9	18787	PASS
95	95	100	100	100.0	38419	PASS
96	95	5	9	6.9	2636	PASS
173	174	0.00	2	1.3	423	PASS
174	95	50	120	81.6	31357	PASS
175	174	5	9	7.3	2290	PASS
176	174	95	101	98.4	30848	PASS
177	176	5	9	6.0	1837	PASS

m/z	Abundance
39.90	290.0
44.00	407.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

m/z	Abundance
36.00	267.0
36.90	1616.0
38.00	1526.0
38.90	710.0
39.90	330.0
43.90	603.0
44.90	419.0
46.90	441.0
48.10	203.0
49.00	1647.0
50.00	6603.0
51.00	2203.0
55.90	486.0
56.90	957.0
60.10	329.0
61.00	1834.0
62.00	1621.0
63.00	1782.0
64.00	296.0
65.00	598.0
68.00	3735.0
69.00	4034.0
70.00	278.0
71.90	227.0
72.90	1942.0
74.00	6599.0
75.00	19664.0
76.00	1675.0
77.10	228.0
78.00	208.0
78.90	1385.0
79.80	437.0
80.90	1418.0
81.80	358.0
87.00	1397.0
88.00	1442.0
90.80	175.0
91.90	1130.0
93.00	1719.0
94.00	4633.0
95.00	39048.0
96.00	2664.0
103.90	220.0
105.90	212.0
115.80	188.0
116.80	275.0
117.70	104.0
118.90	267.0
127.80	141.0
129.80	166.0
135.00	123.0
140.80	493.0
143.00	600.0
145.00	293.0
147.90	109.0
171.00	126.0
172.10	434.0
173.00	484.0
174.00	31032.0
175.00	2281.0
176.00	30032.0
177.00	1695.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

m/z	Abundance
36.00	267.0
37.00	1624.0
38.00	1522.0
38.90	760.0
39.90	320.0
43.90	560.0
44.90	427.0
47.00	497.0
48.10	192.0
49.00	1624.0
50.00	6882.0
51.00	2125.0
52.10	122.0
55.90	462.0
56.90	964.0
60.00	302.0
61.00	2025.0
62.00	1536.0
63.00	1884.0
63.90	297.0
65.00	536.0
68.00	3794.0
69.00	4246.0
70.00	308.0
71.90	267.0
72.90	1771.0
74.00	6780.0
75.00	19264.0
76.00	1631.0
77.20	231.0
78.10	213.0
78.90	1529.0
79.80	444.0
80.90	1413.0
81.80	353.0
85.80	109.0
87.00	1577.0
88.00	1462.0
90.80	175.0
91.90	1090.0
93.00	1648.0
94.00	4893.0
95.00	39480.0
96.00	2758.0
103.90	195.0
105.90	262.0
115.80	176.0
116.80	290.0
117.80	139.0
118.90	299.0
127.70	125.0
129.90	150.0
134.90	145.0
140.90	463.0
143.00	614.0
145.00	230.0
172.00	509.0
173.00	403.0
174.00	32152.0
175.00	2355.0
176.00	31768.0
177.00	1888.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

m/z	Abundance
36.00	232.0
37.00	1592.0
38.00	1372.0
39.00	735.0
39.90	318.0
43.90	562.0
45.00	358.0
47.00	506.0
48.10	179.0
49.00	1437.0
50.00	6418.0
51.00	1912.0
52.10	124.0
55.90	406.0
56.90	932.0
59.80	305.0
60.90	2072.0
62.00	1518.0
63.00	1733.0
63.90	272.0
65.00	376.0
68.00	3484.0
69.00	3782.0
70.00	252.0
72.00	280.0
72.90	1611.0
74.00	6080.0
75.00	17432.0
76.00	1415.0
77.20	208.0
78.10	124.0
78.90	1550.0
79.90	400.0
80.90	1271.0
81.80	281.0
87.00	1536.0
88.00	1371.0
90.80	154.0
91.90	981.0
93.00	1598.0
94.00	4637.0
95.00	36728.0
96.00	2487.0
103.80	186.0
105.90	259.0
115.90	179.0
116.90	242.0
117.80	164.0
118.90	300.0
127.70	142.0
129.90	126.0
134.90	122.0
140.90	440.0
142.90	607.0
145.00	279.0
147.80	108.0
155.00	117.0
172.00	528.0
172.80	381.0
174.00	30888.0
175.00	2235.0
176.00	30744.0
177.00	1929.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095