
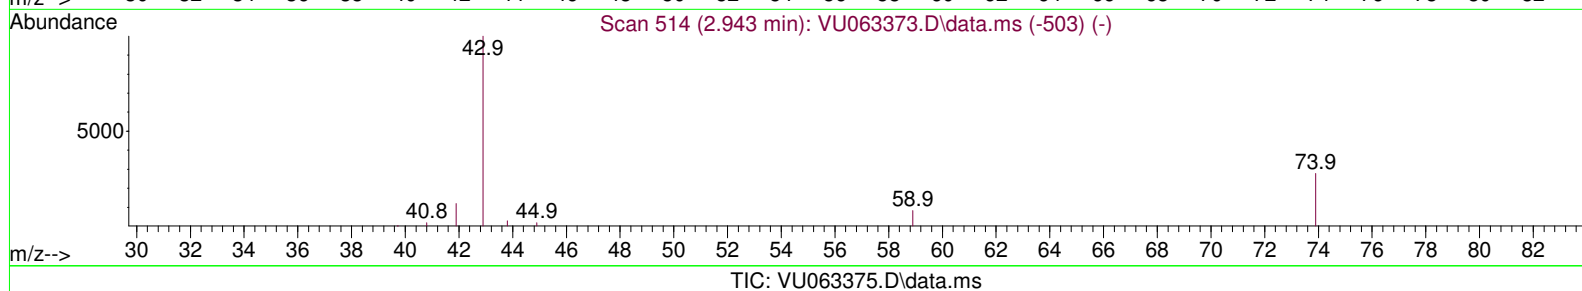
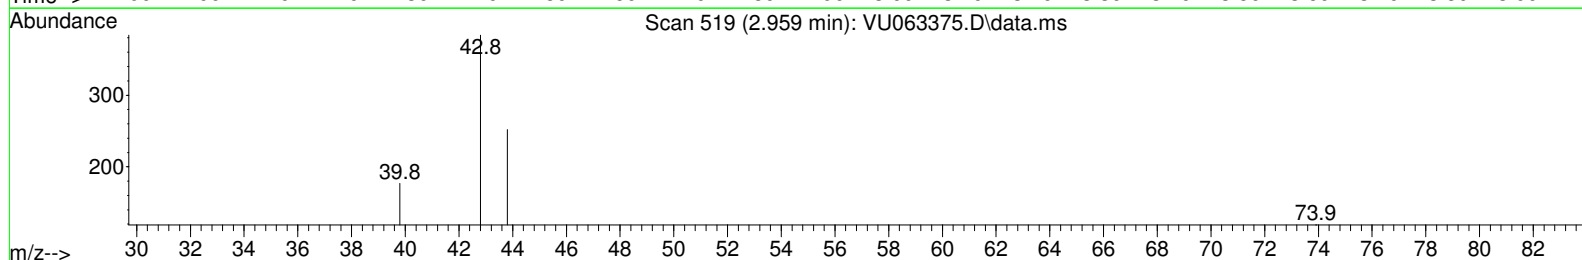


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061025\
Data File : VU063375.D
Acq On : 10 Jun 2025 11:16
Operator : MD/SY
Sample : Q2117-02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 10 11:40:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

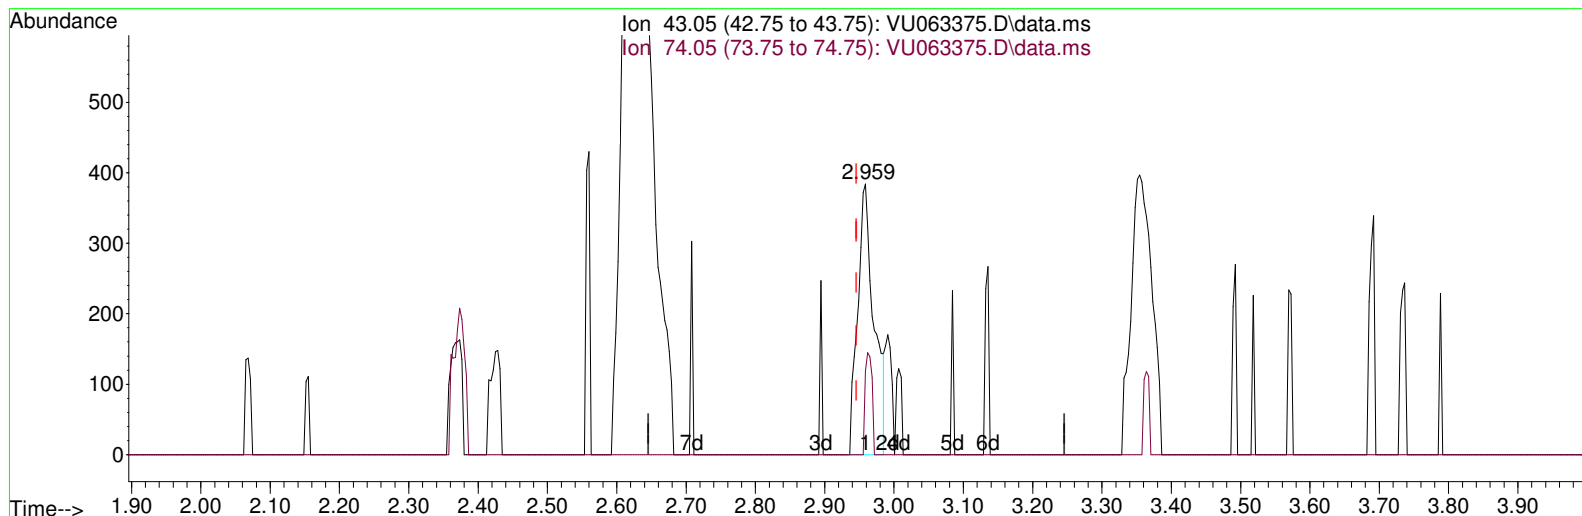

(15) Methyl Acetate (T)




2.959min (+ 0.013) 0.17 ug/L

response 626

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	24.40	15.81#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061025\
Data File : VU063375.D
Acq On : 10 Jun 2025 11:16
Operator : MD/SY
Sample : Q2117-02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 10 11:40:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

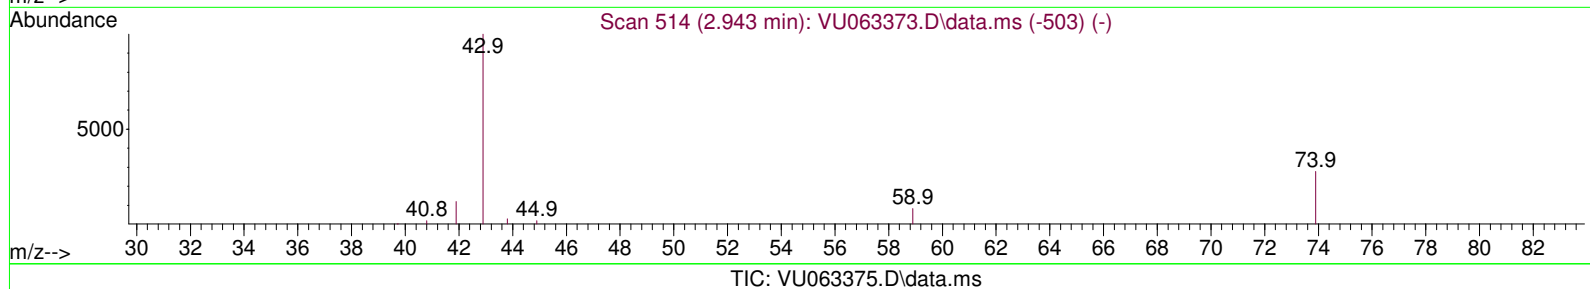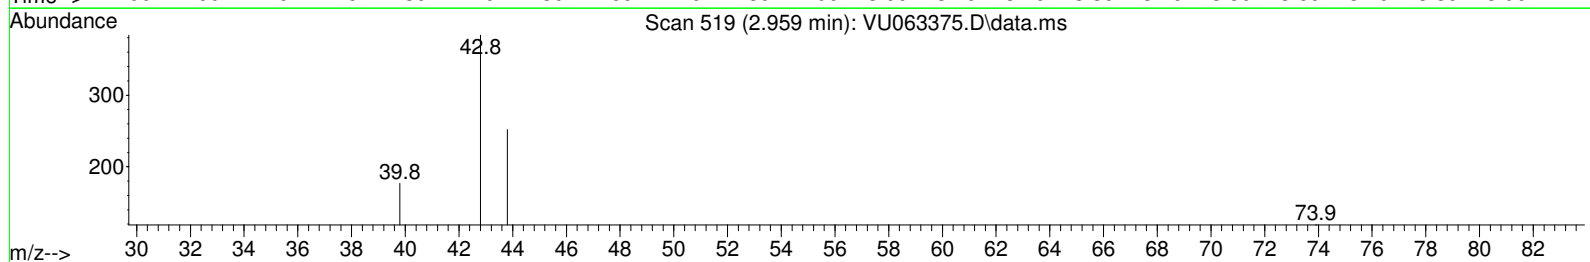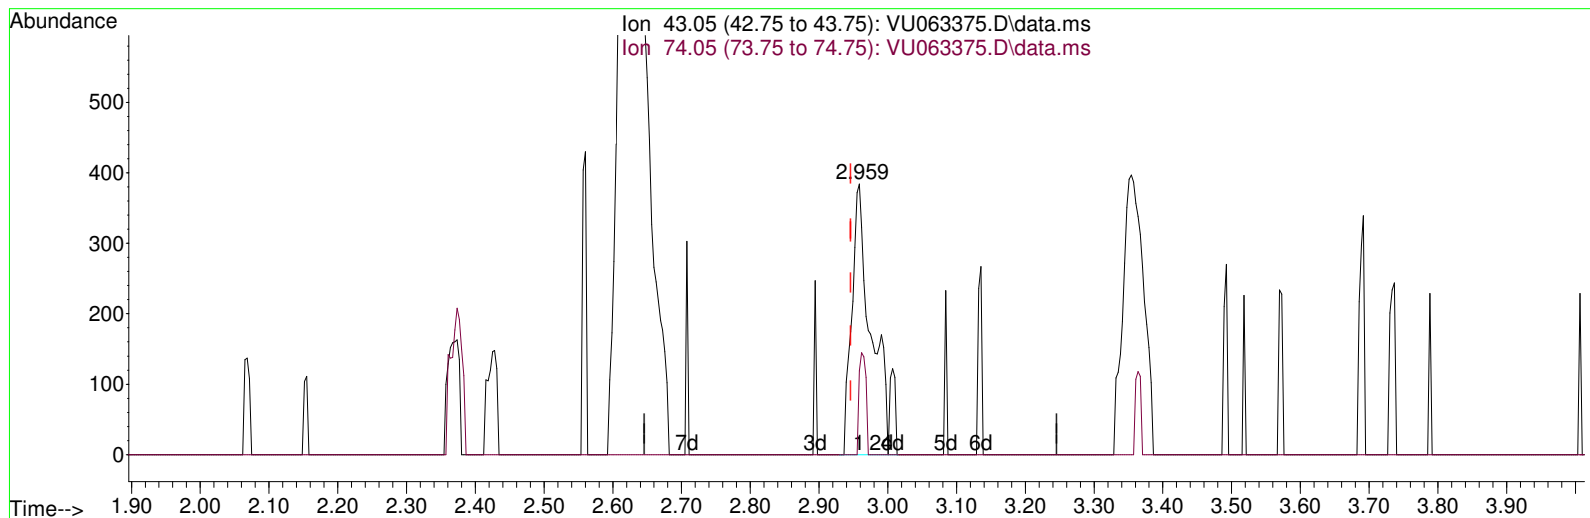

(15) Methyl Acetate (T)




2.959min (+ 0.013) 0.22 ug/L m

response 803

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	24.40	12.33#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061025\
Data File : VU063375.D
Acq On : 10 Jun 2025 11:16
Operator : MD/SY
Sample : Q2117-02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 10 11:40:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

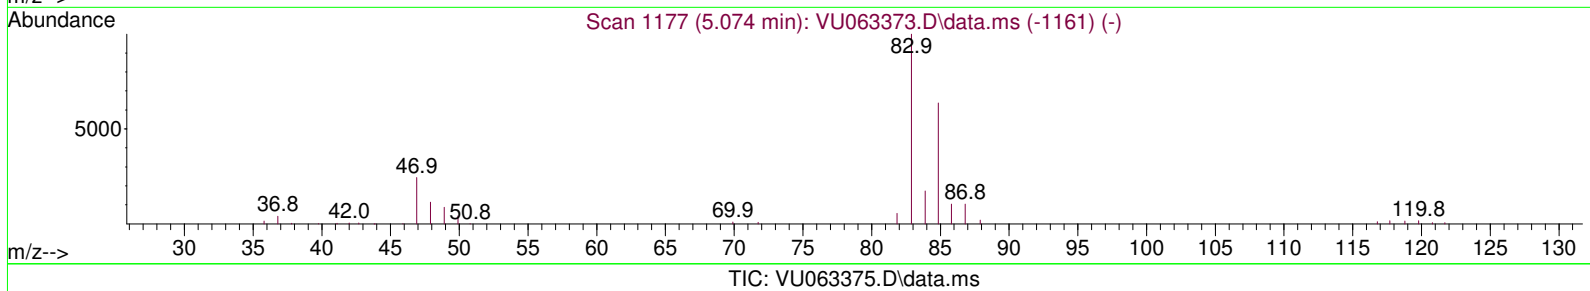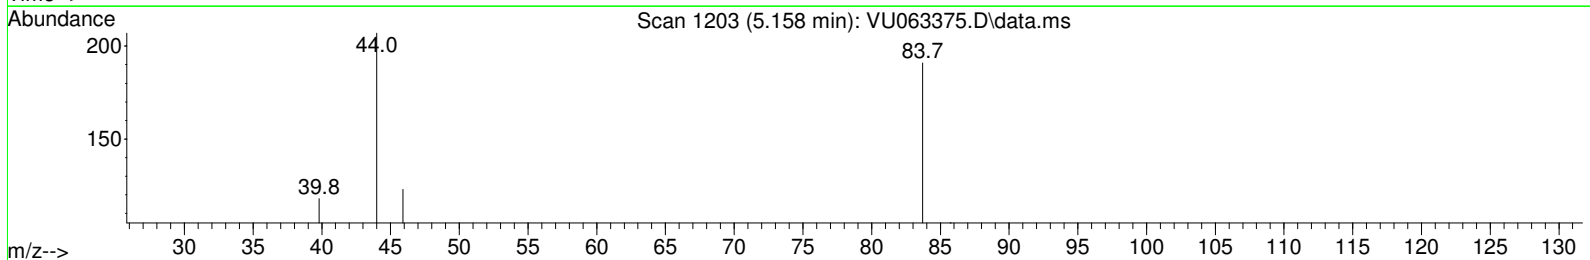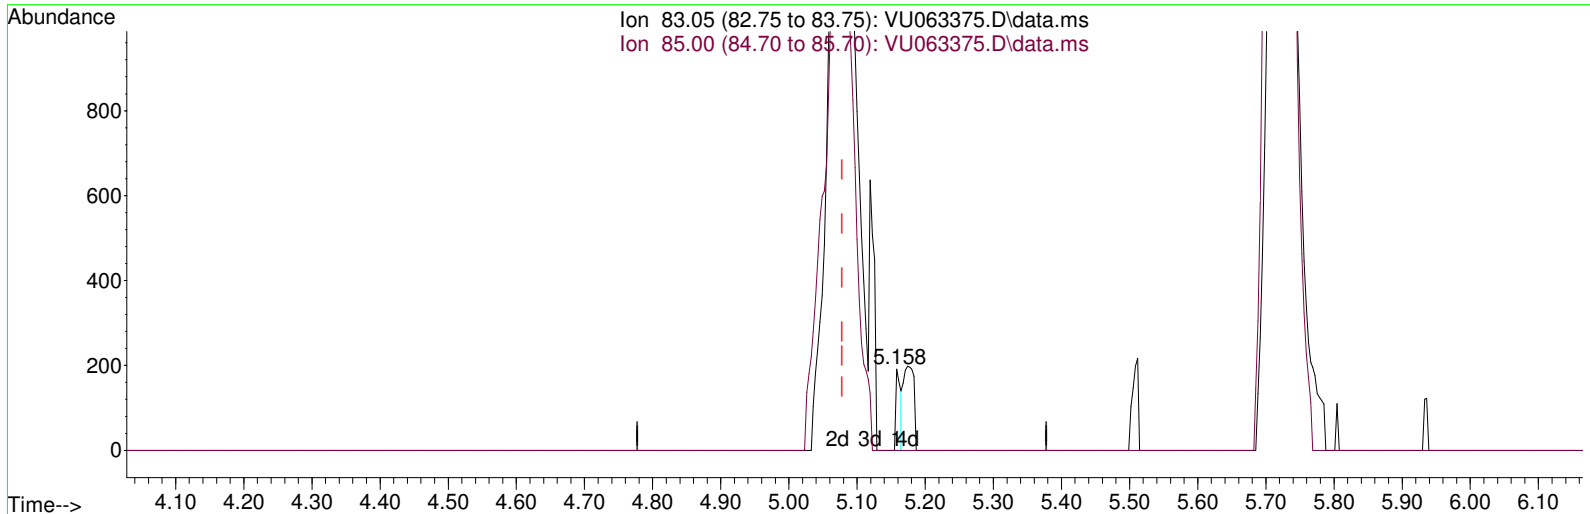

(25) Chloroform (T)




5.158min (+ 0.080) 0.01 ug/L

response 96

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	65.20	54.97
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061025\
Data File : VU063375.D
Acq On : 10 Jun 2025 11:16
Operator : MD/SY
Sample : Q2117-02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 10 11:40:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

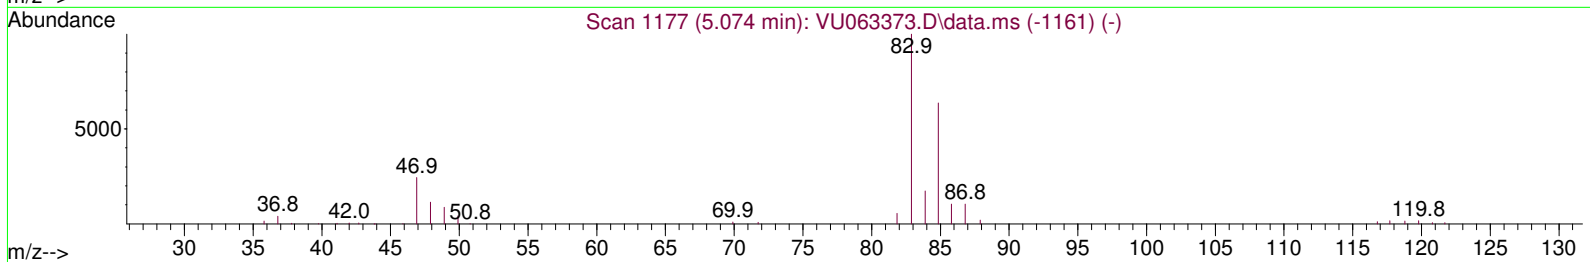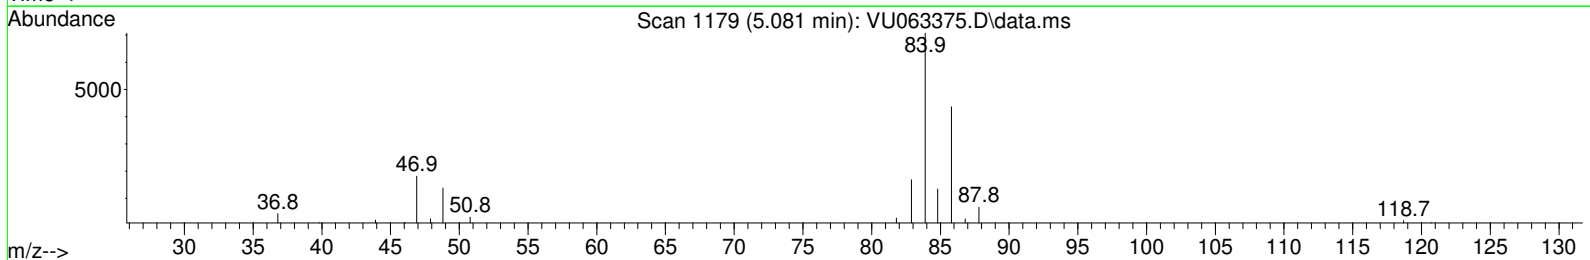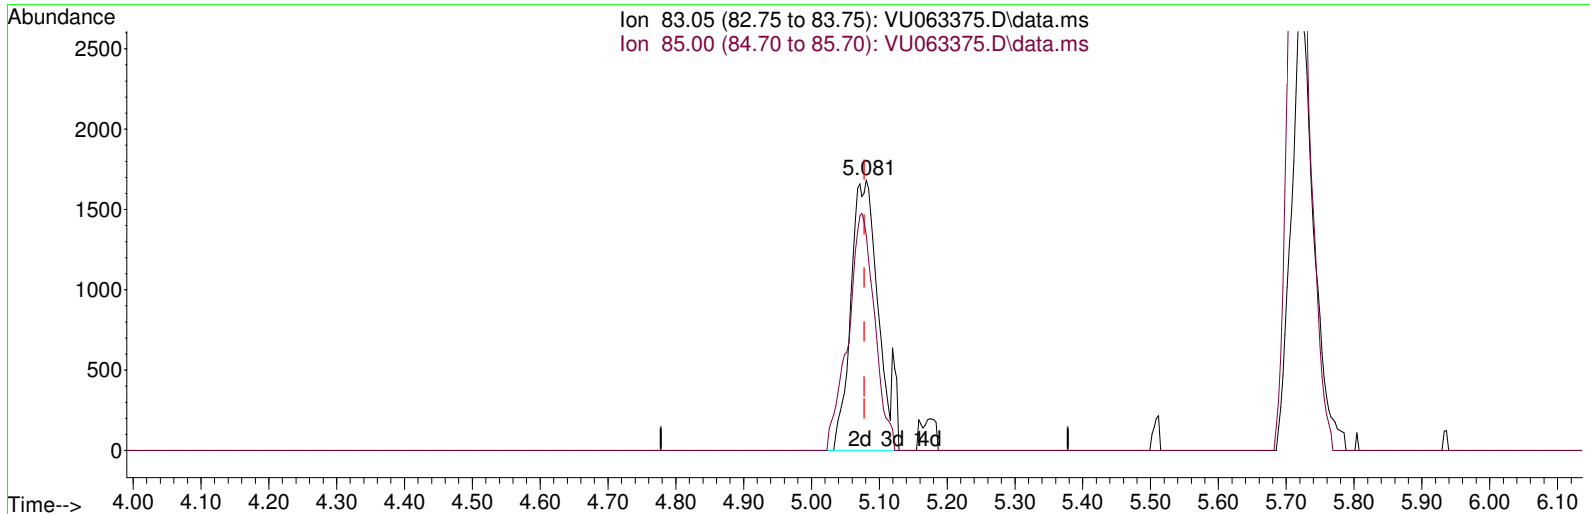

TIC: VU063375.D\data.ms

(25) Chloroform (T)




5.081min (+ 0.003) 0.30 ug/L m

response 4836

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	65.20	79.56
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061025\
Data File : VU063375.D
Acq On : 10 Jun 2025 11:16
Operator : MD/SY
Sample : Q2117-02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 10 11:40:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

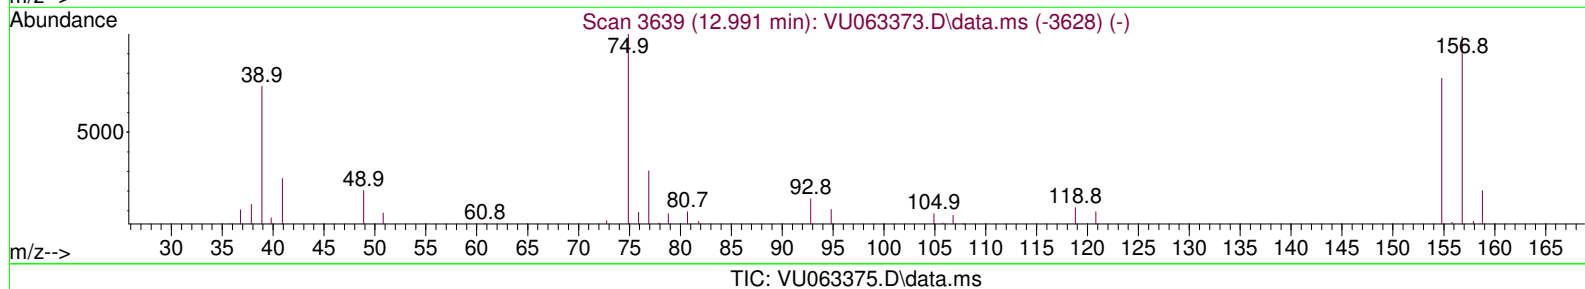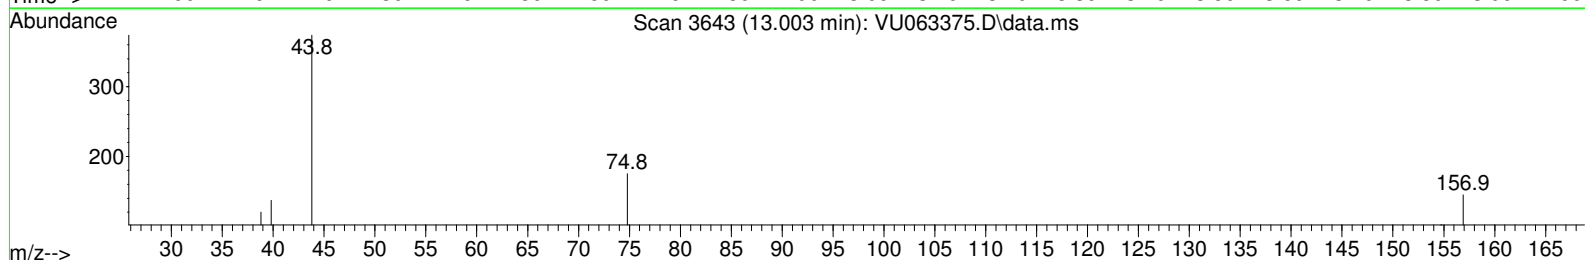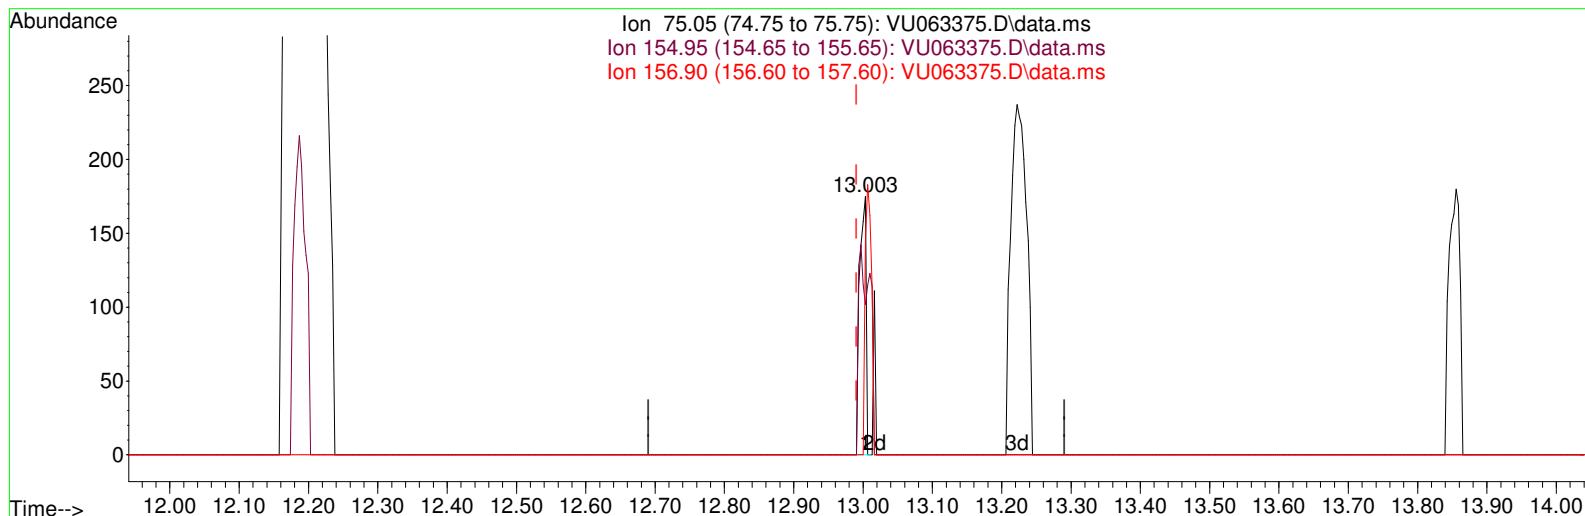

(68) 1,2-Dibromo-3-chloropropane (T)




13.003min (+ 0.013) 0.11 ug/L

response 114

Ion	Exp%	Act%
75.05	100.00	100.00
154.95	77.00	58.29#
156.90	96.70	82.86
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061025\
Data File : VU063375.D
Acq On : 10 Jun 2025 11:16
Operator : MD/SY
Sample : Q2117-02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 10 11:40:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

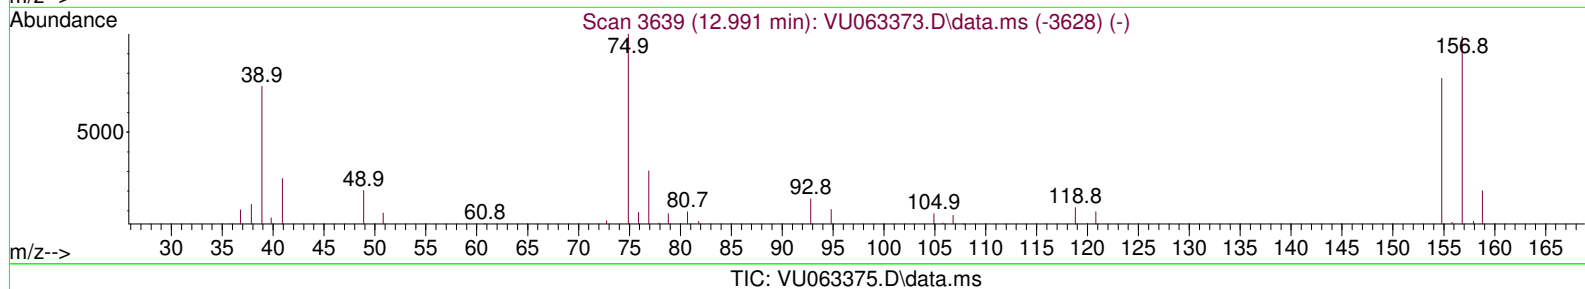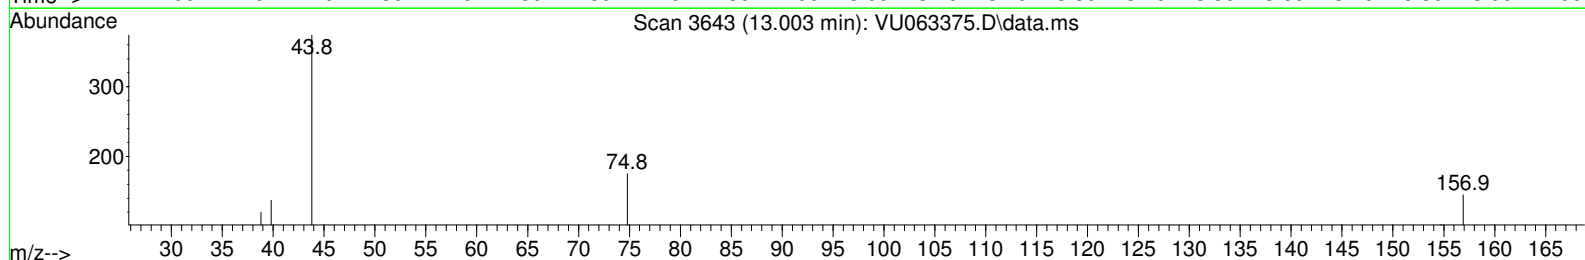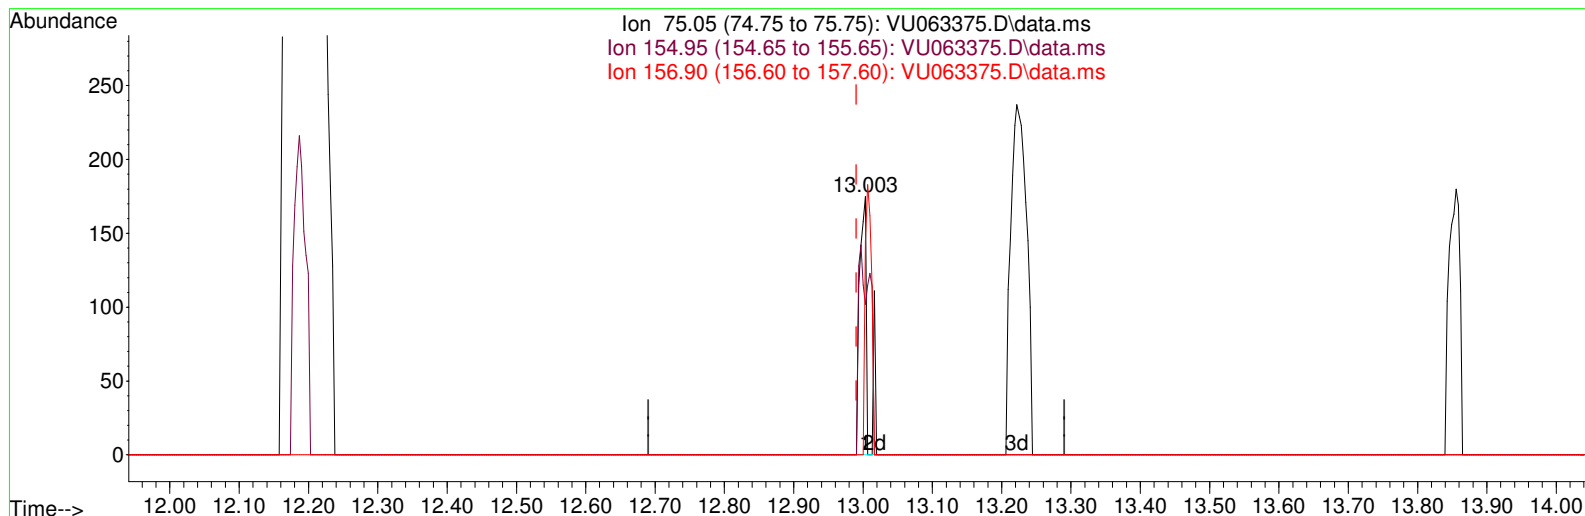

(68) 1,2-Dibromo-3-chloropropane (T)

13.003min (+ 0.013) 0.13 ug/L m

response 135

Ion	Exp%	Act%
75.05	100.00	100.00
154.95	77.00	58.29#
156.90	96.70	82.86
0.00	0.00	0.00