
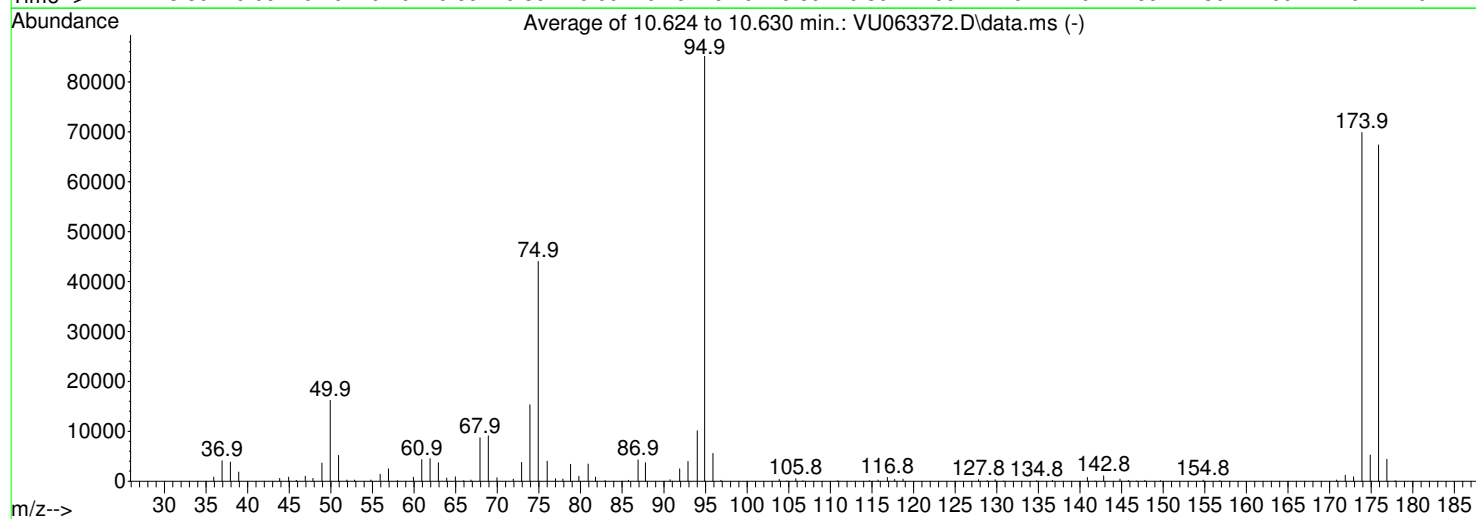


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061025\
Data File : VU063372.D
Acq On : 10 Jun 2025 08:59
Operator : MD/SY
Sample : BFB083
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB083

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Title : VOC Analysis
Last Update : Wed Jun 11 12:25:16 2025

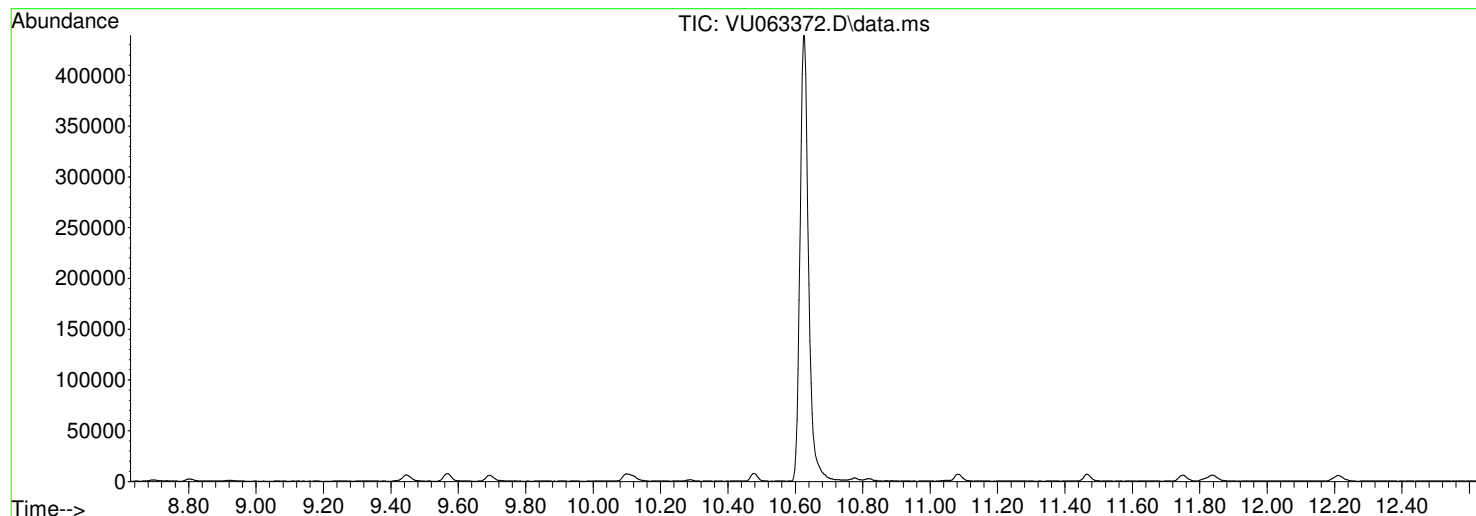

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	16161	PASS
75	95	30	80	51.7	43992	PASS
95	95	100	100	100.0	85107	PASS
96	95	5	9	6.5	5532	PASS
173	174	0.00	2	1.2	872	PASS
174	95	50	120	82.1	69835	PASS
175	174	5	9	7.5	5233	PASS
176	174	95	101	96.4	67320	PASS
177	176	5	9	6.5	4379	PASS

m/z	Abundance
39.90	198.0
43.80	224.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
35.90	813.0
36.90	4351.0
37.90	4033.0
38.90	1828.0
39.80	172.0
43.90	779.0
44.90	827.0
45.90	153.0
46.90	1010.0
47.90	576.0
48.90	3766.0
49.90	16904.0
50.90	5521.0
51.90	278.0
52.90	195.0
54.80	226.0
55.90	1491.0
56.90	2579.0
58.00	109.0
59.90	805.0
60.90	4561.0
61.90	4661.0
62.90	3942.0
63.90	681.0
64.90	915.0
66.00	117.0
66.80	237.0
67.90	9189.0
68.90	9461.0
69.90	718.0
71.90	441.0
72.90	3958.0
73.90	16052.0
74.90	45864.0
76.00	4249.0
77.00	504.0
77.90	386.0
78.80	3391.0
79.80	1044.0
80.90	3615.0
81.80	827.0
82.90	136.0
85.70	191.0
86.90	4234.0
87.80	3755.0
90.80	330.0
91.90	2482.0
92.90	4119.0
94.00	10334.0
94.90	87352.0
95.90	5729.0
96.90	117.0
103.80	377.0
104.80	165.0
105.80	535.0
106.70	140.0
110.90	105.0
115.70	239.0
116.80	704.0
117.70	319.0
118.80	479.0
127.80	343.0
128.80	132.0
129.80	281.0
130.80	137.0
134.80	122.0
136.70	136.0
140.90	803.0
141.80	108.0
142.80	1129.0
144.80	443.0
145.70	188.0
147.80	156.0
154.80	239.0
156.80	143.0
170.80	233.0
171.90	1181.0
172.90	882.0
173.90	71120.0
174.90	5282.0
175.90	68376.0
176.90	4638.0
177.90	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
35.90	826.0
36.90	4191.0
37.90	3920.0
38.90	1946.0
39.80	178.0
43.90	769.0
44.90	860.0
45.80	182.0
46.90	986.0
47.80	579.0
48.90	3710.0
49.90	16496.0
50.90	5242.0
51.90	270.0
52.90	216.0
54.80	209.0
55.90	1377.0
56.90	2522.0
58.00	119.0
59.90	833.0
60.90	4423.0
61.90	4643.0
62.90	3788.0
63.90	629.0
64.90	825.0
65.90	113.0
66.90	253.0
67.90	8954.0
68.90	9355.0
70.00	686.0
71.90	422.0
72.90	3835.0
73.90	15774.0
74.90	45368.0
76.00	4167.0
77.00	528.0
77.80	431.0
78.80	3479.0
79.80	1040.0
80.90	3520.0
81.80	800.0
83.00	128.0
85.80	176.0
86.90	4433.0
87.80	3801.0
90.80	335.0
91.90	2488.0
92.90	4121.0
94.00	10387.0
94.90	87904.0
95.90	5682.0
96.80	146.0
103.80	362.0
105.80	521.0
106.70	135.0
110.90	110.0
114.70	116.0
115.80	239.0
116.80	725.0
117.80	362.0
118.80	441.0
127.80	325.0
128.90	115.0
129.80	324.0
134.80	122.0
136.70	156.0
140.90	761.0
142.80	1072.0
144.80	397.0
145.80	138.0
146.80	104.0
147.80	199.0
149.70	103.0
154.80	237.0
156.80	101.0
170.80	212.0
171.90	1246.0
172.90	892.0
173.90	71528.0
174.90	5385.0
175.90	69592.0
176.90	4489.0
177.90	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
35.90	703.0
36.90	3649.0
37.90	3486.0
38.90	1791.0
39.80	199.0
43.90	744.0
44.90	781.0
45.80	179.0
46.90	949.0
47.80	559.0
48.90	3445.0
49.90	15083.0
50.90	4704.0
51.90	225.0
52.80	189.0
54.80	198.0
55.90	1211.0
56.90	2358.0
58.00	119.0
59.90	756.0
60.90	3943.0
61.90	4246.0
62.90	3349.0
63.90	559.0
65.00	776.0
65.90	104.0
66.90	239.0
67.90	7882.0
68.90	8480.0
70.00	616.0
71.90	395.0
72.90	3474.0
73.90	14060.0
74.90	40744.0
76.00	3689.0
77.00	478.0
77.80	380.0
78.80	3298.0
79.80	940.0
80.90	3175.0
81.80	753.0
85.80	176.0
86.90	4231.0
87.80	3447.0
90.70	304.0
91.90	2361.0
92.90	3698.0
94.00	9622.0
94.90	80064.0
95.90	5185.0
96.80	173.0
103.90	352.0
105.90	421.0
114.70	148.0
115.80	269.0
116.90	699.0
117.70	353.0
118.70	426.0
127.80	267.0
128.90	106.0
129.80	296.0
134.80	115.0
136.70	168.0
140.90	643.0
142.90	965.0
144.80	364.0
145.90	108.0
147.80	199.0
149.70	114.0
154.80	220.0
170.90	165.0
171.90	1193.0
172.90	843.0
173.90	66856.0
174.90	5032.0
175.90	63992.0
176.90	4009.0
177.90	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083