

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061119\
 Data File : VU032621.D
 Acq On : 11 Jun 2019 19:38
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	33	rBV	3883	3144	0.50%	0.063%
2	1.396	88	95	105	rBV	86095	89532	14.20%	1.785%
3	1.675	175	182	196	rVB	68863	85632	13.58%	1.707%
4	2.267	356	366	380	rVB	147761	222827	35.33%	4.443%
5	2.479	427	432	435	rBV2	264	240	0.04%	0.005%
6	2.698	495	500	502	rBV3	213	217	0.03%	0.004%
7	2.830	531	541	558	rBV2	3703	8190	1.30%	0.163%
8	3.026	597	602	604	rBV	155	149	0.02%	0.003%
9	3.068	609	615	618	rBV2	221	237	0.04%	0.005%
10	3.572	766	772	775	rBV	239	221	0.04%	0.004%
11	3.608	775	783	789	rVV2	222	333	0.05%	0.007%
12	3.814	843	847	849	rBV2	223	169	0.03%	0.003%
13	3.846	854	857	861	rVB2	208	184	0.03%	0.004%
14	3.881	861	868	870	rBV2	166	207	0.03%	0.004%
15	3.952	885	890	895	rBV	279	314	0.05%	0.006%
16	4.097	931	935	941	rBV2	346	467	0.07%	0.009%
17	4.170	946	958	985	rBV	60760	162825	25.82%	3.247%
18	4.563	1077	1080	1085	rVB3	223	231	0.04%	0.005%
19	4.640	1088	1104	1127	rBV2	105255	247301	39.21%	4.931%
20	4.736	1132	1134	1137	rVB2	413	215	0.03%	0.004%
21	4.823	1158	1161	1166	rVB3	315	241	0.04%	0.005%
22	4.875	1174	1177	1179	rBV2	218	156	0.02%	0.003%
23	4.945	1195	1199	1204	rBV2	267	269	0.04%	0.005%
24	4.971	1204	1207	1210	rBV	223	170	0.03%	0.003%
25	5.151	1260	1263	1267	rBV2	195	152	0.02%	0.003%
26	5.212	1279	1282	1287	rVB2	194	165	0.03%	0.003%
27	5.251	1289	1294	1297	rBV2	115	137	0.02%	0.003%
28	5.334	1297	1320	1346	rBV2	216410	630643	100.00%	12.574%
29	5.714	1434	1438	1443	rVV2	227	243	0.04%	0.005%
30	5.765	1452	1454	1461	rVB2	233	155	0.02%	0.003%
31	5.881	1476	1490	1516	rBV	200122	390626	61.94%	7.789%
32	6.135	1565	1569	1573	rVB3	176	177	0.03%	0.004%
33	6.174	1573	1581	1601	rBV6	4664	9939	1.58%	0.198%
34	6.325	1614	1628	1653	rBV	139457	280231	44.44%	5.588%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061119\
 Data File : VU032621.D
 Acq On : 11 Jun 2019 19:38
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

35	6.614	1715	1718	1721	rBV	200	173	0.03%	0.003%
36	6.714	1747	1749	1754	rVB2	209	163	0.03%	0.003%
37	6.739	1754	1757	1760	rVB2	208	148	0.02%	0.003%
38	6.759	1760	1763	1766	rBV2	208	174	0.03%	0.003%
39	6.813	1776	1780	1782	rBV2	182	144	0.02%	0.003%
40	6.871	1793	1798	1801	rBV2	256	194	0.03%	0.004%
41	6.903	1801	1808	1812	rVV2	142	166	0.03%	0.003%
42	6.984	1825	1833	1836	rBV	277	306	0.05%	0.006%
43	7.064	1856	1858	1863	rVB2	224	175	0.03%	0.003%
44	7.090	1863	1866	1871	rBV2	207	142	0.02%	0.003%
45	7.225	1897	1908	1948	rBV	77310	144868	22.97%	2.889%
46	7.360	1948	1950	1957	rVB2	444	390	0.06%	0.008%
47	7.392	1957	1960	1966	rBV2	399	424	0.07%	0.008%
48	7.460	1978	1981	1986	rVB2	305	223	0.04%	0.004%
49	7.492	1986	1991	1994	rBV2	151	179	0.03%	0.004%
50	7.559	2000	2012	2031	rBV	288021	501680	79.55%	10.003%
51	7.846	2091	2101	2127	rBV	51542	91590	14.52%	1.826%
52	8.122	2183	2187	2190	rBV2	325	253	0.04%	0.005%
53	8.164	2196	2200	2208	rBV3	404	575	0.09%	0.011%
54	8.254	2224	2228	2230	rBV	189	146	0.02%	0.003%
55	8.309	2234	2245	2288	rBV2	166044	339258	53.80%	6.764%
56	8.582	2325	2330	2333	rBV3	296	302	0.05%	0.006%
57	8.945	2439	2443	2446	rBV2	202	164	0.03%	0.003%
58	8.977	2450	2453	2457	rVB	236	167	0.03%	0.003%
59	9.032	2463	2470	2473	rBV2	158	178	0.03%	0.004%
60	9.083	2474	2486	2518	rBV	294279	495043	78.50%	9.871%
61	9.540	2626	2628	2633	rBV	138	145	0.02%	0.003%
62	9.707	2675	2680	2682	rBV2	233	219	0.03%	0.004%
63	9.800	2706	2709	2712	rVB2	257	175	0.03%	0.003%
64	10.148	2814	2817	2820	rVB	243	156	0.02%	0.003%
65	10.173	2821	2825	2828	rBV2	131	135	0.02%	0.003%
66	10.312	2863	2868	2870	rBV2	236	186	0.03%	0.004%
67	10.350	2875	2880	2882	rBV	350	251	0.04%	0.005%
68	10.427	2891	2904	2923	rBV	198071	323867	51.36%	6.458%
69	10.534	2934	2937	2940	rBV	258	202	0.03%	0.004%
70	10.601	2952	2958	2967	rBV	775	1056	0.17%	0.021%
71	10.691	2981	2986	2989	rBV2	245	228	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061119\
 Data File : VU032621.D
 Acq On : 11 Jun 2019 19:38
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

72	10.852	3033	3036	3038	rBV2	229	153	0.02%	0.003%
73	11.119	3115	3119	3124	rBV2	200	224	0.04%	0.004%
74	11.148	3124	3128	3132	rBV2	149	149	0.02%	0.003%
75	11.479	3220	3231	3252	rBV	298661	485768	77.03%	9.686%
76	11.746	3311	3314	3318	rBV4	211	224	0.04%	0.004%
77	11.855	3334	3348	3374	rBV	287056	482281	76.47%	9.616%
78	12.482	3537	3543	3551	rVB4	541	752	0.12%	0.015%
79	12.559	3564	3567	3569	rBV	219	145	0.02%	0.003%
80	12.665	3596	3600	3604	rBV2	298	279	0.04%	0.006%
81	12.691	3604	3608	3611	rVV2	288	219	0.03%	0.004%
82	12.910	3672	3676	3679	rBV2	171	160	0.03%	0.003%
83	12.929	3680	3682	3688	rVB	182	172	0.03%	0.003%
84	13.041	3714	3717	3719	rBV2	217	134	0.02%	0.003%
85	13.083	3727	3730	3732	rBV	274	153	0.02%	0.003%
86	13.363	3812	3817	3821	rVB2	293	317	0.05%	0.006%
87	13.707	3920	3924	3929	rBV2	351	392	0.06%	0.008%
88	13.733	3929	3932	3936	rVV2	237	181	0.03%	0.004%
89	13.755	3936	3939	3943	rBV2	319	266	0.04%	0.005%
90	13.865	3970	3973	3976	rBV2	200	135	0.02%	0.003%
91	13.900	3981	3984	3986	rBV2	278	177	0.03%	0.004%
92	14.061	4031	4034	4042	rBV3	341	509	0.08%	0.010%
93	14.099	4043	4046	4048	rBV3	262	164	0.03%	0.003%
94	14.115	4048	4051	4057	rVB2	532	430	0.07%	0.009%
95	14.154	4060	4063	4064	rBV2	272	148	0.02%	0.003%
96	14.267	4095	4098	4108	rVB2	574	812	0.13%	0.016%
97	14.321	4112	4115	4118	rVB2	342	230	0.04%	0.005%
98	14.366	4126	4129	4134	rBV2	267	223	0.04%	0.004%
99	14.961	4311	4314	4319	rBV3	345	345	0.05%	0.007%
100	15.276	4409	4412	4417	rBV2	336	354	0.06%	0.007%


Sum of corrected areas: 5015280

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061119\
Data File : VU032621.D
Acq On : 11 Jun 2019 19:38
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

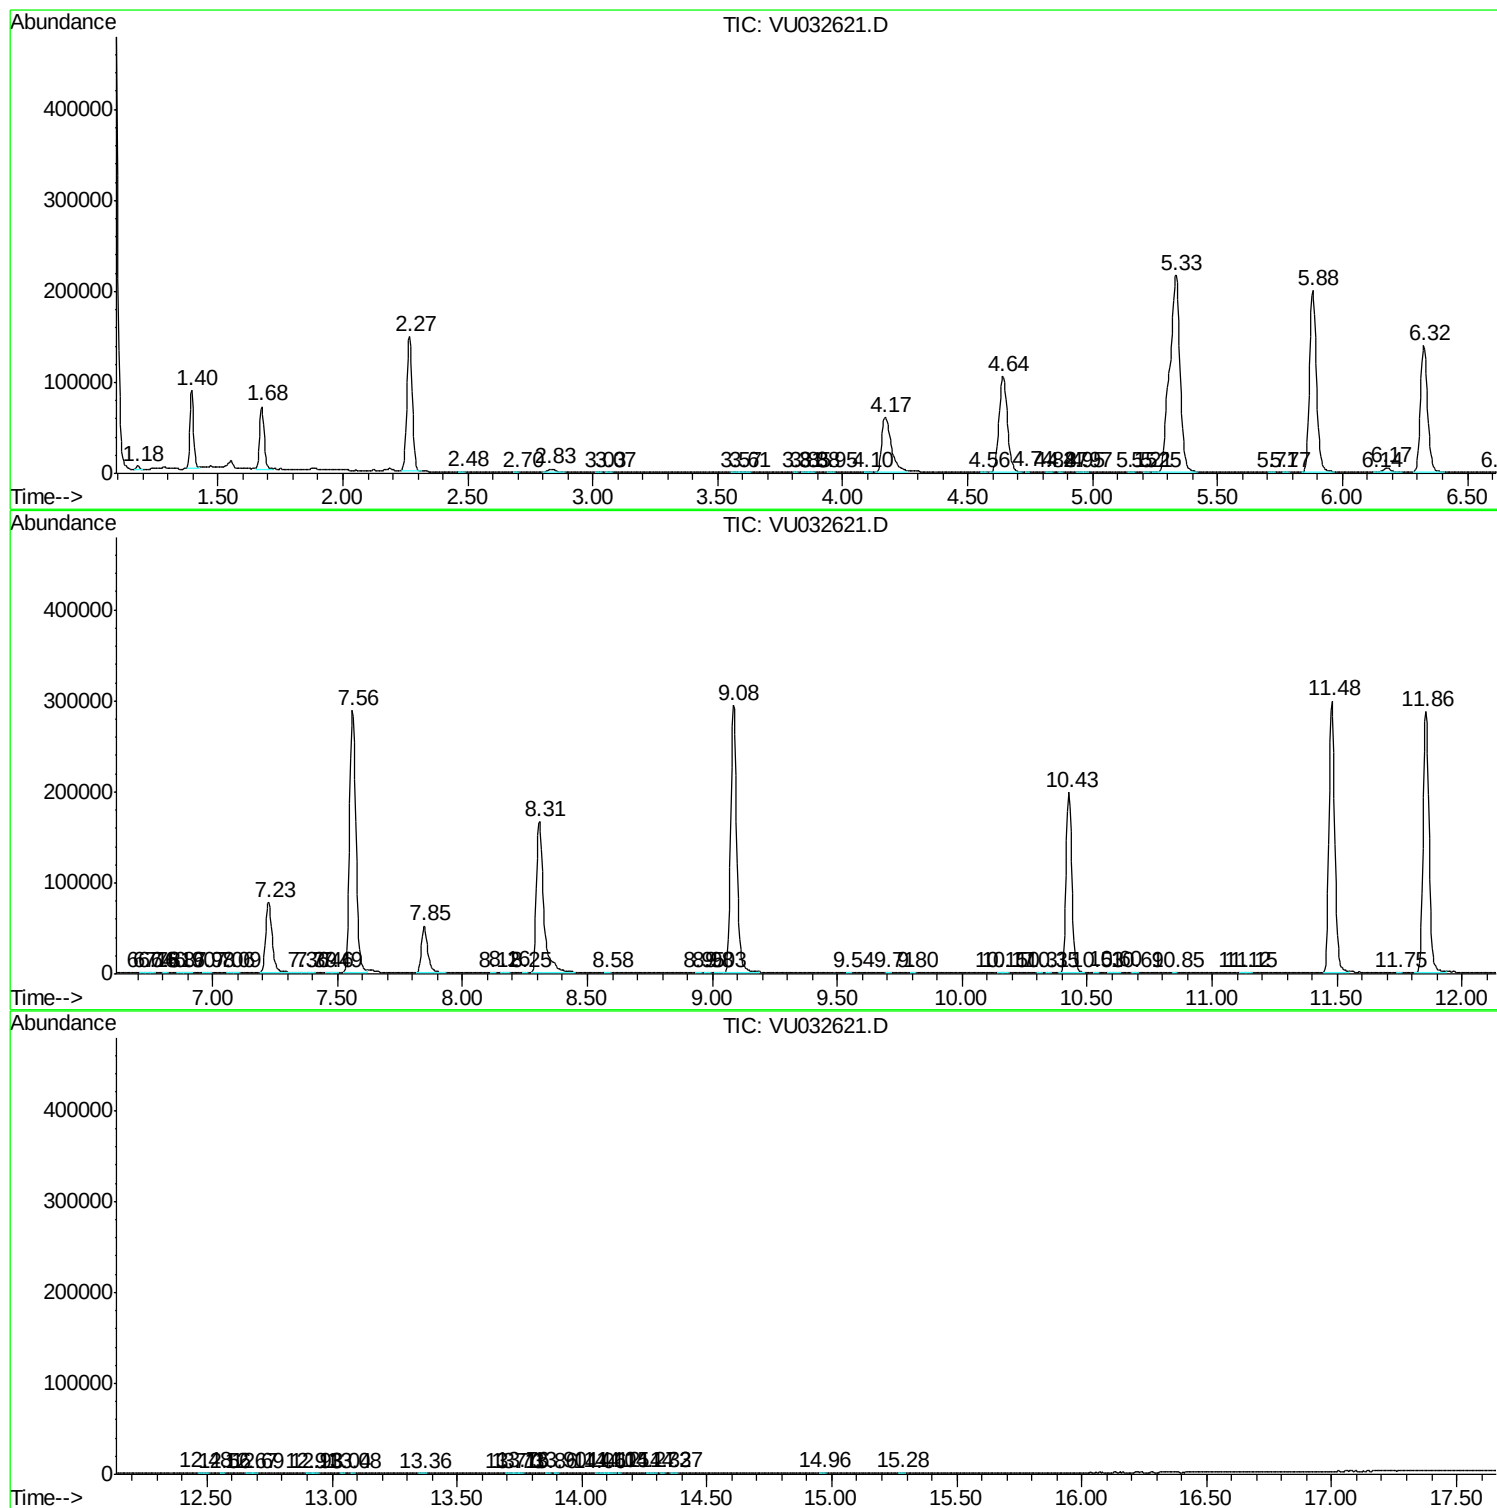

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061119\
Data File : VU032621.D
Acq On : 11 Jun 2019 19:38
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061119\
Data File : VU032621.D
Acq On : 11 Jun 2019 19:38
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc