


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061119\
 Data File : VU032594.D
 Acq On : 11 Jun 2019 08:57
 Operator : JC/SP
 Sample : BFB53
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB53

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis
 Last Update : Wed Jun 12 07:28:55 2019

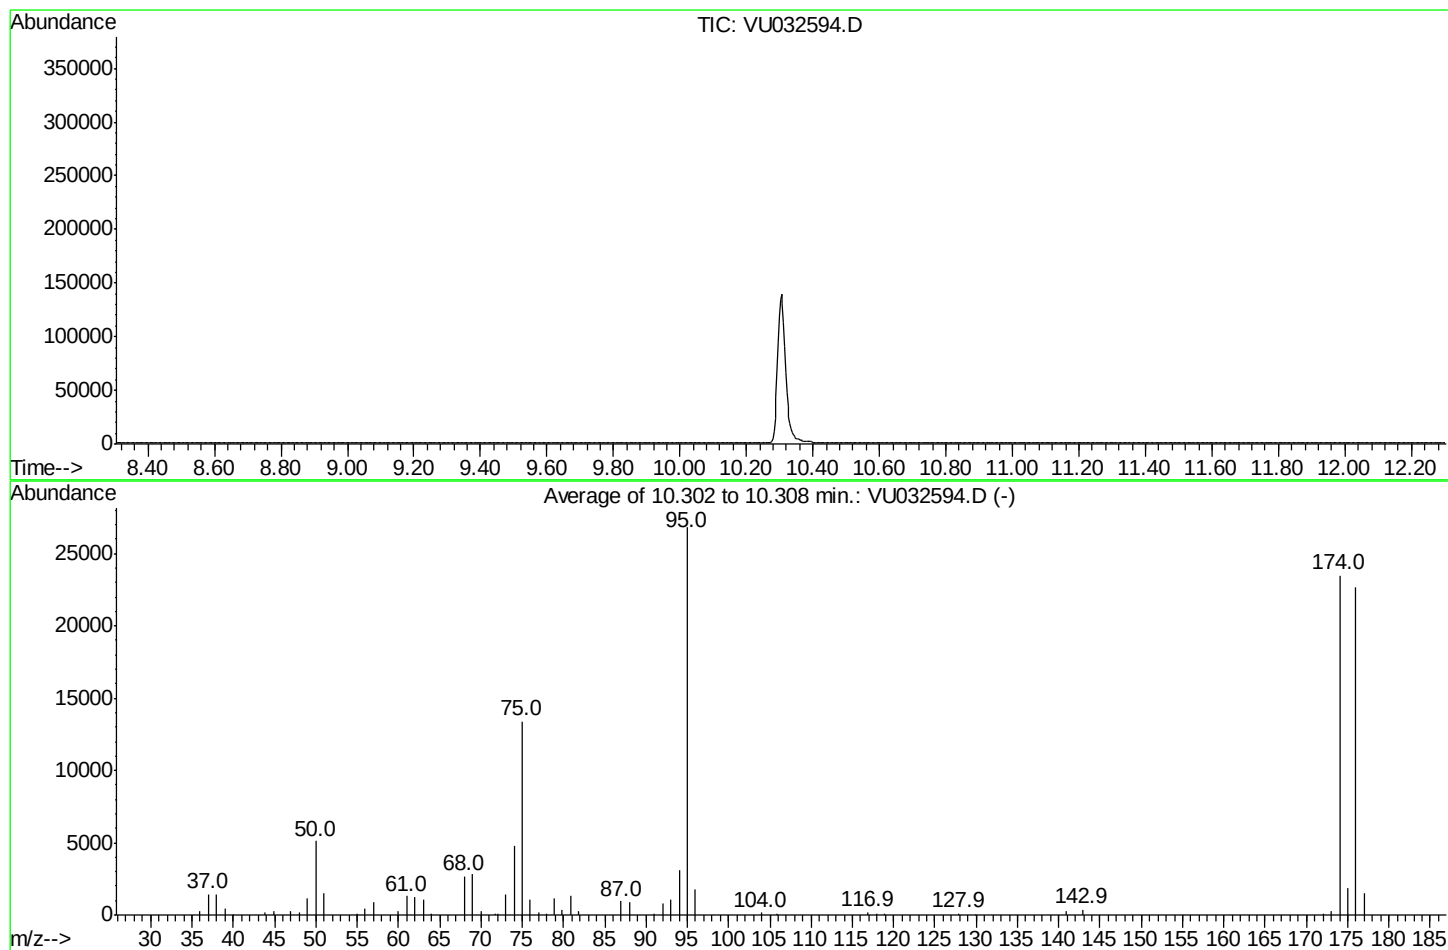

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	5103	PASS
75	95	30	80	50.0	13401	PASS
95	95	100	100	100.0	26816	PASS
96	95	5	9	6.7	1799	PASS
173	174	0.00	2	1.0	246	PASS
174	95	50	120	87.7	23509	PASS
175	174	5	9	8.0	1892	PASS
176	174	95	101	96.5	22680	PASS
177	176	5	9	6.5	1479	PASS

Scan 2854 (10.267 min): VU032594.D
BFB53

m/z	Abundance
39.90	618.0
44.00	357.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
35.00	247.0
37.00	1428.0
38.00	1394.0
39.00	453.0
39.00	661.0
43.00	496.0
44.00	244.0
46.00	229.0
48.10	190.0
49.00	1142.0
50.00	5292.0
51.00	1585.0
55.00	106.0
56.00	439.0
57.00	887.0
59.00	245.0
61.00	1322.0
62.00	1337.0
63.00	1058.0
64.00	146.0
68.00	2705.0
69.00	2826.0
70.00	321.0
71.80	147.0
73.00	1314.0
74.00	4962.0
75.00	13561.0
76.00	1122.0
77.00	219.0
78.00	114.0
78.90	1139.0
79.80	318.0
80.90	1341.0
81.90	295.0
87.00	1042.0
88.00	872.0
90.90	122.0
92.00	855.0
93.00	1143.0
94.00	3195.0
95.00	26912.0
96.00	1772.0
103.90	164.0
105.90	119.0
116.90	209.0
117.90	108.0
118.90	125.0
129.90	104.0
140.90	287.0
142.90	354.0
173.00	285.0
174.00	22768.0
175.00	1810.0
176.00	22424.0
177.00	1463.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
35.00	272.0
37.00	1488.0
38.00	1453.0
39.00	468.0
39.00	649.0
43.00	539.0
44.00	240.0
46.00	280.0
48.00	173.0
49.00	1171.0
50.00	5269.0
51.00	1557.0
55.00	103.0
56.00	447.0
57.00	872.0
60.00	262.0
61.00	1334.0
62.00	1285.0
63.00	1086.0
64.00	140.0
68.00	2740.0
69.00	2867.0
70.00	293.0
71.00	169.0
73.00	1446.0
74.00	5002.0
75.00	13758.0
76.00	1152.0
77.00	225.0
78.00	100.0
78.00	1157.0
79.00	327.0
80.00	1339.0
81.00	306.0
87.00	972.0
88.00	982.0
90.00	126.0
92.00	847.0
93.00	1130.0
94.00	3245.0
95.00	27656.0
96.00	1860.0
104.00	165.0
105.00	118.0
116.00	183.0
117.00	105.0
118.00	127.0
127.00	131.0
140.00	307.0
142.00	412.0
172.00	125.0
173.00	232.0
174.00	24208.0
175.00	1956.0
176.00	23424.0
177.00	1538.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
35.00	258.0
37.00	1386.0
38.00	1321.0
39.00	464.0
39.00	625.0
43.00	577.0
44.00	233.0
47.00	275.0
47.00	151.0
49.00	1083.0
50.00	4749.0
51.00	1494.0
55.00	487.0
57.00	795.0
60.00	264.0
61.00	1233.0
62.00	1185.0
63.00	1024.0
64.00	109.0
68.00	2623.0
69.00	2725.0
70.00	222.0
72.00	170.0
73.00	1379.0
74.00	4512.0
75.00	12885.0
76.00	1039.0
77.00	178.0
78.00	1160.0
79.00	307.0
80.00	1232.0
81.00	278.0
87.00	905.0
88.00	910.0
90.00	133.0
92.00	750.0
93.00	990.0
94.00	2984.0
95.00	25880.0
96.00	1767.0
104.00	170.0
105.00	134.0
116.00	147.0
117.00	107.0
118.00	129.0
127.00	141.0
140.00	314.0
142.00	429.0
172.00	122.0
173.00	221.0
174.00	23552.0
175.00	1911.0
176.00	22192.0
176.00	1436.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53