

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061120\
 Data File : VU038779.D
 Acq On : 10 Jun 2020 16:30
 Operator : SY/MD
 Sample : VU0611WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	98	rBV	177885	199802	11.43%	1.406%
2	1.932	176	184	196	rVB	151686	197458	11.29%	1.389%
3	2.594	377	390	413	rBV	354085	609709	34.86%	4.290%
4	2.912	487	489	491	rBV	302	130	0.01%	0.001%
5	2.954	500	502	504	rBV2	443	225	0.01%	0.002%
6	3.134	553	558	559	rBV	440	365	0.02%	0.003%
7	3.176	568	571	572	rBV	466	265	0.02%	0.002%
8	3.224	572	586	600	rVV	7581	16821	0.96%	0.118%
9	3.288	603	606	610	rVB	205	133	0.01%	0.001%
10	3.311	610	613	615	rBV	264	172	0.01%	0.001%
11	3.420	645	647	649	rBV2	294	104	0.01%	0.001%
12	3.433	649	651	654	rBV2	403	265	0.02%	0.002%
13	3.523	678	679	682	rBV2	263	164	0.01%	0.001%
14	3.578	693	696	698	rBV	169	93	0.01%	0.001%
15	3.613	704	707	709	rBV2	458	285	0.02%	0.002%
16	3.661	720	722	723	rBV	154	69	0.00%	0.000%
17	3.703	733	735	736	rBV	219	64	0.00%	0.000%
18	3.748	748	749	750	rBV	216	43	0.00%	0.000%
19	3.761	750	753	762	rVB2	383	633	0.04%	0.004%
20	3.806	762	767	772	rBV2	307	431	0.02%	0.003%
21	3.861	781	784	785	rBV2	215	131	0.01%	0.001%
22	3.996	823	826	827	rBV2	192	100	0.01%	0.001%
23	4.034	836	838	841	rBV2	163	92	0.01%	0.001%
24	4.121	863	865	867	rBV	145	91	0.01%	0.001%
25	4.350	935	936	937	rBV	155	31	0.00%	0.000%
26	4.391	947	949	951	rBV	227	102	0.01%	0.001%
27	4.427	956	960	963	rBV2	126	101	0.01%	0.001%
28	4.497	976	982	987	rVB2	262	330	0.02%	0.002%
29	4.591	1008	1011	1014	rBV	534	299	0.02%	0.002%
30	4.668	1019	1035	1065	rBV2	202660	517656	29.60%	3.642%
31	5.002	1137	1139	1140	rBV	196	87	0.00%	0.001%
32	5.102	1153	1170	1189	rBV	323416	701392	40.11%	4.935%
33	5.237	1209	1212	1215	rBV3	251	213	0.01%	0.001%
34	5.269	1219	1222	1224	rBV	213	110	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061120\
 Data File : VU038779.D
 Acq On : 10 Jun 2020 16:30
 Operator : SY/MD
 Sample : VU0611WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

35	5.324	1230	1239	1241	rBV2	1542	1903	0.11%	0.013%
36	5.407	1261	1265	1277	rVB7	832	1221	0.07%	0.009%
37	5.478	1285	1287	1290	rBV	251	135	0.01%	0.001%
38	5.517	1293	1299	1301	rBV2	281	269	0.02%	0.002%
39	5.533	1301	1304	1308	rBV	307	215	0.01%	0.002%
40	5.607	1321	1327	1330	rBV2	237	270	0.02%	0.002%
41	5.684	1347	1351	1352	rBV	149	104	0.01%	0.001%
42	5.761	1352	1375	1408	rBV2	640531	1748779	100.00%	12.303%
43	6.070	1467	1471	1473	rBV3	731	558	0.03%	0.004%
44	6.137	1489	1492	1494	rBV2	467	276	0.02%	0.002%
45	6.179	1502	1505	1506	rBV2	260	141	0.01%	0.001%
46	6.205	1510	1513	1516	rBV2	199	170	0.01%	0.001%
47	6.282	1521	1537	1562	rBV	591259	1154021	65.99%	8.119%
48	6.468	1593	1595	1597	rVB2	464	186	0.01%	0.001%
49	6.517	1606	1610	1612	rBV2	501	326	0.02%	0.002%
50	6.568	1613	1626	1644	rBV5	8584	26799	1.53%	0.189%
51	6.722	1660	1674	1700	rVB	399474	771100	44.09%	5.425%
52	6.829	1704	1707	1708	rBV2	731	390	0.02%	0.003%
53	6.944	1740	1743	1746	rBV2	556	285	0.02%	0.002%
54	6.996	1758	1759	1761	rBV	193	55	0.00%	0.000%
55	7.083	1784	1786	1789	rBV	196	130	0.01%	0.001%
56	7.115	1794	1796	1800	rVB	223	109	0.01%	0.001%
57	7.147	1803	1806	1810	rVB	381	337	0.02%	0.002%
58	7.173	1810	1814	1816	rBV	213	140	0.01%	0.001%
59	7.211	1818	1826	1836	rVB3	2024	2788	0.16%	0.020%
60	7.292	1847	1851	1855	rBV2	270	223	0.01%	0.002%
61	7.314	1855	1858	1860	rBV2	139	71	0.00%	0.000%
62	7.327	1860	1862	1863	rBV	90	45	0.00%	0.000%
63	7.407	1884	1887	1889	rBV2	280	146	0.01%	0.001%
64	7.436	1894	1896	1900	rVB2	253	145	0.01%	0.001%
65	7.455	1900	1902	1905	rBV2	117	57	0.00%	0.000%
66	7.481	1905	1910	1914	rBV2	248	244	0.01%	0.002%
67	7.529	1921	1925	1926	rBV	234	168	0.01%	0.001%
68	7.594	1930	1945	1967	rBV	217229	384523	21.99%	2.705%
69	7.700	1973	1978	1979	rBV3	1223	852	0.05%	0.006%
70	7.812	2009	2013	2014	rBV2	884	650	0.04%	0.005%
71	7.841	2021	2022	2024	rVB2	369	126	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061120\
 Data File : VU038779.D
 Acq On : 10 Jun 2020 16:30
 Operator : SY/MD
 Sample : VU0611WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

72	7.867	2026	2030	2031	rBV2	234	141	0.01%	0.001%
73	7.925	2032	2048	2079	rBV	741057	1356657	77.58%	9.545%
74	8.205	2123	2135	2152	rBV2	154848	259703	14.85%	1.827%
75	8.394	2191	2194	2198	rBV2	273	280	0.02%	0.002%
76	8.436	2203	2207	2210	rBV2	474	439	0.03%	0.003%
77	8.504	2220	2228	2232	rBV2	526	738	0.04%	0.005%
78	8.571	2247	2249	2250	rBV2	378	134	0.01%	0.001%
79	8.607	2257	2260	2262	rBV2	303	148	0.01%	0.001%
80	8.658	2262	2276	2306	rBV	618442	1095510	62.64%	7.707%
81	9.005	2382	2384	2386	rVB	283	145	0.01%	0.001%
82	9.041	2389	2395	2397	rBV2	405	417	0.02%	0.003%
83	9.140	2424	2426	2428	rBV	130	58	0.00%	0.000%
84	9.153	2428	2430	2433	rBV2	291	206	0.01%	0.001%
85	9.314	2477	2480	2483	rVB2	399	229	0.01%	0.002%
86	9.372	2495	2498	2500	rBV2	252	143	0.01%	0.001%
87	9.388	2500	2503	2504	rVV2	211	99	0.01%	0.001%
88	9.439	2505	2519	2554	rVV	855938	1470080	84.06%	10.343%
89	9.594	2562	2567	2569	rBV3	734	728	0.04%	0.005%
90	9.664	2587	2589	2590	rBV3	338	93	0.01%	0.001%
91	9.680	2590	2594	2596	rBV	329	273	0.02%	0.002%
92	10.307	2787	2789	2791	rBV2	733	447	0.03%	0.003%
93	10.774	2922	2934	2954	rVB	570999	907399	51.89%	6.384%
94	11.060	3021	3023	3026	rBV2	547	288	0.02%	0.002%
95	11.668	3207	3212	3214	rBV2	576	518	0.03%	0.004%
96	11.828	3249	3262	3277	rBV	903630	1425669	81.52%	10.030%
97	12.208	3367	3380	3399	rBV	835025	1347439	77.05%	9.480%


Sum of corrected areas: 14213904

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061120\
Data File : VU038779.D
Acq On : 10 Jun 2020 16:30
Operator : SY/MD
Sample : VU0611WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

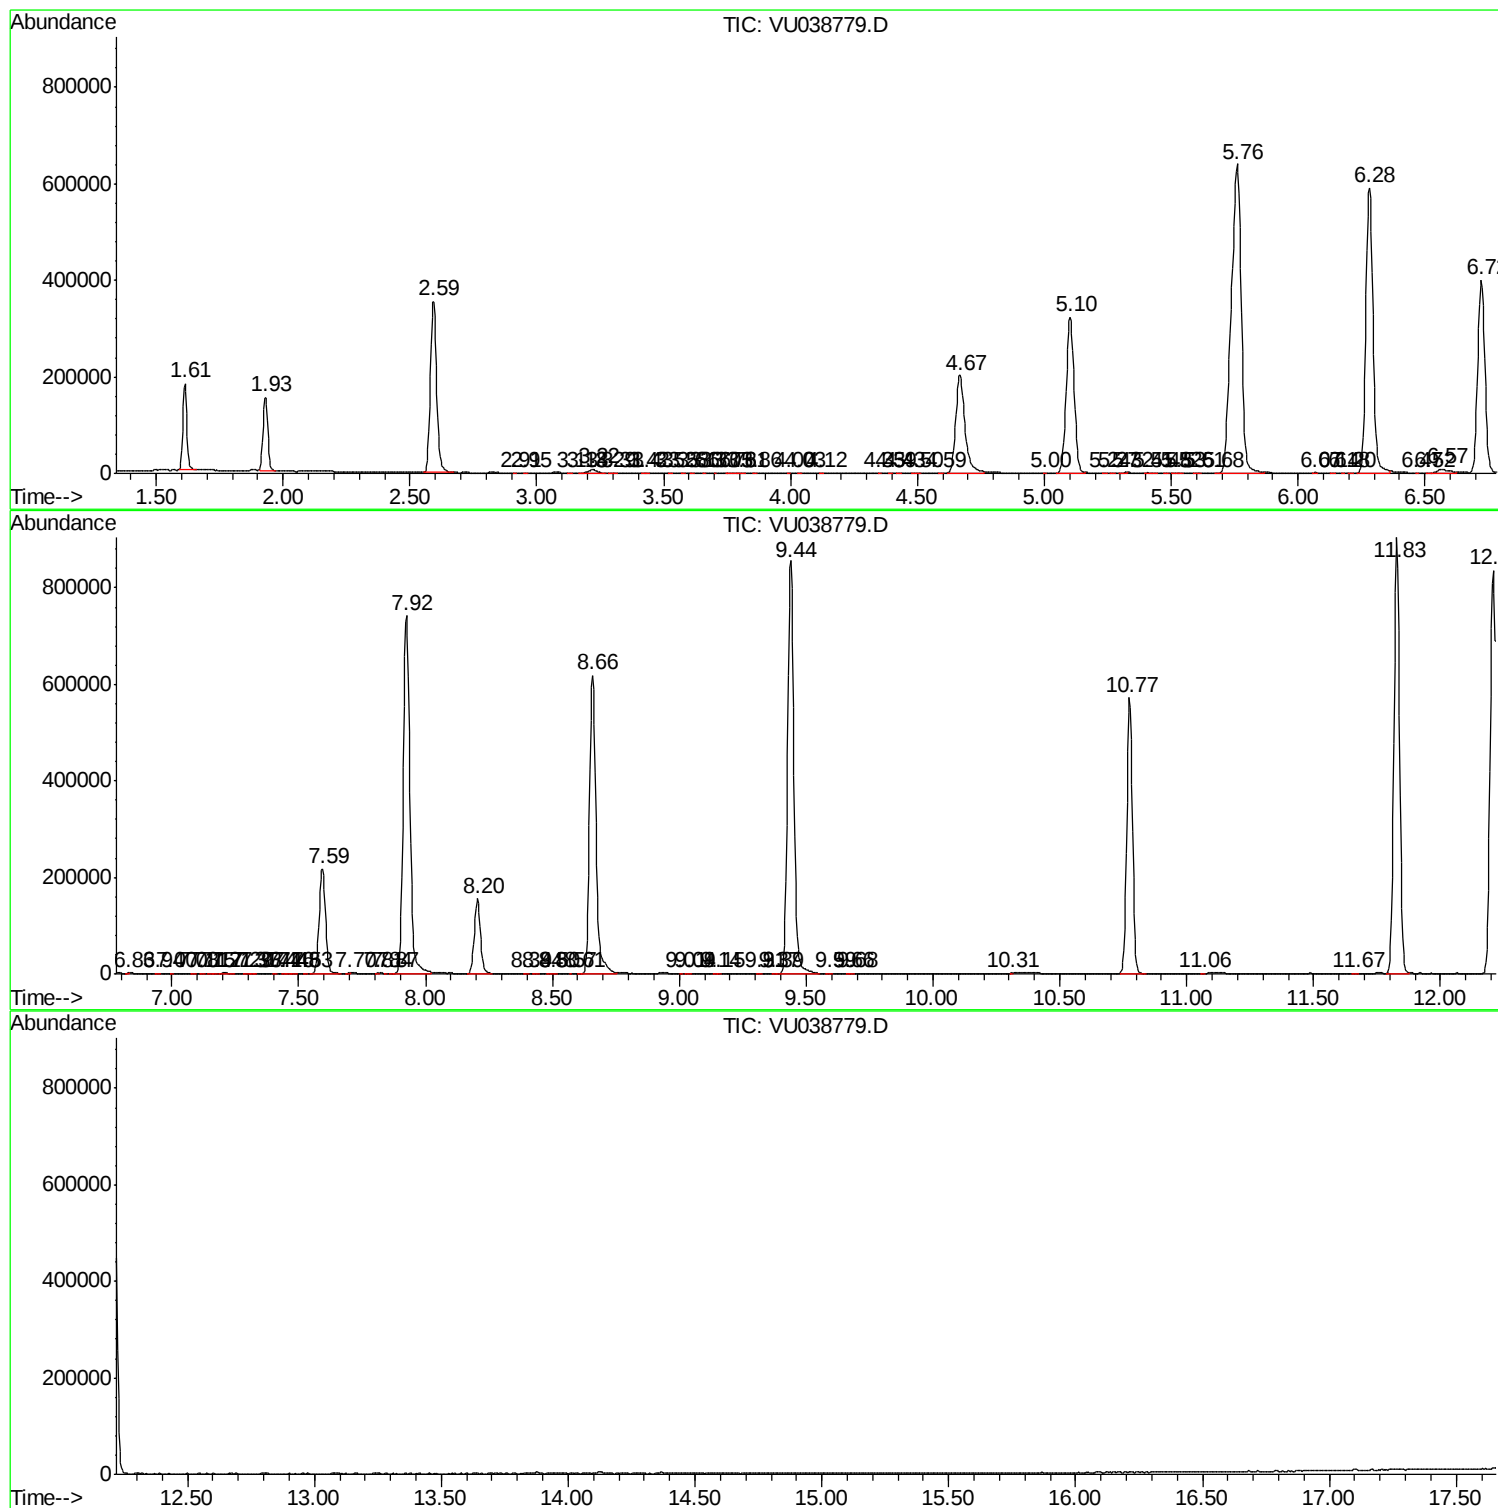

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061120\
Data File : VU038779.D
Acq On : 10 Jun 2020 16:30
Operator : SY/MD
Sample : VU0611WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061120\
Data File : VU038779.D
Acq On : 10 Jun 2020 16:30
Operator : SY/MD
Sample : VU0611WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc