

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061120\
 Data File : VU038783.D
 Acq On : 10 Jun 2020 18:11
 Operator : SY/MD
 Sample : L2913-06DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D85DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.369	5	9	20	rBV2	4957	5310	0.17%	0.026%
2	1.501	44	50	58	rBV3	16623	19373	0.63%	0.095%
3	1.613	75	85	95	rBV2	317194	354286	11.59%	1.739%
4	1.675	99	104	110	rVB	12178	12844	0.42%	0.063%
5	1.745	122	126	137	rVB	10251	12446	0.41%	0.061%
6	1.929	175	183	195	rVB	204282	264984	8.67%	1.301%
7	2.012	202	209	219	rVB	23446	32890	1.08%	0.161%
8	2.176	254	260	267	rVV2	11380	13477	0.44%	0.066%
9	2.224	268	275	289	rVB3	19617	31618	1.03%	0.155%
10	2.340	303	311	320	rVB2	12282	18132	0.59%	0.089%
11	2.440	335	342	350	rVB3	6526	9489	0.31%	0.047%
12	2.488	350	357	368	rVB2	8993	13388	0.44%	0.066%
13	2.591	377	389	408	rBV	460222	768188	25.12%	3.770%
14	2.810	453	457	458	rBV3	798	584	0.02%	0.003%
15	2.983	508	511	512	rVV2	744	405	0.01%	0.002%
16	2.993	512	514	517	rVV4	1179	728	0.02%	0.004%
17	3.044	520	530	546	rVV2	10642	22986	0.75%	0.113%
18	3.166	556	568	578	rBV2	19684	40348	1.32%	0.198%
19	3.401	637	641	643	rVB3	810	606	0.02%	0.003%
20	3.623	703	710	714	rBV5	951	1049	0.03%	0.005%
21	3.719	737	740	743	rBV2	545	406	0.01%	0.002%
22	3.761	750	753	757	rVB3	535	452	0.01%	0.002%
23	3.864	777	785	787	rBV2	444	517	0.02%	0.003%
24	4.006	824	829	833	rVV4	675	741	0.02%	0.004%
25	4.031	834	837	845	rVB4	716	724	0.02%	0.004%
26	4.205	882	891	896	rBV4	1922	3171	0.10%	0.016%
27	4.279	909	914	918	rBV2	623	636	0.02%	0.003%
28	4.475	970	975	978	rVV3	433	414	0.01%	0.002%
29	4.568	990	1004	1017	rBV5	7317	17298	0.57%	0.085%
30	4.662	1018	1033	1070	rBV	229609	583422	19.08%	2.864%
31	5.102	1152	1170	1191	rBV	366059	799228	26.14%	3.923%
32	5.321	1232	1238	1243	rBV4	1481	1984	0.06%	0.010%
33	5.420	1257	1269	1284	rVB5	12231	27908	0.91%	0.137%
34	5.575	1313	1317	1320	rVB2	534	466	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061120\
 Data File : VU038783.D
 Acq On : 10 Jun 2020 18:11
 Operator : SY/MD
 Sample : L2913-06DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D85DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

35	5.597	1320	1324	1327	rBV	561	385	0.01%	0.002%
36	5.758	1352	1374	1381	rBV2	761262	2023513	66.18%	9.932%
37	5.806	1382	1389	1419	rVB	1561469	3057542	100.00%	15.007%
38	6.054	1457	1466	1477	rVB6	8190	14464	0.47%	0.071%
39	6.215	1512	1516	1521	rVB5	761	691	0.02%	0.003%
40	6.279	1521	1536	1574	rBV	685097	1318359	43.12%	6.471%
41	6.494	1601	1603	1610	rVB2	523	487	0.02%	0.002%
42	6.562	1612	1624	1634	rBV4	11692	29328	0.96%	0.144%
43	6.719	1658	1673	1691	rBV	454492	891101	29.14%	4.374%
44	6.790	1692	1695	1697	rVB3	1603	1046	0.03%	0.005%
45	6.835	1703	1709	1716	rVB6	1214	1721	0.06%	0.008%
46	7.205	1817	1824	1831	rVV6	2396	3982	0.13%	0.020%
47	7.591	1930	1944	1968	rBV	255931	446825	14.61%	2.193%
48	7.703	1971	1979	1982	rBV6	1751	2319	0.08%	0.011%
49	7.813	2005	2013	2020	rBV4	1011	1362	0.04%	0.007%
50	7.922	2030	2047	2061	rBV	880755	1574793	51.51%	7.729%
51	7.993	2062	2069	2083	rVB	100464	181526	5.94%	0.891%
52	8.121	2104	2109	2121	rVB3	2383	3829	0.13%	0.019%
53	8.198	2121	2133	2154	rBV	184274	307379	10.05%	1.509%
54	8.292	2156	2162	2167	rVB5	1537	2304	0.08%	0.011%
55	8.571	2245	2249	2252	rBB2	818	420	0.01%	0.002%
56	8.655	2258	2275	2305	rBV	669586	1218119	39.84%	5.979%
57	8.819	2316	2326	2336	rVB8	2800	4897	0.16%	0.024%
58	8.861	2336	2339	2344	rVB3	639	557	0.02%	0.003%
59	8.935	2352	2362	2368	rBV4	3291	5584	0.18%	0.027%
60	9.353	2487	2492	2494	rBV3	530	478	0.02%	0.002%
61	9.382	2497	2501	2504	rBV3	640	677	0.02%	0.003%
62	9.433	2504	2517	2553	rVB	952786	1655731	54.15%	8.127%
63	9.587	2553	2565	2579	rBV	156259	257252	8.41%	1.263%
64	9.713	2589	2604	2619	rVB2	28445	50014	1.64%	0.245%
65	9.845	2638	2645	2650	rBV5	2184	2994	0.10%	0.015%
66	9.964	2676	2682	2692	rVV9	2211	3174	0.10%	0.016%
67	10.028	2696	2702	2708	rVV6	2078	3093	0.10%	0.015%
68	10.066	2710	2714	2719	rVV3	1602	2049	0.07%	0.010%
69	10.115	2719	2729	2745	rVB	52072	85438	2.79%	0.419%
70	10.295	2781	2785	2789	rVB3	974	937	0.03%	0.005%
71	10.346	2798	2801	2806	rVB3	517	560	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061120\
 Data File : VU038783.D
 Acq On : 10 Jun 2020 18:11
 Operator : SY/MD
 Sample : L2913-06DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D85DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

72	10.375	2806	2810	2813	rBV4	1111	840	0.03%	0.004%
73	10.439	2824	2830	2837	rVB4	842	1081	0.04%	0.005%
74	10.497	2838	2848	2858	rVB3	2631	4158	0.14%	0.020%
75	10.665	2894	2900	2904	rVB4	1157	1067	0.03%	0.005%
76	10.771	2920	2933	2953	rVB	617772	989861	32.37%	4.858%
77	10.919	2972	2979	2985	rVB4	1669	1996	0.07%	0.010%
78	10.989	2991	3001	3006	rBV4	2798	4790	0.16%	0.024%
79	11.304	3091	3099	3111	rVV2	5125	8099	0.26%	0.040%
80	11.353	3111	3114	3120	rVB3	596	434	0.01%	0.002%
81	11.410	3129	3132	3135	rBV2	889	659	0.02%	0.003%
82	11.478	3144	3153	3162	rBV3	7017	9739	0.32%	0.048%
83	11.822	3247	3260	3276	rBV	998821	1579756	51.67%	7.754%
84	11.906	3279	3286	3294	rVB2	6829	9734	0.32%	0.048%
85	11.967	3302	3305	3307	rBV2	540	437	0.01%	0.002%
86	12.002	3314	3316	3323	rVB2	416	373	0.01%	0.002%
87	12.102	3340	3347	3357	rVB6	3430	5111	0.17%	0.025%
88	12.205	3366	3379	3398	rVV	939041	1515690	49.57%	7.439%
89	12.742	3542	3546	3550	rVB2	455	406	0.01%	0.002%
90	12.790	3554	3561	3563	rBV3	789	899	0.03%	0.004%
91	13.320	3723	3726	3731	rBV3	513	493	0.02%	0.002%
92	13.864	3893	3895	3902	rVB4	840	713	0.02%	0.003%
93	14.018	3939	3943	3949	rBV3	634	702	0.02%	0.003%
94	14.073	3957	3960	3963	rBV2	580	526	0.02%	0.003%
95	14.111	3964	3972	3982	rVB2	11402	17842	0.58%	0.088%
96	14.233	4006	4010	4013	rBV4	937	894	0.03%	0.004%
97	14.359	4045	4049	4052	rVB3	1096	785	0.03%	0.004%
98	14.751	4168	4171	4173	rBV2	668	452	0.01%	0.002%
99	15.233	4318	4321	4325	rBV3	723	527	0.02%	0.003%
100	15.288	4336	4338	4341	rBV3	688	454	0.01%	0.002%


Sum of corrected areas: 20373946

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061120\
Data File : VU038783.D
Acq On : 10 Jun 2020 18:11
Operator : SY/MD
Sample : L2913-06DL 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D85DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

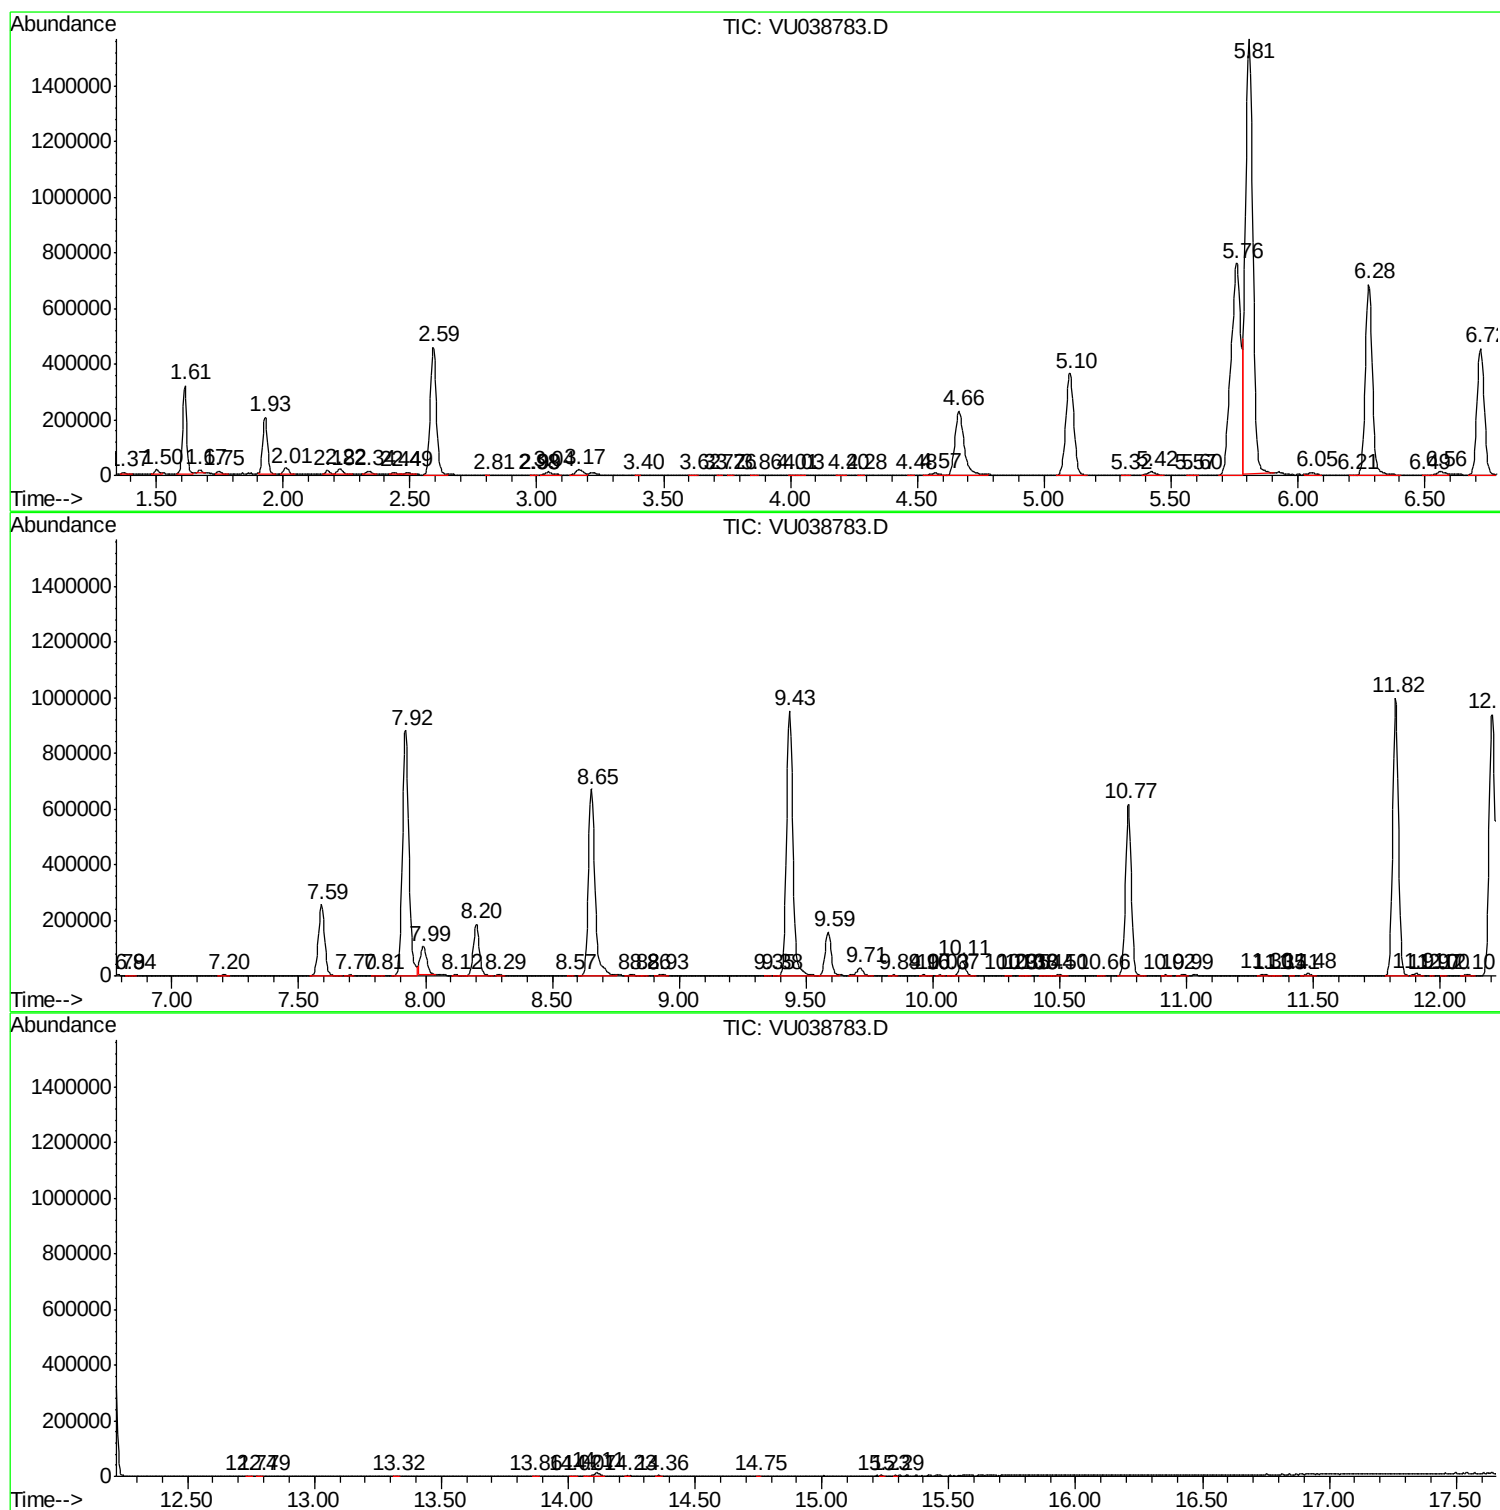

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061120\
Data File : VU038783.D
Acq On : 10 Jun 2020 18:11
Operator : SY/MD
Sample : L2913-06DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D85DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061120\
Data File : VU038783.D
Acq On : 10 Jun 2020 18:11
Operator : SY/MD
Sample : L2913-06DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D85DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc