

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061120\
 Data File : VU038784.D
 Acq On : 10 Jun 2020 18:33
 Operator : SY/MD
 Sample : L2913-07DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D93DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	77	85	97	rBV	310458	345707	16.05%	1.950%
2	1.928	175	183	197	rVB	221380	287767	13.36%	1.623%
3	2.012	202	209	219	rVB	36611	48795	2.27%	0.275%
4	2.591	378	389	407	rVB	497975	829399	38.51%	4.677%
5	2.928	492	494	496	rBV2	421	219	0.01%	0.001%
6	2.983	508	511	512	rBV3	530	324	0.02%	0.002%
7	3.054	523	533	534	rBV4	1945	2806	0.13%	0.016%
8	3.170	560	569	576	rBV3	15783	29580	1.37%	0.167%
9	3.391	628	638	640	rBV6	1912	2986	0.14%	0.017%
10	3.491	661	669	674	rBV2	428	699	0.03%	0.004%
11	3.549	682	687	690	rBV2	335	296	0.01%	0.002%
12	3.665	718	723	725	rBV	321	281	0.01%	0.002%
13	3.758	747	752	754	rBV2	182	187	0.01%	0.001%
14	3.851	772	781	784	rBV2	424	544	0.03%	0.003%
15	3.903	793	797	802	rVV2	440	428	0.02%	0.002%
16	3.925	802	804	808	rVB2	317	155	0.01%	0.001%
17	4.012	829	831	833	rBV	379	220	0.01%	0.001%
18	4.070	843	849	858	rBV3	357	479	0.02%	0.003%
19	4.108	858	861	863	rBV	288	186	0.01%	0.001%
20	4.208	888	892	900	rVB3	637	798	0.04%	0.005%
21	4.247	902	904	907	rBV	293	211	0.01%	0.001%
22	4.282	912	915	921	rBV2	374	353	0.02%	0.002%
23	4.346	932	935	938	rVB3	435	261	0.01%	0.001%
24	4.469	969	973	977	rBV2	421	340	0.02%	0.002%
25	4.514	984	987	990	rBV2	339	201	0.01%	0.001%
26	4.571	996	1005	1017	rVB3	7858	17423	0.81%	0.098%
27	4.665	1017	1034	1073	rBV	247874	638434	29.65%	3.600%
28	5.012	1138	1142	1144	rBV2	321	257	0.01%	0.001%
29	5.102	1152	1170	1196	rBV	409029	883418	41.02%	4.982%
30	5.295	1226	1230	1232	rBV3	759	520	0.02%	0.003%
31	5.321	1233	1238	1246	rVV4	1449	2204	0.10%	0.012%
32	5.424	1258	1270	1283	rVB7	11342	24024	1.12%	0.135%
33	5.472	1283	1285	1288	rVB2	398	157	0.01%	0.001%
34	5.504	1292	1295	1298	rVB	482	317	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061120\
 Data File : VU038784.D
 Acq On : 10 Jun 2020 18:33
 Operator : SY/MD
 Sample : L2913-07DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D93DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

35	5.526	1300	1302	1304	rBV	270	135	0.01%	0.001%
36	5.543	1304	1307	1313	rBV2	414	354	0.02%	0.002%
37	5.591	1320	1322	1327	rVB	416	241	0.01%	0.001%
38	5.639	1330	1337	1339	rBV2	304	261	0.01%	0.001%
39	5.655	1339	1342	1346	rBV3	281	273	0.01%	0.002%
40	5.758	1351	1374	1380	rBV2	841259	2153543	100.00%	12.144%
41	6.279	1522	1536	1561	rBV	685750	1322907	61.43%	7.460%
42	6.468	1592	1595	1603	rVB3	717	803	0.04%	0.005%
43	6.565	1612	1625	1633	rBV5	11767	28927	1.34%	0.163%
44	6.719	1659	1673	1690	rBV	498317	974392	45.25%	5.495%
45	6.944	1740	1743	1744	rBV2	379	225	0.01%	0.001%
46	6.996	1754	1759	1762	rBV2	458	385	0.02%	0.002%
47	7.057	1772	1778	1781	rBV	319	348	0.02%	0.002%
48	7.121	1794	1798	1799	rBV	241	150	0.01%	0.001%
49	7.205	1815	1824	1832	rBV5	2857	5080	0.24%	0.029%
50	7.308	1853	1856	1857	rVV	322	164	0.01%	0.001%
51	7.327	1860	1862	1864	rBV	436	178	0.01%	0.001%
52	7.346	1864	1868	1870	rBV	277	153	0.01%	0.001%
53	7.404	1883	1886	1888	rBV	261	167	0.01%	0.001%
54	7.420	1888	1891	1892	rBV	289	143	0.01%	0.001%
55	7.478	1905	1909	1912	rBV	168	177	0.01%	0.001%
56	7.587	1930	1943	1964	rBV	281895	499453	23.19%	2.817%
57	7.703	1973	1979	1992	rVB8	1847	3042	0.14%	0.017%
58	7.813	2009	2013	2016	rBV2	407	375	0.02%	0.002%
59	7.922	2032	2047	2063	rBV	960409	1743050	80.94%	9.829%
60	8.198	2120	2133	2151	rBV	198285	332222	15.43%	1.873%
61	8.388	2190	2192	2196	rVB2	289	199	0.01%	0.001%
62	8.456	2209	2213	2217	rBV2	388	277	0.01%	0.002%
63	8.520	2230	2233	2235	rBV	200	158	0.01%	0.001%
64	8.565	2244	2247	2248	rBV2	532	287	0.01%	0.002%
65	8.652	2260	2274	2305	rBV	727837	1309547	60.81%	7.385%
66	8.854	2335	2337	2340	rBV3	535	399	0.02%	0.002%
67	8.909	2352	2354	2357	rBV2	466	326	0.02%	0.002%
68	8.967	2368	2372	2374	rBV2	657	440	0.02%	0.002%
69	9.028	2387	2391	2394	rBV2	192	167	0.01%	0.001%
70	9.095	2408	2412	2418	rBV3	493	617	0.03%	0.003%
71	9.134	2423	2424	2427	rVB2	419	170	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061120\
 Data File : VU038784.D
 Acq On : 10 Jun 2020 18:33
 Operator : SY/MD
 Sample : L2913-07DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D93DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

72	9.214	2445	2449	2452	rBV2	382	308	0.01%	0.002%
73	9.237	2453	2456	2458	rBV2	284	182	0.01%	0.001%
74	9.356	2489	2493	2495	rBV	428	291	0.01%	0.002%
75	9.433	2503	2517	2553	rVB	955950	1670262	77.56%	9.419%
76	9.587	2553	2565	2582	rBV	112602	189703	8.81%	1.070%
77	9.848	2637	2646	2650	rBV8	2876	4414	0.20%	0.025%
78	9.957	2675	2680	2688	rBV4	2761	3682	0.17%	0.021%
79	10.025	2695	2701	2709	rBV5	2559	3678	0.17%	0.021%
80	10.115	2721	2729	2740	rVB2	7993	13601	0.63%	0.077%
81	10.176	2745	2748	2751	rBV2	271	219	0.01%	0.001%
82	10.295	2780	2785	2790	rVB5	2040	2198	0.10%	0.012%
83	10.443	2823	2831	2837	rVB7	2037	2844	0.13%	0.016%
84	10.494	2840	2847	2857	rVB5	2147	3282	0.15%	0.019%
85	10.632	2885	2890	2893	rBV2	467	475	0.02%	0.003%
86	10.664	2896	2900	2903	rBV3	1149	763	0.04%	0.004%
87	10.703	2908	2912	2915	rBV	375	321	0.01%	0.002%
88	10.771	2916	2933	2955	rBV	676952	1085021	50.38%	6.119%
89	10.854	2957	2959	2962	rBV3	505	255	0.01%	0.001%
90	11.304	3093	3099	3104	rBV	2761	3053	0.14%	0.017%
91	11.481	3146	3154	3164	rVB5	2923	4654	0.22%	0.026%
92	11.822	3247	3260	3279	rBV	1015323	1582270	73.47%	8.923%
93	11.902	3280	3285	3295	rVB5	6196	8269	0.38%	0.047%
94	12.105	3339	3348	3357	rVB3	9929	15996	0.74%	0.090%
95	12.201	3365	3378	3395	rBV	1010541	1624587	75.44%	9.161%
96	12.307	3408	3411	3412	rBV3	1080	686	0.03%	0.004%
97	12.414	3442	3444	3450	rBV2	437	446	0.02%	0.003%
98	12.671	3522	3524	3525	rBV	1067	412	0.02%	0.002%
99	12.690	3525	3530	3540	rVB7	3025	4455	0.21%	0.025%
100	14.115	3966	3973	3979	rBV3	5451	6935	0.32%	0.039%


Sum of corrected areas: 17732973

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061120\
Data File : VU038784.D
Acq On : 10 Jun 2020 18:33
Operator : SY/MD
Sample : L2913-07DL 40X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D93DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

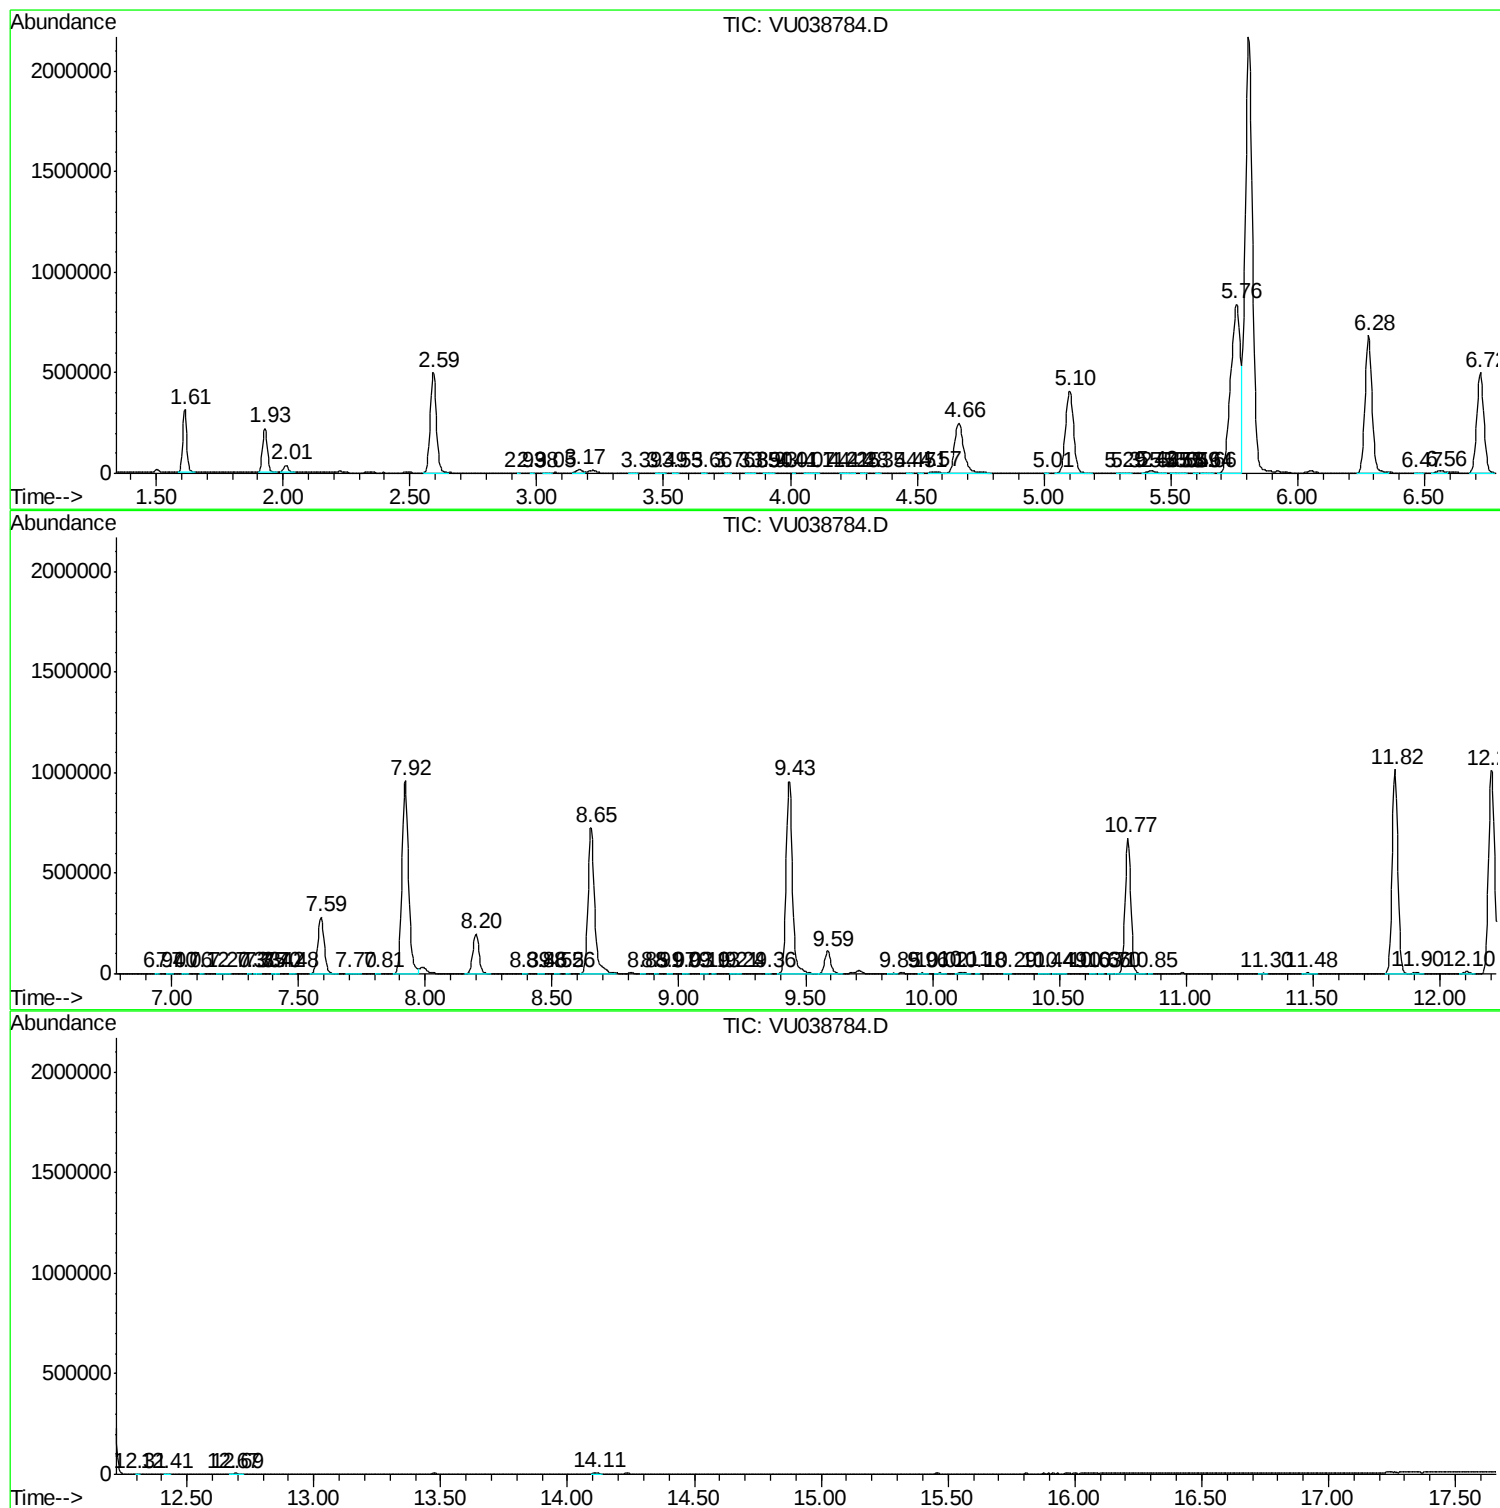

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061120\
Data File : VU038784.D
Acq On : 10 Jun 2020 18:33
Operator : SY/MD
Sample : L2913-07DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D93DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061120\
Data File : VU038784.D
Acq On : 10 Jun 2020 18:33
Operator : SY/MD
Sample : L2913-07DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D93DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc