

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061120\
 Data File : VU038785.D
 Acq On : 10 Jun 2020 18:55
 Operator : SY/MD
 Sample : L2913-08DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D95DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.369	5	9	16	rBV4	3933	3823	0.09%	0.017%
2	1.501	44	50	57	rBV2	13822	16388	0.40%	0.075%
3	1.613	77	85	97	rBV	316437	340382	8.22%	1.555%
4	1.929	175	183	199	rVB	217539	278848	6.73%	1.274%
5	2.009	202	208	219	rVB2	30254	42893	1.04%	0.196%
6	2.224	270	275	285	rVB3	5767	8529	0.21%	0.039%
7	2.343	306	312	320	rBV8	2544	3390	0.08%	0.015%
8	2.491	350	358	367	rBV3	5473	9176	0.22%	0.042%
9	2.594	376	390	420	rVB	487820	835976	20.18%	3.819%
10	2.803	451	455	456	rBV2	520	331	0.01%	0.002%
11	3.038	522	528	529	rBV2	1706	1152	0.03%	0.005%
12	3.166	558	568	577	rBV2	16549	33869	0.82%	0.155%
13	3.221	579	585	602	rVV	15901	32915	0.79%	0.150%
14	3.385	629	636	637	rBV3	1576	1663	0.04%	0.008%
15	3.607	700	705	706	rBV2	444	325	0.01%	0.001%
16	3.832	773	775	782	rVB2	330	372	0.01%	0.002%
17	4.102	854	859	864	rVB3	336	351	0.01%	0.002%
18	4.208	886	892	896	rBV4	526	548	0.01%	0.003%
19	4.571	991	1005	1018	rBV4	6905	16376	0.40%	0.075%
20	4.665	1018	1034	1065	rBV	251068	657733	15.88%	3.005%
21	4.967	1125	1128	1133	rBV4	577	479	0.01%	0.002%
22	5.102	1151	1170	1193	rVV	408156	870874	21.03%	3.979%
23	5.324	1232	1239	1251	rVB3	2423	4976	0.12%	0.023%
24	5.420	1257	1269	1282	rVV6	9370	20532	0.50%	0.094%
25	5.520	1295	1300	1307	rBV2	453	521	0.01%	0.002%
26	5.761	1351	1375	1380	rBV2	820476	2112442	51.00%	9.651%
27	5.806	1382	1389	1421	rVB	2077389	4141991	100.00%	18.924%
28	6.054	1459	1466	1479	rVB4	9438	17354	0.42%	0.079%
29	6.279	1520	1536	1573	rBV	675542	1312318	31.68%	5.996%
30	6.562	1610	1624	1634	rBV4	10841	28086	0.68%	0.128%
31	6.719	1658	1673	1692	rBV	495474	966610	23.34%	4.416%
32	6.822	1703	1705	1707	rBV2	587	358	0.01%	0.002%
33	6.838	1707	1710	1716	rVB5	1816	1901	0.05%	0.009%
34	7.083	1782	1786	1790	rVB2	391	343	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U061120\
 Data File : VU038785.D
 Acq On : 10 Jun 2020 18:55
 Operator : SY/MD
 Sample : L2913-08DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D95DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

35	7.208	1817	1825	1835	rVB6	2582	4052	0.10%	0.019%
36	7.587	1928	1943	1964	rBV	274600	482778	11.66%	2.206%
37	7.700	1975	1978	1979	rBV2	904	562	0.01%	0.003%
38	7.764	1993	1998	1999	rBV3	494	448	0.01%	0.002%
39	7.777	2000	2002	2009	rVB5	605	516	0.01%	0.002%
40	7.922	2031	2047	2062	rBV	959217	1727082	41.70%	7.891%
41	8.198	2120	2133	2152	rBV	199623	332300	8.02%	1.518%
42	8.375	2184	2188	2193	rBV2	330	331	0.01%	0.002%
43	8.414	2198	2200	2204	rVB2	439	342	0.01%	0.002%
44	8.443	2204	2209	2210	rBV2	671	512	0.01%	0.002%
45	8.578	2244	2251	2254	rBV4	733	768	0.02%	0.004%
46	8.655	2260	2275	2310	rBV	740473	1340033	32.35%	6.122%
47	8.812	2318	2324	2325	rBV4	2605	2703	0.07%	0.012%
48	8.851	2333	2336	2340	rVB2	385	326	0.01%	0.001%
49	8.951	2364	2367	2371	rBV3	563	493	0.01%	0.002%
50	9.288	2469	2472	2478	rBV3	480	489	0.01%	0.002%
51	9.433	2494	2517	2553	rBV	950800	1652956	39.91%	7.552%
52	9.587	2554	2565	2582	rBV	103944	170242	4.11%	0.778%
53	9.665	2586	2589	2590	rBV3	1066	575	0.01%	0.003%
54	9.710	2596	2603	2614	rVB3	14013	23670	0.57%	0.108%
55	9.845	2637	2645	2649	rVV5	3139	3892	0.09%	0.018%
56	9.880	2649	2656	2665	rVB6	3604	5708	0.14%	0.026%
57	9.960	2676	2681	2689	rVB4	3210	3999	0.10%	0.018%
58	10.031	2695	2703	2709	rBV6	2677	4089	0.10%	0.019%
59	10.115	2721	2729	2740	rVB4	7990	11582	0.28%	0.053%
60	10.195	2752	2754	2761	rBV2	353	328	0.01%	0.001%
61	10.291	2777	2784	2788	rBV5	1210	1674	0.04%	0.008%
62	10.382	2806	2812	2819	rBV3	1315	1597	0.04%	0.007%
63	10.430	2822	2827	2828	rBV3	1258	1053	0.03%	0.005%
64	10.497	2840	2848	2856	rVB3	2048	2949	0.07%	0.013%
65	10.664	2894	2900	2906	rBV4	1205	1316	0.03%	0.006%
66	10.771	2916	2933	2953	rBV	674554	1088934	26.29%	4.975%
67	10.867	2961	2963	2970	rVB2	648	566	0.01%	0.003%
68	10.906	2970	2975	2976	rBV	913	631	0.02%	0.003%
69	10.989	2992	3001	3005	rBV4	2555	3627	0.09%	0.017%
70	11.079	3026	3029	3035	rBV3	719	718	0.02%	0.003%
71	11.205	3064	3068	3073	rVB2	476	331	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061120\
 Data File : VU038785.D
 Acq On : 10 Jun 2020 18:55
 Operator : SY/MD
 Sample : L2913-08DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D95DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

72	11.301	3091	3098	3104	rBV3	2070	2920	0.07%	0.013%
73	11.333	3106	3108	3110	rBV2	819	469	0.01%	0.002%
74	11.410	3129	3132	3134	rBV3	1372	1106	0.03%	0.005%
75	11.478	3147	3153	3160	rVB4	2531	3076	0.07%	0.014%
76	11.693	3218	3220	3225	rBV	639	489	0.01%	0.002%
77	11.738	3229	3234	3235	rBV2	458	335	0.01%	0.002%
78	11.822	3247	3260	3277	rBV	1010364	1568553	37.87%	7.166%
79	11.906	3277	3286	3294	rVB5	5603	8363	0.20%	0.038%
80	11.941	3294	3297	3299	rBV3	752	461	0.01%	0.002%
81	12.005	3313	3317	3320	rBV2	559	444	0.01%	0.002%
82	12.105	3339	3348	3358	rVB3	10158	14185	0.34%	0.065%
83	12.205	3365	3379	3394	rBV	1007389	1623748	39.20%	7.418%
84	12.443	3447	3453	3455	rBV2	789	763	0.02%	0.003%
85	12.626	3505	3510	3514	rBV4	571	512	0.01%	0.002%
86	12.674	3523	3525	3526	rVV2	746	371	0.01%	0.002%
87	12.690	3526	3530	3544	rVB5	2600	3615	0.09%	0.017%
88	12.796	3557	3563	3566	rBV2	767	805	0.02%	0.004%
89	12.886	3589	3591	3594	rBV	427	337	0.01%	0.002%
90	13.195	3684	3687	3690	rBV	669	449	0.01%	0.002%
91	13.298	3716	3719	3723	rBV2	495	368	0.01%	0.002%
92	13.471	3764	3773	3779	rBV5	3111	4238	0.10%	0.019%
93	13.645	3823	3827	3831	rBV5	1353	1267	0.03%	0.006%
94	13.690	3838	3841	3846	rBV2	455	464	0.01%	0.002%
95	13.860	3890	3894	3897	rBV4	678	466	0.01%	0.002%
96	14.108	3965	3971	3981	rVB2	4475	6574	0.16%	0.030%
97	14.172	3989	3991	3993	rBV2	515	329	0.01%	0.002%
98	14.237	4003	4011	4022	rBV3	2702	4186	0.10%	0.019%
99	14.481	4084	4087	4089	rBV3	618	372	0.01%	0.002%
100	14.770	4173	4177	4182	rBV4	596	626	0.02%	0.003%


Sum of corrected areas: 21887888

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061120\
Data File : VU038785.D
Acq On : 10 Jun 2020 18:55
Operator : SY/MD
Sample : L2913-08DL 40X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D95DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

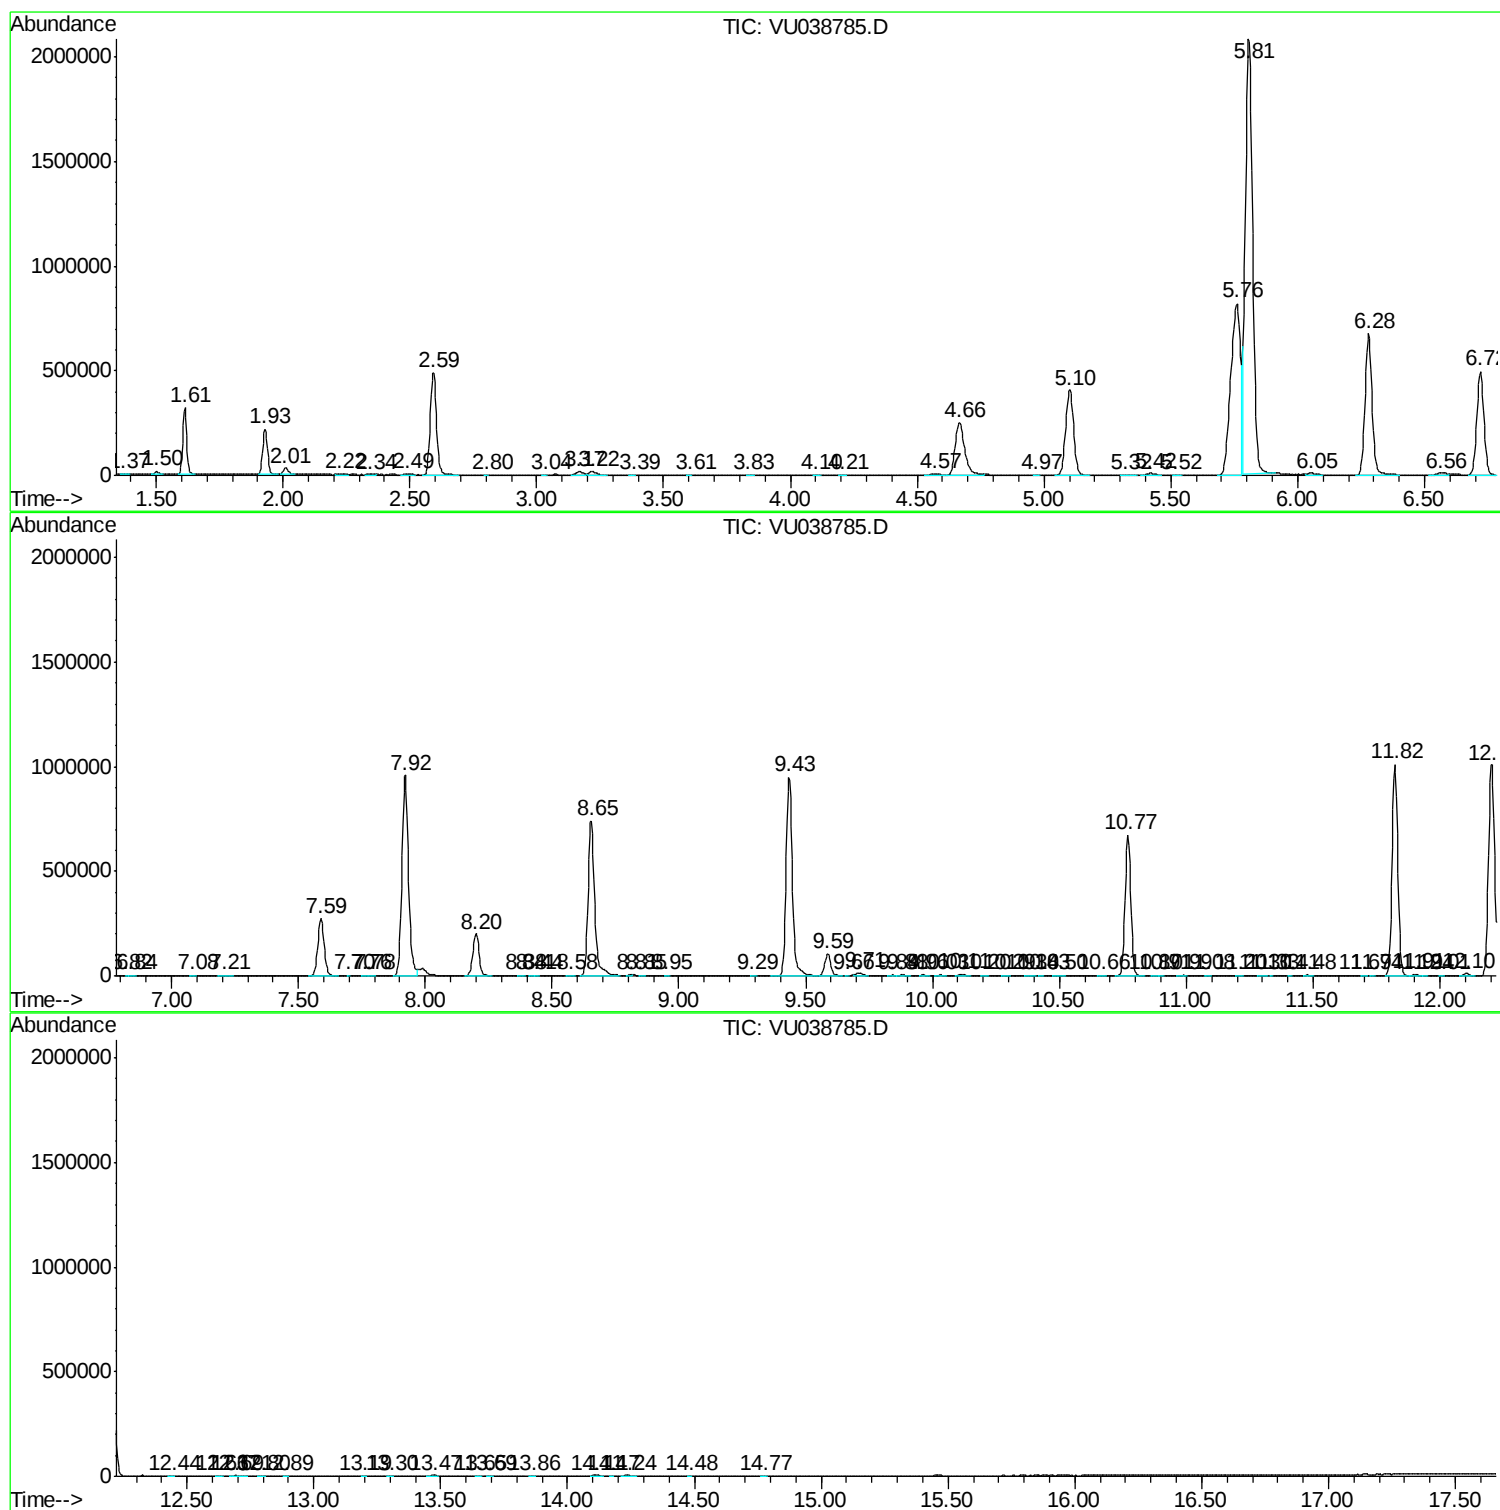

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061120\
Data File : VU038785.D
Acq On : 10 Jun 2020 18:55
Operator : SY/MD
Sample : L2913-08DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D95DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061120\
Data File : VU038785.D
Acq On : 10 Jun 2020 18:55
Operator : SY/MD
Sample : L2913-08DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D95DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc