


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061120\
 Data File : VU038777.D
 Acq On : 10 Jun 2020 14:17
 Operator : SY/MD
 Sample : BFB53
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB53

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis
 Last Update : Thu Jun 11 10:55:48 2020

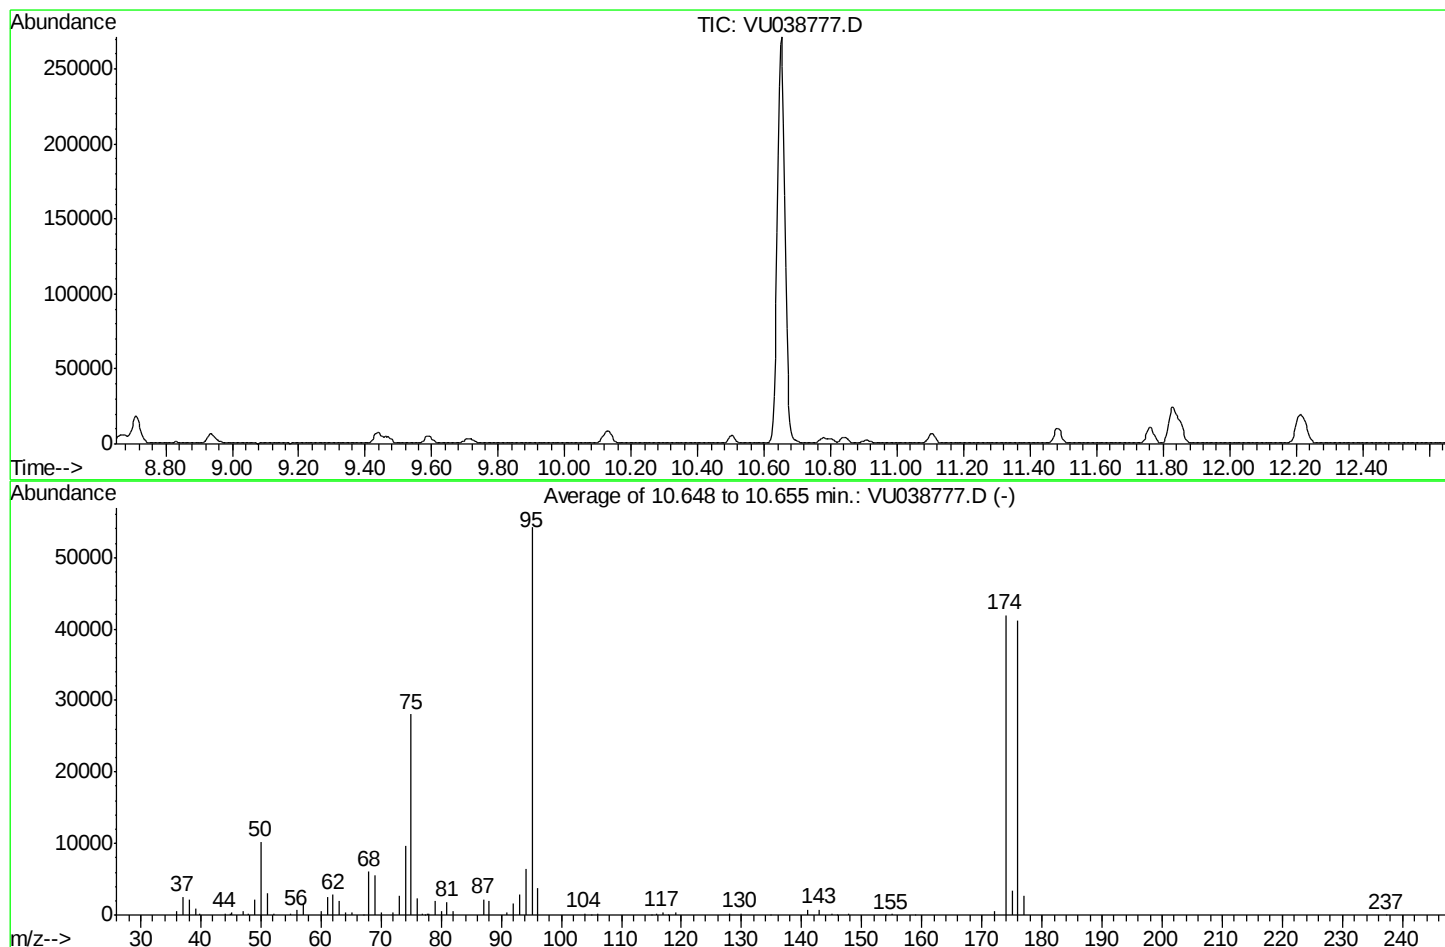

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	10291	PASS
75	95	30	80	51.8	28082	PASS
95	95	100	100	100.0	54216	PASS
96	95	5	9	6.9	3734	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.3	41922	PASS
175	174	5	9	8.0	3343	PASS
176	174	95	101	98.3	41213	PASS
177	176	5	9	6.4	2649	PASS

m/z	Abundance
35.00	521.0
37.00	2661.0
38.00	2095.0
39.00	926.0
40.00	255.0
44.00	729.0
45.00	467.0
47.00	713.0
47.90	268.0
49.00	2086.0
50.00	10608.0
51.00	3249.0
52.10	228.0
55.00	177.0
55.90	718.0
57.00	1708.0
60.00	488.0
61.00	2641.0
62.00	2694.0
63.00	2110.0
64.10	323.0
65.10	297.0
67.10	159.0
68.00	6289.0
69.00	5754.0
70.00	415.0
72.00	326.0
73.00	2738.0
74.00	9808.0
75.00	28856.0
76.00	2615.0
76.90	198.0
77.70	276.0
79.00	2027.0
80.00	621.0
80.90	1821.0
81.90	455.0
87.00	2341.0
88.00	2417.0
90.90	340.0
92.00	1863.0
93.00	2995.0
94.10	6449.0
95.10	54504.0
96.00	3570.0
103.80	278.0
105.90	222.0
115.80	164.0
116.90	407.0
117.80	166.0
119.00	367.0
127.90	211.0
129.90	218.0
134.80	102.0
140.90	671.0
143.00	710.0
145.00	152.0
147.80	103.0
155.10	173.0
172.00	544.0
174.00	41704.0
175.10	3310.0
176.00	41248.0
177.00	2696.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
35.90	523.0
37.00	2584.0
38.00	2123.0
39.00	888.0
40.00	281.0
44.00	716.0
45.20	547.0
46.90	598.0
47.90	269.0
49.10	2314.0
50.00	10497.0
51.00	3094.0
52.10	173.0
55.00	149.0
55.90	685.0
57.00	1611.0
60.10	554.0
61.00	2601.0
62.00	2891.0
63.00	1994.0
64.10	296.0
65.10	357.0
68.00	6247.0
69.00	5844.0
70.10	406.0
72.00	363.0
73.00	2840.0
74.00	9946.0
75.00	28880.0
76.00	2452.0
77.00	266.0
77.80	346.0
78.90	2112.0
79.90	563.0
80.90	1826.0
81.90	546.0
87.00	2163.0
88.00	2044.0
90.90	325.0
92.00	1766.0
93.10	2968.0
94.10	6693.0
95.10	56064.0
96.00	3924.0
103.90	250.0
104.90	116.0
106.00	223.0
114.90	123.0
115.80	128.0
116.90	443.0
117.70	113.0
118.90	383.0
127.90	201.0
129.90	235.0
134.80	105.0
140.90	728.0
143.00	797.0
145.00	156.0
145.90	104.0
147.80	175.0
155.10	156.0
158.80	119.0
172.00	548.0
174.00	43168.0
175.10	3392.0
176.00	42544.0
177.00	2744.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	509.0
37.00	2420.0
38.00	1993.0
39.10	778.0
39.90	305.0
44.00	779.0
45.20	587.0
46.90	446.0
47.90	270.0
49.10	2257.0
50.00	9768.0
51.10	2743.0
55.00	112.0
55.90	625.0
57.00	1276.0
60.00	506.0
61.00	2355.0
62.00	2883.0
63.10	1763.0
64.10	295.0
65.10	350.0
68.00	5655.0
69.00	5213.0
70.00	398.0
72.00	368.0
73.10	2651.0
74.00	9065.0
75.00	26512.0
76.00	2193.0
77.20	283.0
78.00	408.0
78.90	1960.0
79.90	568.0
81.00	1752.0
81.90	537.0
87.00	1969.0
87.90	1623.0
90.90	250.0
92.00	1482.0
93.10	2614.0
94.10	6356.0
95.10	52080.0
96.00	3708.0
104.00	215.0
104.90	157.0
106.00	211.0
114.90	111.0
115.90	133.0
116.90	446.0
118.90	344.0
127.90	149.0
129.90	206.0
140.90	722.0
143.00	734.0
145.00	163.0
147.80	193.0
154.00	104.0
155.00	112.0
158.80	118.0
172.00	460.0
174.00	40896.0
175.10	3327.0
176.00	39848.0
177.00	2507.0
237.30	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

Scan 2883 (10.610 min): VU038777.D
BFB53

m/z	Abundance
39.80	155.0
43.90	518.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53