

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049063.D
 Acq On : 11 Jun 2022 19:32
 Operator : SY/MD
 Sample : N3277-06 500X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BA5

Quant Time: Jun 13 01:49:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 13 01:35:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	143995	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	142843	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	66854	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	30800	4.836	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.800%
7) Chloroethane-d5	1.916	69	35352	5.091	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.800%
11) 1,1-Dichloroethene-d2	2.568	65	16528	4.971	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	99.400%
20) 2-Butanone-d5	4.636	46	186436	58.795	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.600%
24) Chloroform-d	5.067	84	101013	4.908	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	5.703	65	59802	5.250	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.000%
32) Benzene-d6	5.729	84	181959	4.744	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
36) 1,2-Dichloropropane-d6	6.690	67	63763	4.878	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.600%
41) Toluene-d8	7.899	98	138489	4.297	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%
43) trans-1,3-Dichloroprop...	8.182	79	20058	4.568	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.400%
46) 2-Hexanone-d5	8.636	63	129784	53.953	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.900%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	61644	5.363	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.200%
66) 1,2-Dichlorobenzene-d4	12.195	152	63751	5.184	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.600%
Target Compounds						
					Qvalue	
34) Trichloroethene	6.542	95	29148	2.636	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049063.D
Acq On : 11 Jun 2022 19:32
Operator : SY/MD
Sample : N3277-06 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA5

Quant Time: Jun 13 01:49:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 13 01:35:15 2022
Response via : Initial Calibration

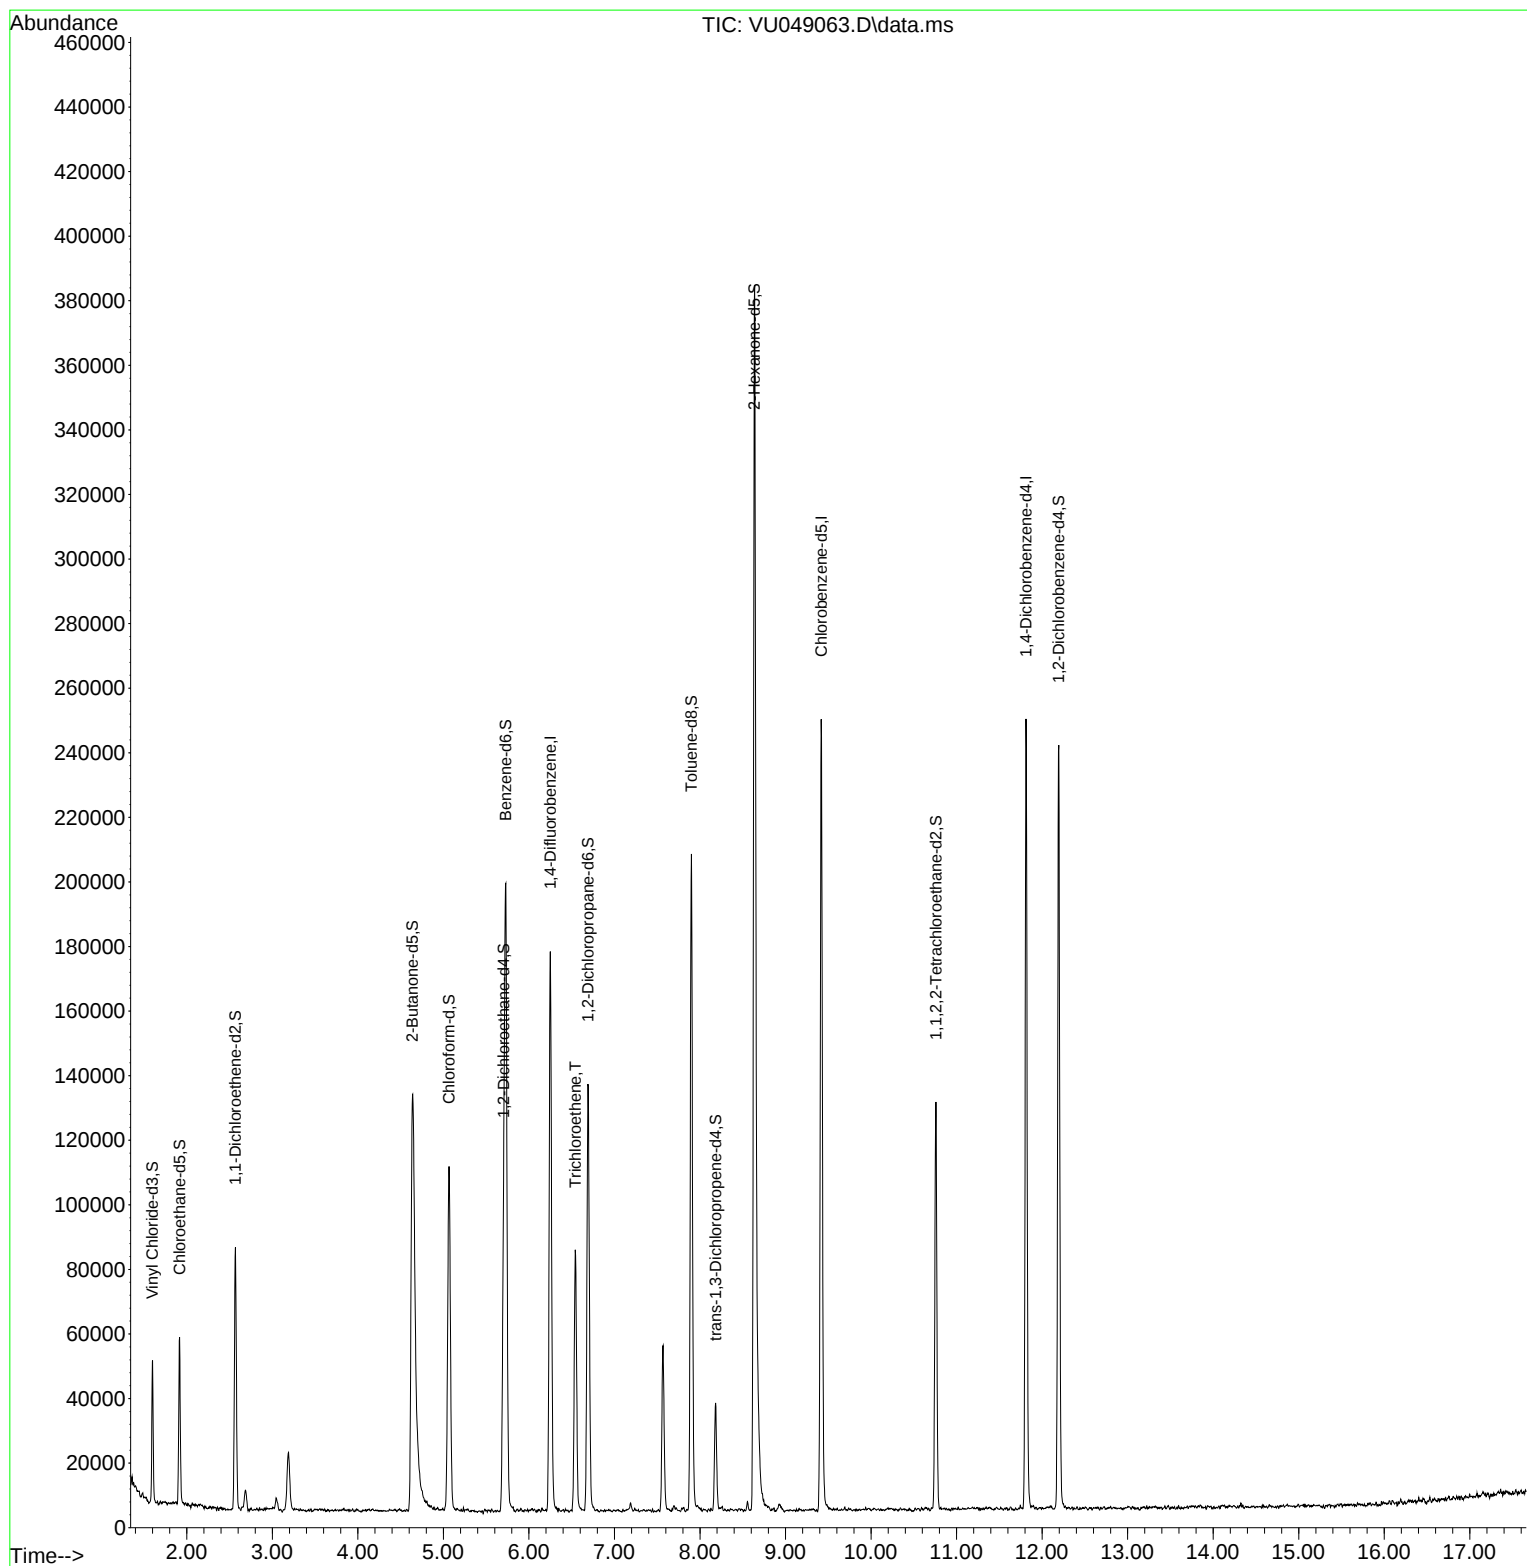

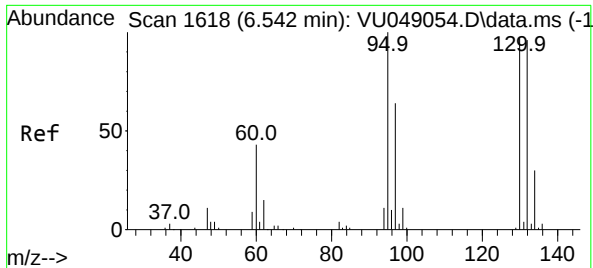

#34
 Trichloroethene
 Concen: 2.636 ug/L
 RT: 6.542 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VU049063.D
 Acq: 11 Jun 2022 19:32

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BA5

Tgt Ion: 95	Resp: 29148
Ion Ratio	Lower Upper
95 100	
97 59.2	44.9 83.5
132 87.4	62.8 116.6
130 96.5	70.4 130.8

