

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049064.D
 Acq On : 11 Jun 2022 19:55
 Operator : SY/MD
 Sample : N3278-01 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC8

Quant Time: Jun 13 01:49:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 13 01:35:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	139242	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	135890	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	61548	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	28165	4.573	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.400%	
7) Chloroethane-d5	1.912	69	33242	4.950	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.000%	
11) 1,1-Dichloroethene-d2	2.568	65	13884	4.318	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	86.400%	
20) 2-Butanone-d5	4.636	46	173070	56.443	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	112.880%	
24) Chloroform-d	5.066	84	100443	5.046	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.000%	
26) 1,2-Dichloroethane-d4	5.703	65	60087	5.455	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	109.000%	
32) Benzene-d6	5.729	84	177231	4.857	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.200%	
36) 1,2-Dichloropropane-d6	6.693	67	64516	5.189	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	103.800%	
41) Toluene-d8	7.899	98	132805	4.331	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.600%	
43) trans-1,3-Dichloroprop...	8.179	79	19923	4.769	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.400%	
46) 2-Hexanone-d5	8.635	63	130353	56.962	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	113.920%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	60591	5.541	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	110.800%	
66) 1,2-Dichlorobenzene-d4	12.192	152	60254	5.322	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	106.400%	
Target Compounds						Qvalue
9) Trichlorofluoromethane	2.141	101	2231	0.133	ug/L	# 81
34) Trichloroethene	6.542	95	18372	1.747	ug/L	91
47) Tetrachloroethene	8.555	164	11009	1.317	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049064.D
Acq On : 11 Jun 2022 19:55
Operator : SY/MD
Sample : N3278-01 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC8

Quant Time: Jun 13 01:49:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 13 01:35:15 2022
Response via : Initial Calibration




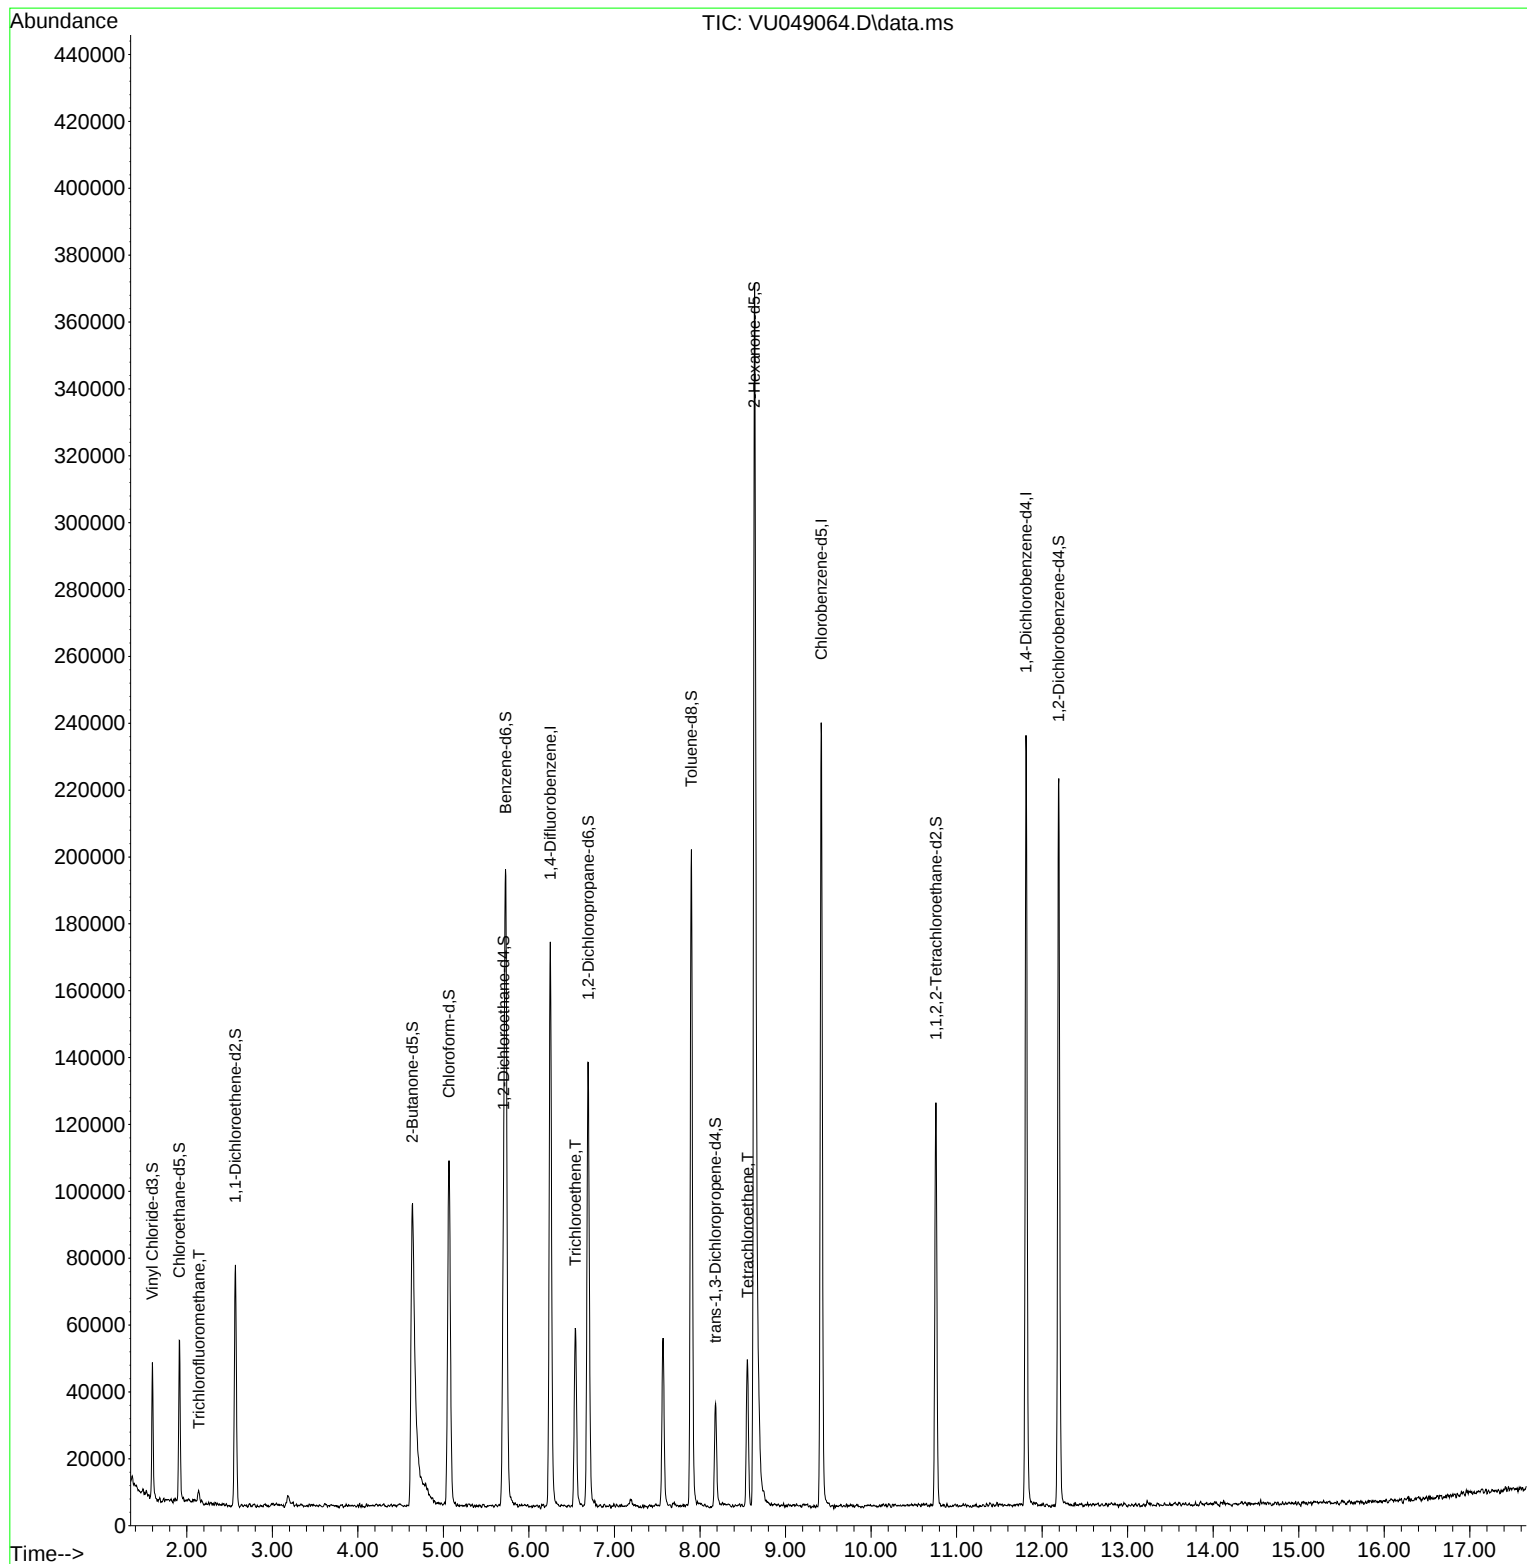


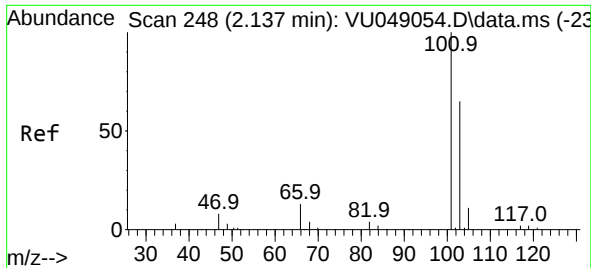

#9
Trichlorofluoromethane
Concen: 0.133 ug/L
RT: 2.141 min Scan# 248
Delta R.T. 0.003 min
Lab File: VU049064.D
Acq: 11 Jun 2022 19:55




Instrument :
MSVOA_U
ClientSampleId :
C0BC8


Tgt Ion:101 Resp: 2231
Ion Ratio Lower Upper
101 100
103 77.9 50.5 75.7#

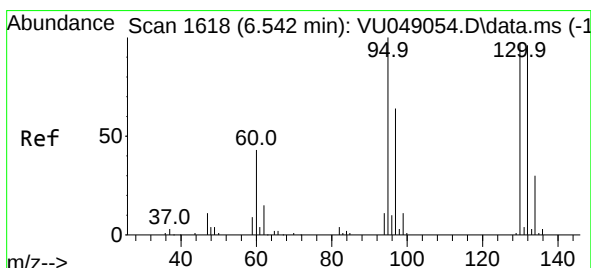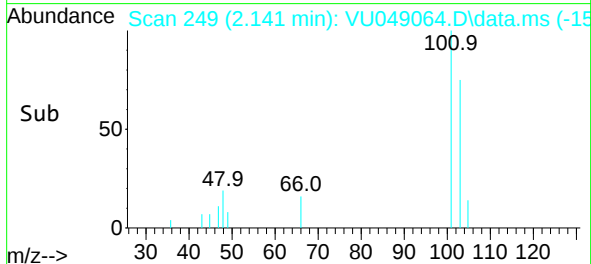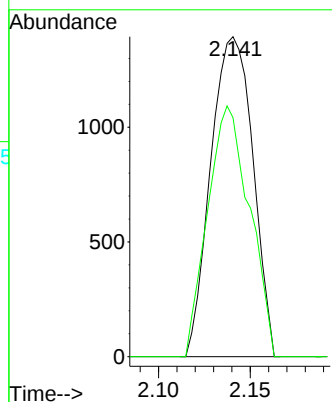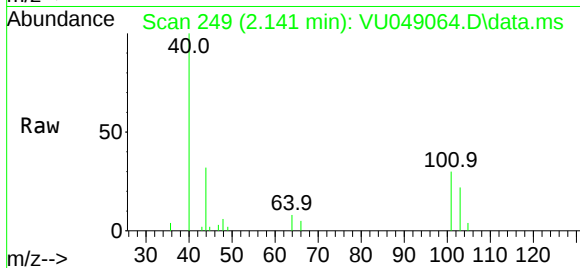

#34
Trichloroethene
Concen: 1.747 ug/L
RT: 6.542 min Scan# 1618
Delta R.T. -0.000 min
Lab File: VU049064.D
Acq: 11 Jun 2022 19:55


Tgt Ion: 95 Resp: 18372
Ion Ratio Lower Upper
95 100
97 71.1 44.9 83.5
132 106.0 62.8 116.6
130 101.9 70.4 130.8

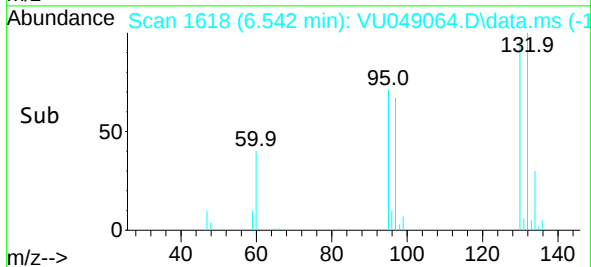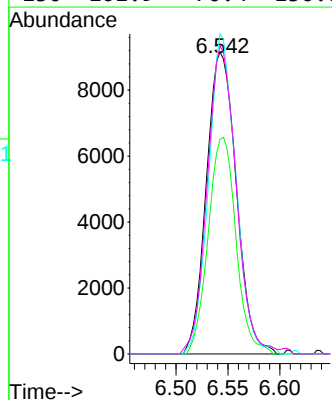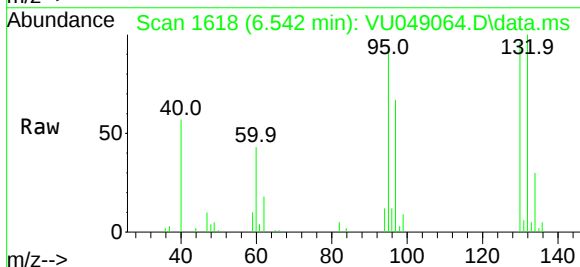

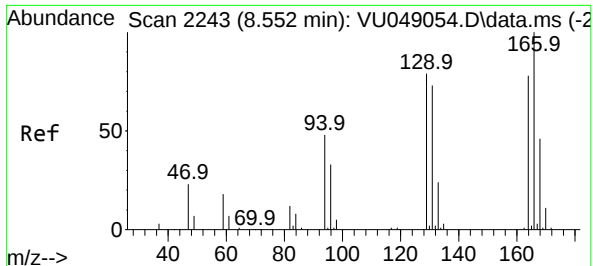

#47
 Tetrachloroethene
 Concen: 1.317 ug/L
 RT: 8.555 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: VU049064.D
 Acq: 11 Jun 2022 19:55

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC8

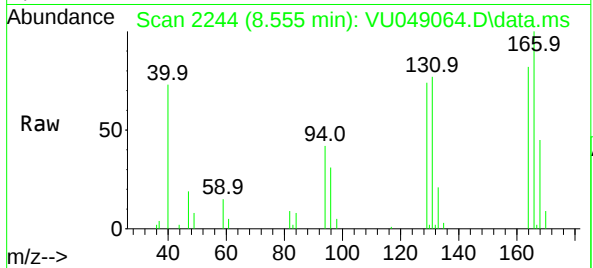

Tgt	Ion:164	Resp:	11009
Ion	Ratio	Lower	Upper
164	100		
129	90.6	67.0	124.4
131	94.4	65.0	120.8
166	121.9	92.5	171.7

