

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049076.D
 Acq On : 12 Jun 2022 00:40
 Operator : SY/MD
 Sample : N3277-20 2000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC7

Quant Time: Jun 13 01:52:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 13 01:35:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	138374	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	137934	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	62216	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	29363	4.798	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.000%
7) Chloroethane-d5	1.916	69	35684	5.347	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.000%
11) 1,1-Dichloroethene-d2	2.568	65	15086	4.722	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.400%
20) 2-Butanone-d5	4.636	46	178171	58.471	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.940%
24) Chloroform-d	5.063	84	100749	5.094	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.800%
26) 1,2-Dichloroethane-d4	5.707	65	60007	5.482	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.600%
32) Benzene-d6	5.729	84	174688	4.717	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.400%
36) 1,2-Dichloropropane-d6	6.694	67	60259	4.774	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.400%
41) Toluene-d8	7.899	98	130887	4.205	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.200%
43) trans-1,3-Dichloroprop...	8.182	79	19046	4.491	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.800%
46) 2-Hexanone-d5	8.636	63	125165	53.884	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.760%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	58520	5.272	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.400%
66) 1,2-Dichlorobenzene-d4	12.195	152	58996	5.155	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.000%
Target Compounds						
					Qvalue	
34) Trichloroethene	6.546	95	7193	0.674	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049076.D
Acq On : 12 Jun 2022 00:40
Operator : SY/MD
Sample : N3277-20 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC7


Quant Time: Jun 13 01:52:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 13 01:35:15 2022
Response via : Initial Calibration

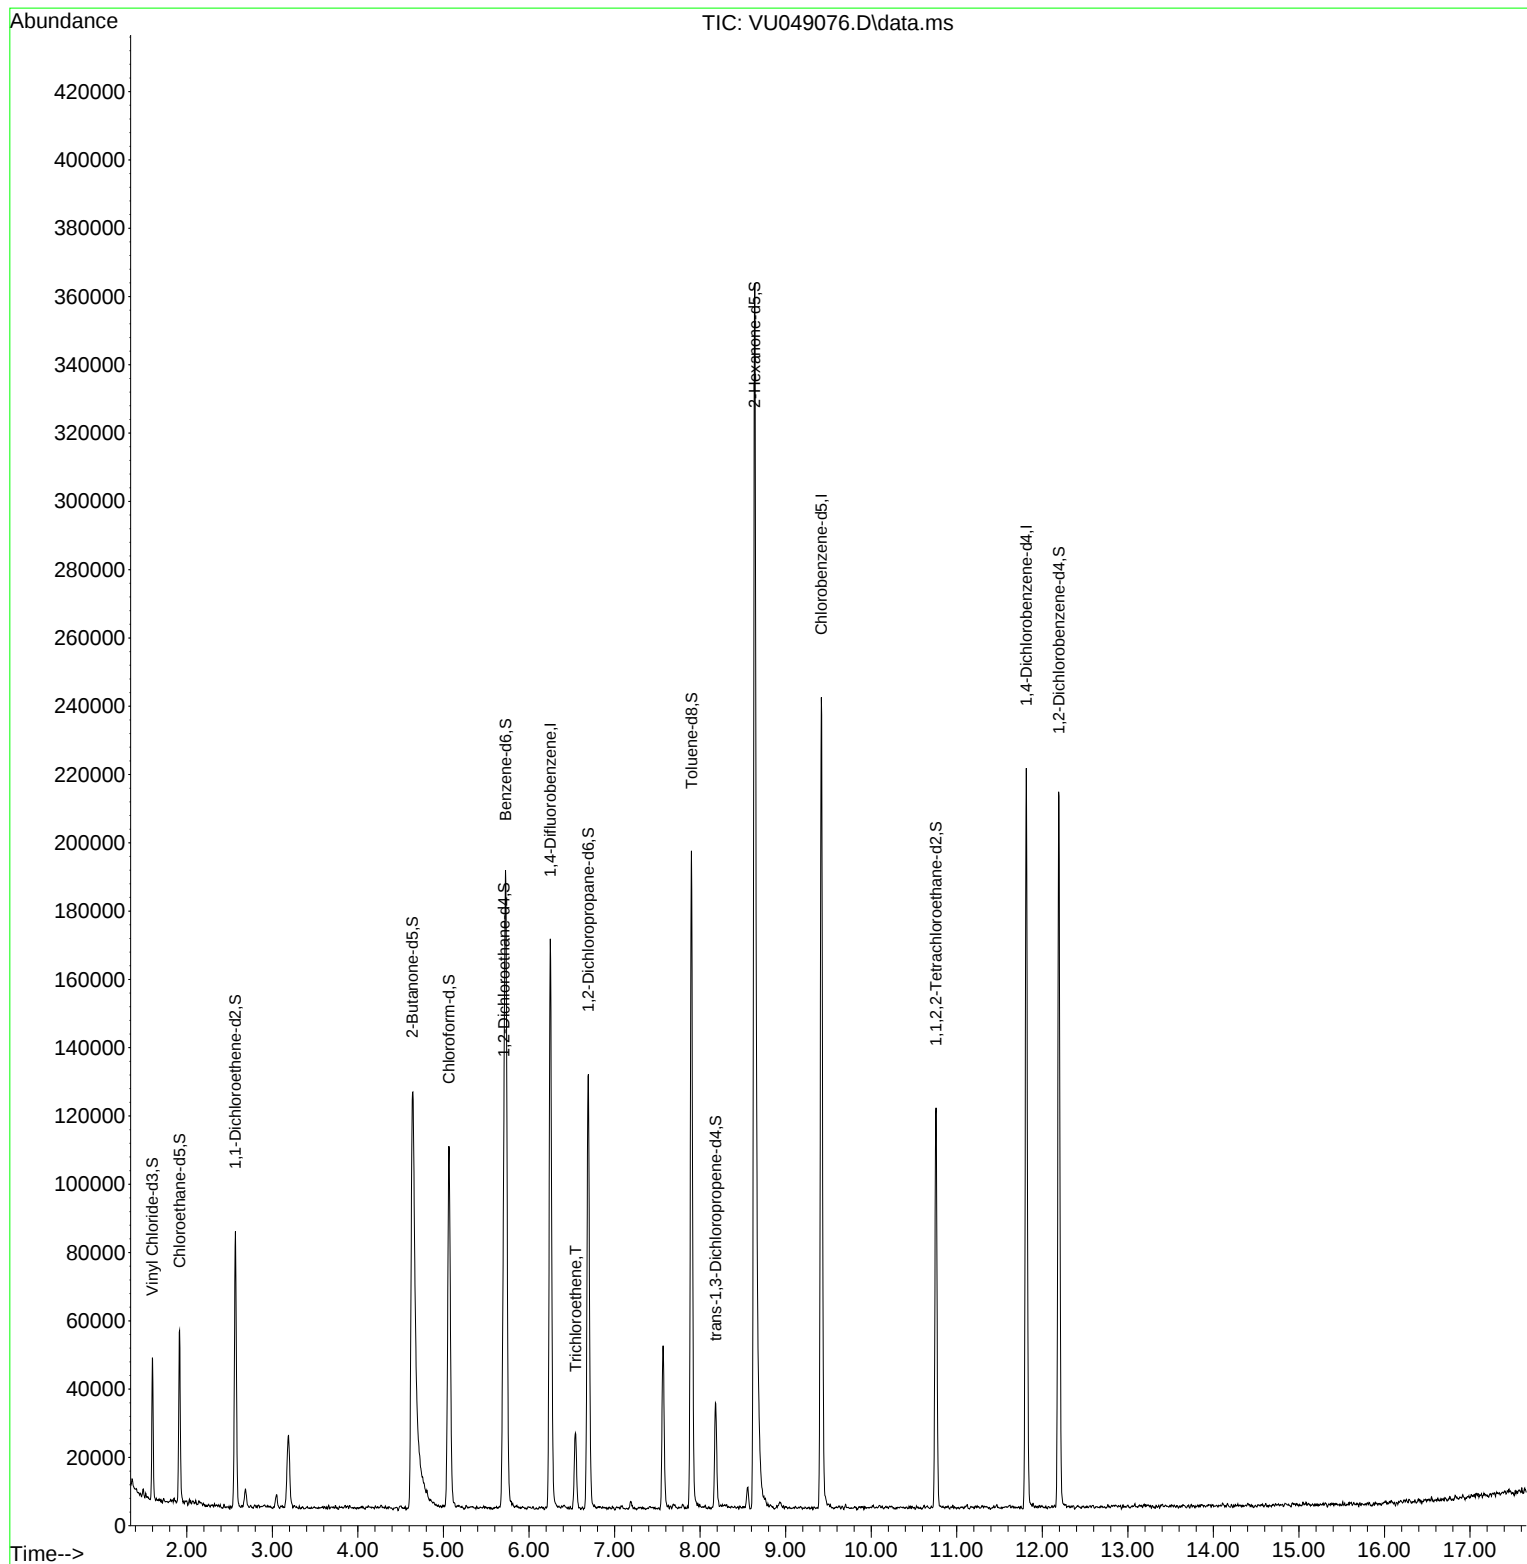

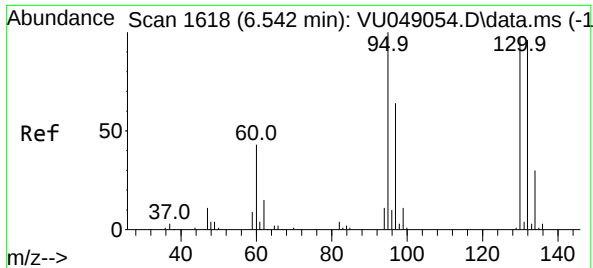

#34
 Trichloroethene
 Concen: 0.674 ug/L
 RT: 6.546 min Scan# 1
 Delta R.T. 0.003 min
 Lab File: VU049076.D
 Acq: 12 Jun 2022 00:40

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC7

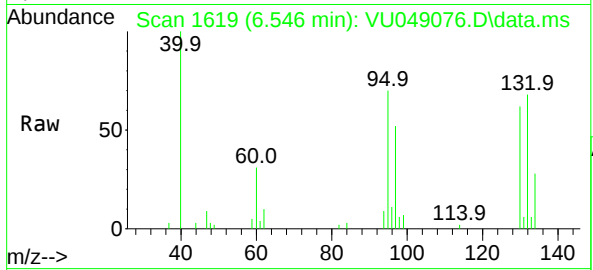

Tgt Ion: 95 Resp: 7193

Ion	Ratio	Lower	Upper
95	100		
97	74.0	44.9	83.5
132	97.7	62.8	116.6
130	88.7	70.4	130.8

