

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049055.D
 Acq On : 11 Jun 2022 16:22
 Operator : SY/MD
 Sample : VU0611WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK084

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	91	rBV	44301	49930	7.12%	1.148%
2	1.916	170	179	192	rBV	52887	66795	9.52%	1.536%
3	2.568	370	382	397	rBV	83379	134891	19.22%	3.102%
4	4.633	1011	1024	1053	rBV	76080	229321	32.68%	5.274%
5	5.063	1142	1158	1181	rBV	106231	234186	33.38%	5.386%
6	5.726	1343	1364	1389	rBV2	192334	514552	73.33%	11.833%
7	6.250	1513	1527	1545	rBV	170720	329110	46.90%	7.569%
8	6.694	1651	1665	1687	rBV2	131158	260375	37.11%	5.988%
9	7.568	1923	1937	1954	rBV2	52116	93396	13.31%	2.148%
10	7.899	2026	2040	2057	rBV	205700	358092	51.03%	8.235%
11	8.182	2117	2128	2148	rBV	32934	58628	8.36%	1.348%
12	8.639	2256	2270	2307	rBV3	299019	701670	100.00%	16.136%
13	9.420	2500	2513	2537	rBV	236771	409299	58.33%	9.413%
14	10.758	2915	2929	2944	rBV	106737	177433	25.29%	4.080%
15	11.816	3246	3258	3276	rBV	218209	353674	50.40%	8.134%
16	12.195	3364	3376	3395	rBV2	212003	353302	50.35%	8.125%
17	13.848	3882	3890	3899	rBV5	4433	7250	1.03%	0.167%
18	14.092	3957	3966	3980	rBV2	5111	8793	1.25%	0.202%
19	14.333	4030	4041	4055	rVB4	4707	7660	1.09%	0.176%




Sum of corrected areas: 4348357

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049055.D
Acq On : 11 Jun 2022 16:22
Operator : SY/MD
Sample : VU0611WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK084

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

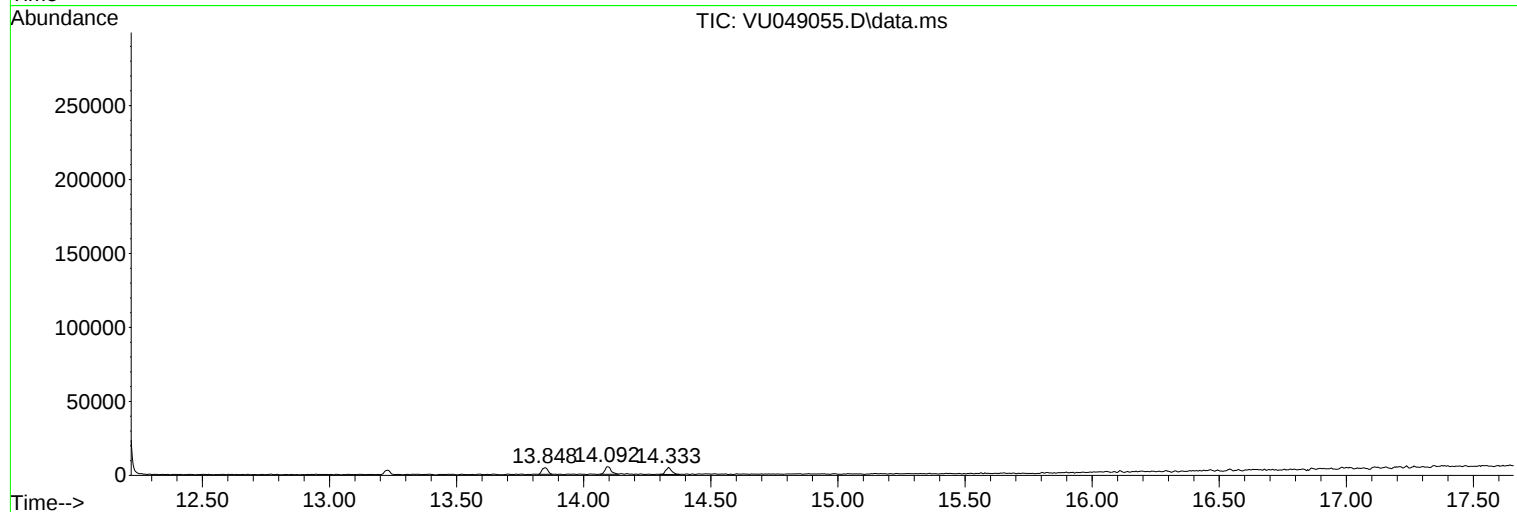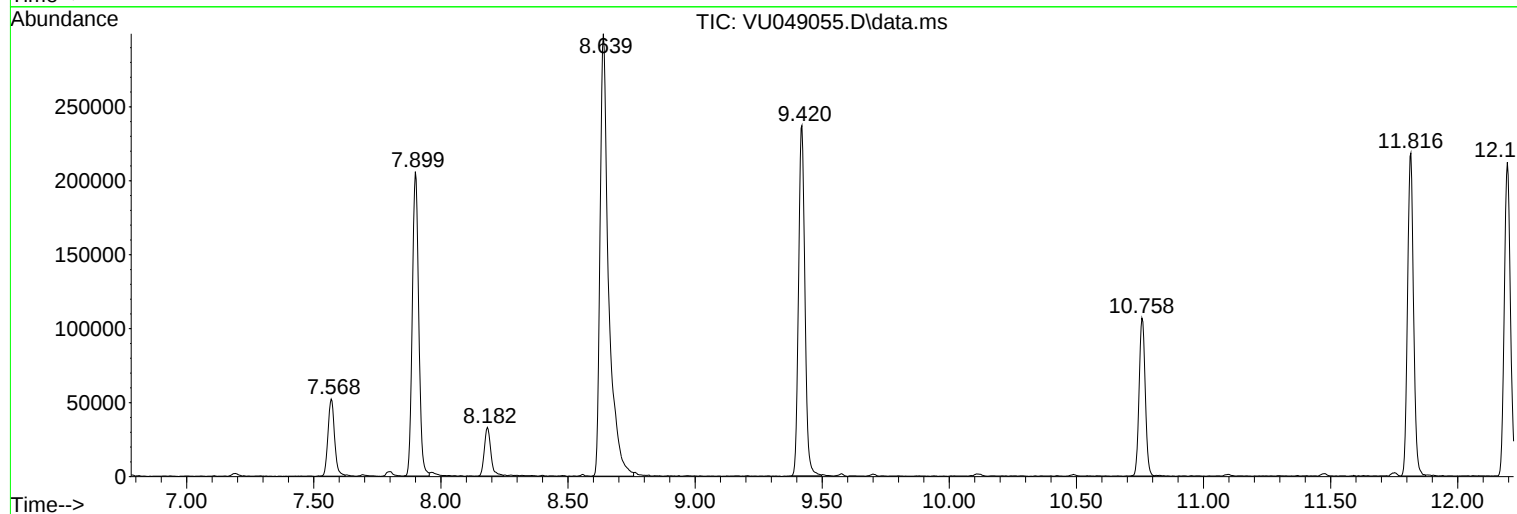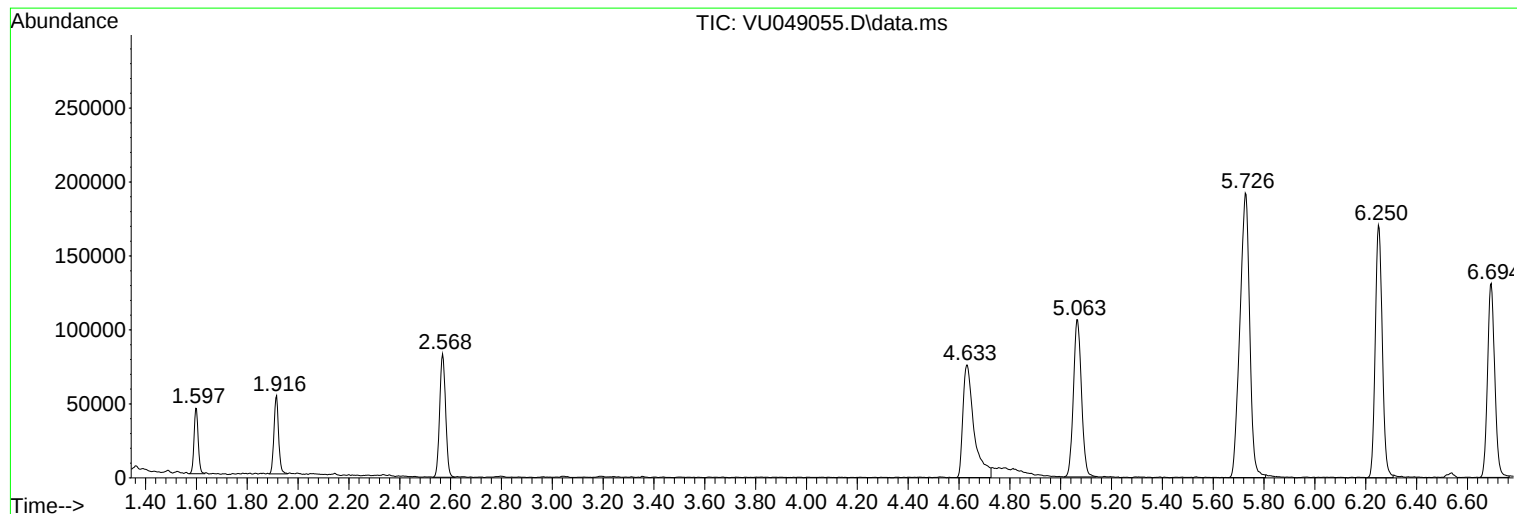

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049055.D
Acq On : 11 Jun 2022 16:22
Operator : SY/MD
Sample : VU0611WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK084

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049055.D
Acq On : 11 Jun 2022 16:22
Operator : SY/MD
Sample : VU0611WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK084

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc