

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049058.D
 Acq On : 11 Jun 2022 17:33
 Operator : SY/MD
 Sample : N3277-04 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B87

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	89	rBV	46003	51162	6.87%	1.045%
2	1.916	170	179	188	rBV	52831	67123	9.01%	1.371%
3	2.568	371	382	395	rVB	88064	142353	19.10%	2.909%
4	3.041	526	529	543	rVB6	4794	8068	1.08%	0.165%
5	3.189	562	575	590	rBV3	10292	24272	3.26%	0.496%
6	4.639	1010	1026	1061	rBV3	121419	400842	53.80%	8.190%
7	5.063	1140	1158	1179	rBV	114291	252459	33.88%	5.158%
8	5.726	1340	1364	1386	rBV4	199878	536297	71.97%	10.958%
9	6.250	1514	1527	1548	rBV	182841	350080	46.98%	7.153%
10	6.546	1606	1619	1635	rVB4	33803	66136	8.88%	1.351%
11	6.690	1652	1664	1689	rBV	140881	273048	36.64%	5.579%
12	7.568	1925	1937	1954	rBV	53945	97589	13.10%	1.994%
13	7.899	2027	2040	2059	rBV	217451	383456	51.46%	7.835%
14	8.179	2117	2127	2148	rBV2	34718	62894	8.44%	1.285%
15	8.555	2232	2244	2254	rBV3	18690	33313	4.47%	0.681%
16	8.636	2257	2269	2300	rBV4	347434	745125	100.00%	15.224%
17	9.417	2499	2512	2532	rBV	265432	446190	59.88%	9.116%
18	10.758	2917	2929	2944	rVB	117064	186489	25.03%	3.810%
19	11.812	3245	3257	3277	rBV	241965	389924	52.33%	7.967%
20	12.192	3364	3375	3393	rBV	227249	377513	50.66%	7.713%




Sum of corrected areas: 4894333

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049058.D
Acq On : 11 Jun 2022 17:33
Operator : SY/MD
Sample : N3277-04 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

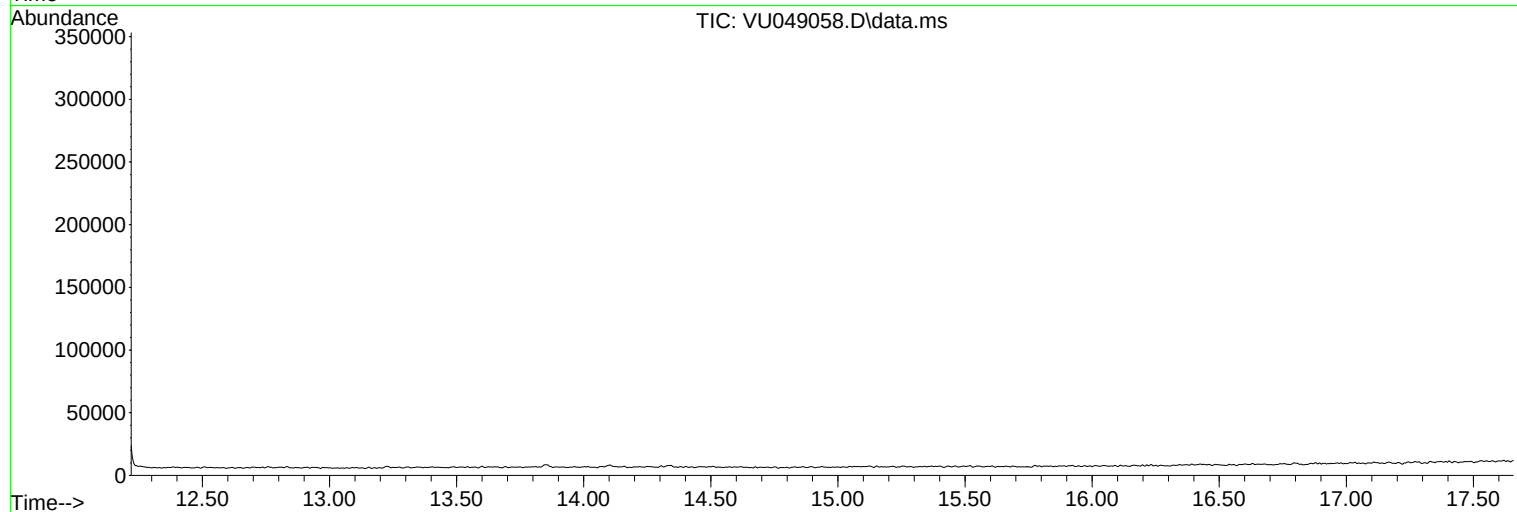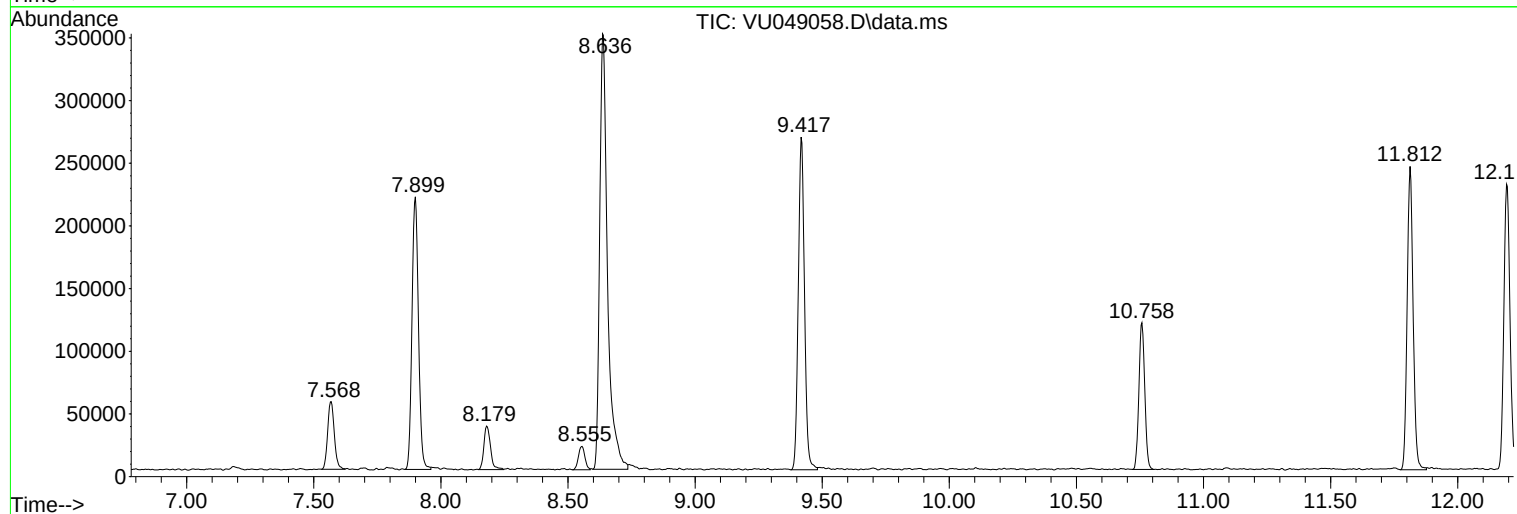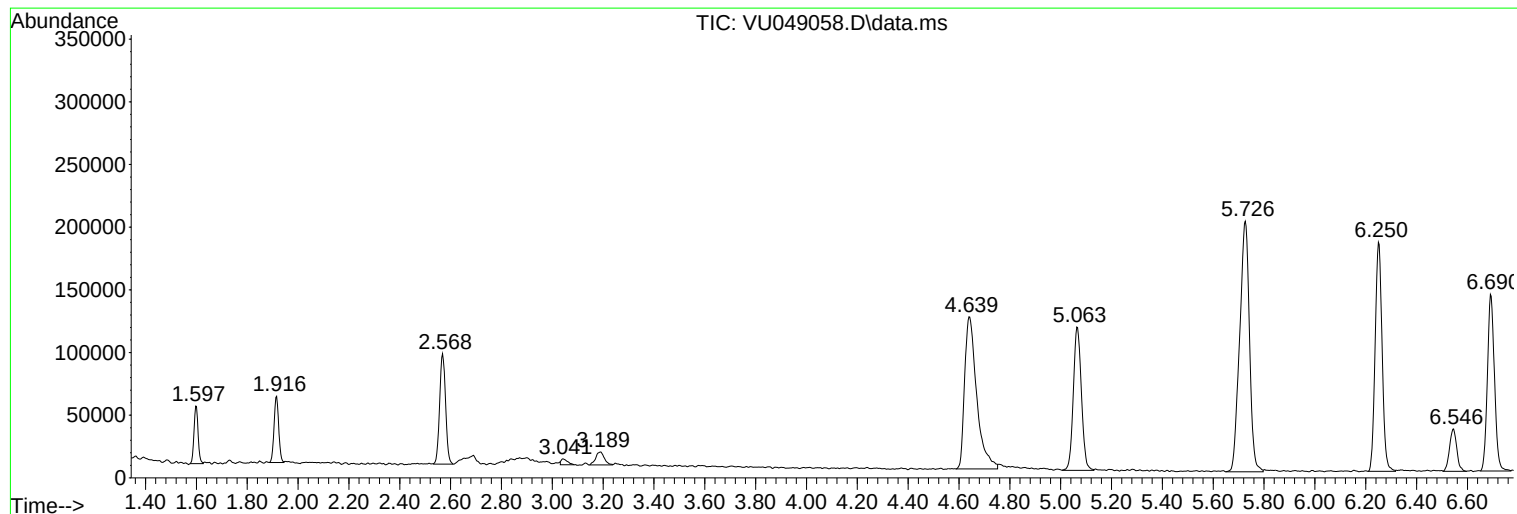

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049058.D
Acq On : 11 Jun 2022 17:33
Operator : SY/MD
Sample : N3277-04 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049058.D
Acq On : 11 Jun 2022 17:33
Operator : SY/MD
Sample : N3277-04 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc