

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049068.D
 Acq On : 11 Jun 2022 21:30
 Operator : SY/MD
 Sample : N3278-05 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BD2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049068.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rVB	42660	47402	5.87%	1.017%
2	1.916	166	179	192	rBV	50501	65668	8.13%	1.409%
3	2.568	370	382	396	rVB	80370	130139	16.11%	2.793%
4	3.186	563	574	588	rBV3	9055	20102	2.49%	0.431%
5	4.636	1007	1025	1057	rBV3	95905	339242	41.99%	7.281%
6	5.064	1144	1158	1181	rBV	103742	228217	28.25%	4.898%
7	5.726	1340	1364	1387	rBV2	188753	505502	62.56%	10.850%
8	6.250	1514	1527	1547	rBV	166565	324577	40.17%	6.967%
9	6.543	1605	1618	1628	rBV10	3425	8102	1.00%	0.174%
10	6.694	1652	1665	1688	rVB	128345	256726	31.77%	5.510%
11	7.565	1925	1936	1953	rVB2	49410	90368	11.18%	1.940%
12	7.899	2024	2040	2062	rBV	203532	358688	44.39%	7.699%
13	8.182	2114	2128	2143	rBV3	31958	57779	7.15%	1.240%
14	8.555	2232	2244	2257	rBV3	39478	65950	8.16%	1.416%
15	8.639	2257	2270	2311	rBV3	358605	807985	100.00%	17.342%
16	9.417	2499	2512	2540	rBV	245866	424569	52.55%	9.113%
17	10.758	2916	2929	2941	rBV2	123502	202943	25.12%	4.356%
18	11.812	3245	3257	3277	rBV	224174	366556	45.37%	7.868%
19	12.192	3363	3375	3390	rBV	223097	358488	44.37%	7.695%




Sum of corrected areas: 4659003

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049068.D
Acq On : 11 Jun 2022 21:30
Operator : SY/MD
Sample : N3278-05 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

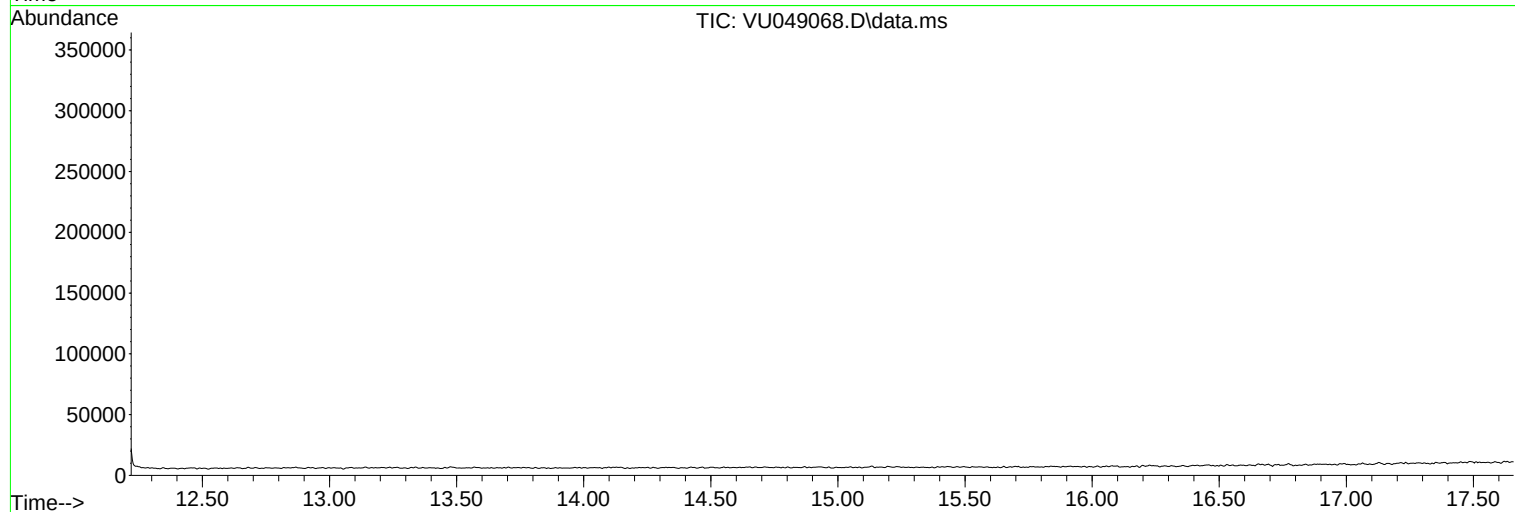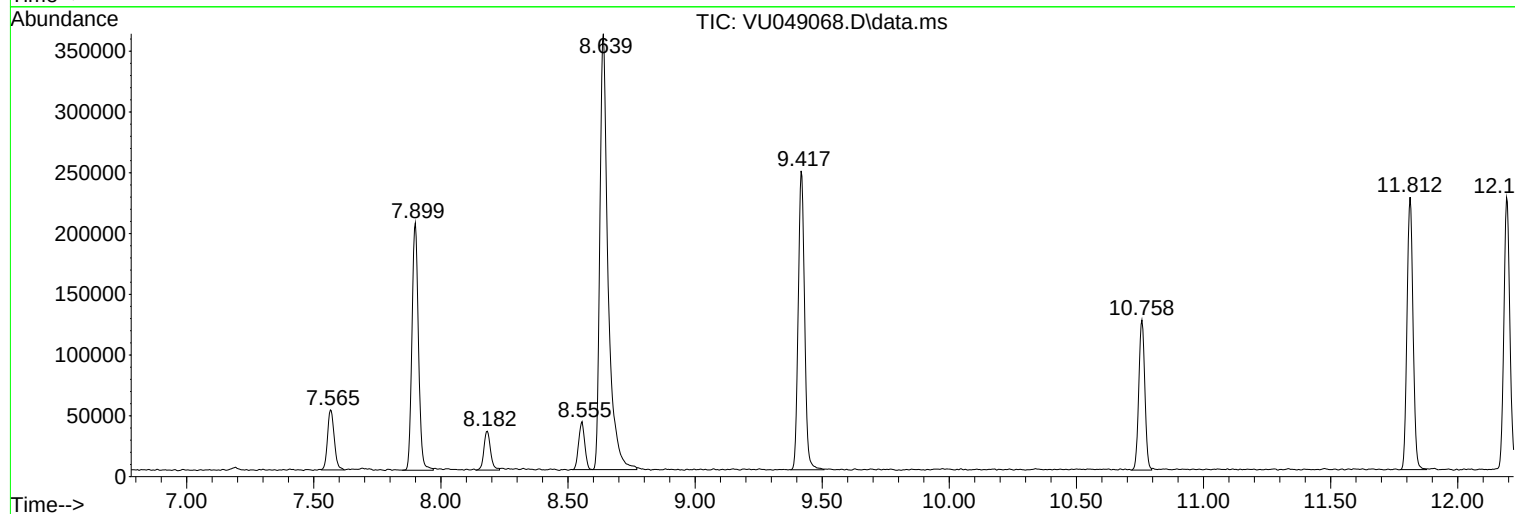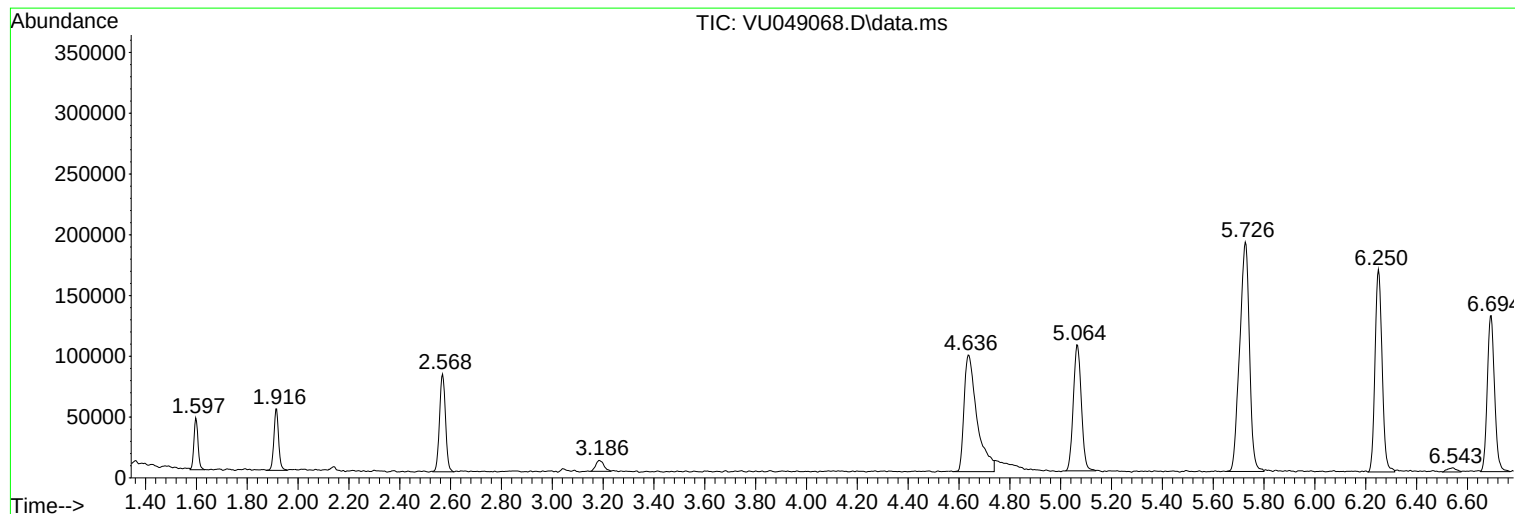

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049068.D
Acq On : 11 Jun 2022 21:30
Operator : SY/MD
Sample : N3278-05 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049068.D
Acq On : 11 Jun 2022 21:30
Operator : SY/MD
Sample : N3278-05 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc