

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049069.D
 Acq On : 11 Jun 2022 21:54
 Operator : SY/MD
 Sample : N3277-05 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BA4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049069.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	93	rVB	42012	47431	3.38%	0.772%
2	1.912	170	178	196	rVB	51588	66074	4.71%	1.076%
3	2.568	368	382	397	rVB2	79034	129116	9.20%	2.102%
4	3.189	560	575	587	rBV	19773	44302	3.16%	0.721%
5	4.636	1008	1025	1051	rBV3	115141	367819	26.21%	5.989%
6	5.067	1143	1159	1176	rBV2	103018	228523	16.29%	3.721%
7	5.726	1340	1364	1387	rBV2	187590	506414	36.09%	8.245%
8	6.250	1514	1527	1545	rBV	171239	326277	23.25%	5.312%
9	6.542	1600	1618	1643	rBV	745076	1403094	100.00%	22.845%
10	6.694	1652	1665	1685	rVB	129393	252101	17.97%	4.105%
11	7.568	1924	1937	1955	rBV	50701	90649	6.46%	1.476%
12	7.899	2027	2040	2064	rBV	204152	357189	25.46%	5.816%
13	8.182	2116	2128	2138	rBV3	31996	54605	3.89%	0.889%
14	8.552	2233	2243	2257	rBV2	19352	32569	2.32%	0.530%
15	8.639	2257	2270	2303	rBV2	353370	827344	58.97%	13.471%
16	9.417	2500	2512	2533	rBV	258368	446289	31.81%	7.266%
17	10.758	2916	2929	2946	rBV	125948	208772	14.88%	3.399%
18	11.812	3245	3257	3271	rBV	236749	383487	27.33%	6.244%
19	12.195	3364	3376	3393	rBV	223217	369779	26.35%	6.021%




Sum of corrected areas: 6141834

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049069.D
Acq On : 11 Jun 2022 21:54
Operator : SY/MD
Sample : N3277-05 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

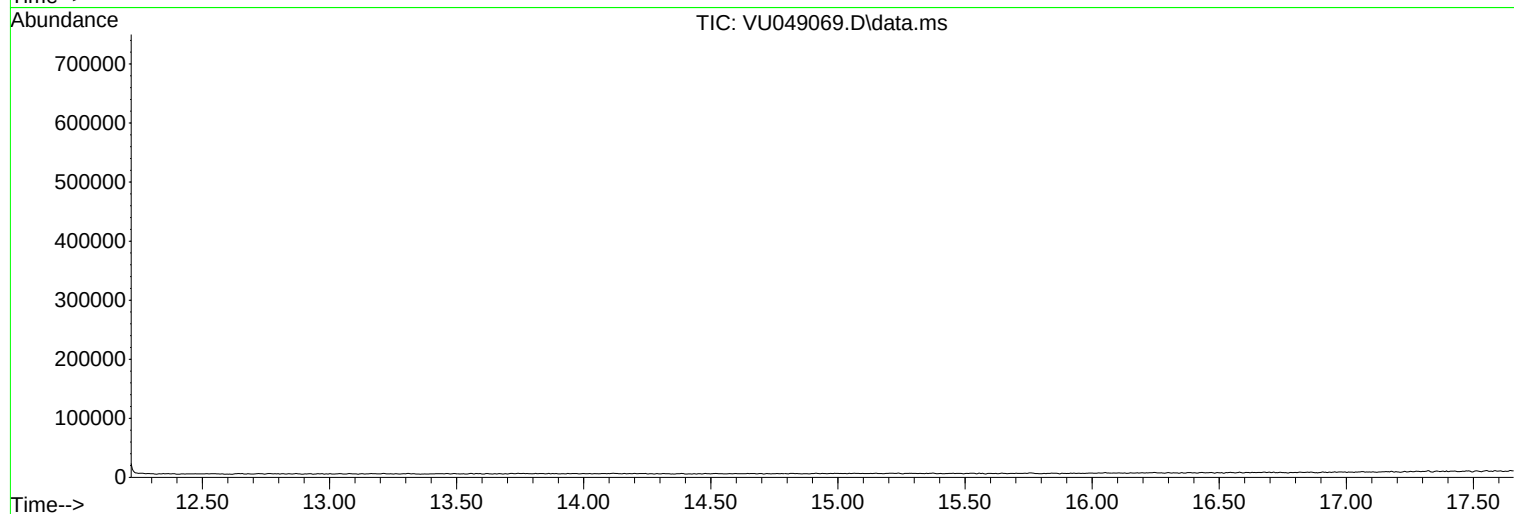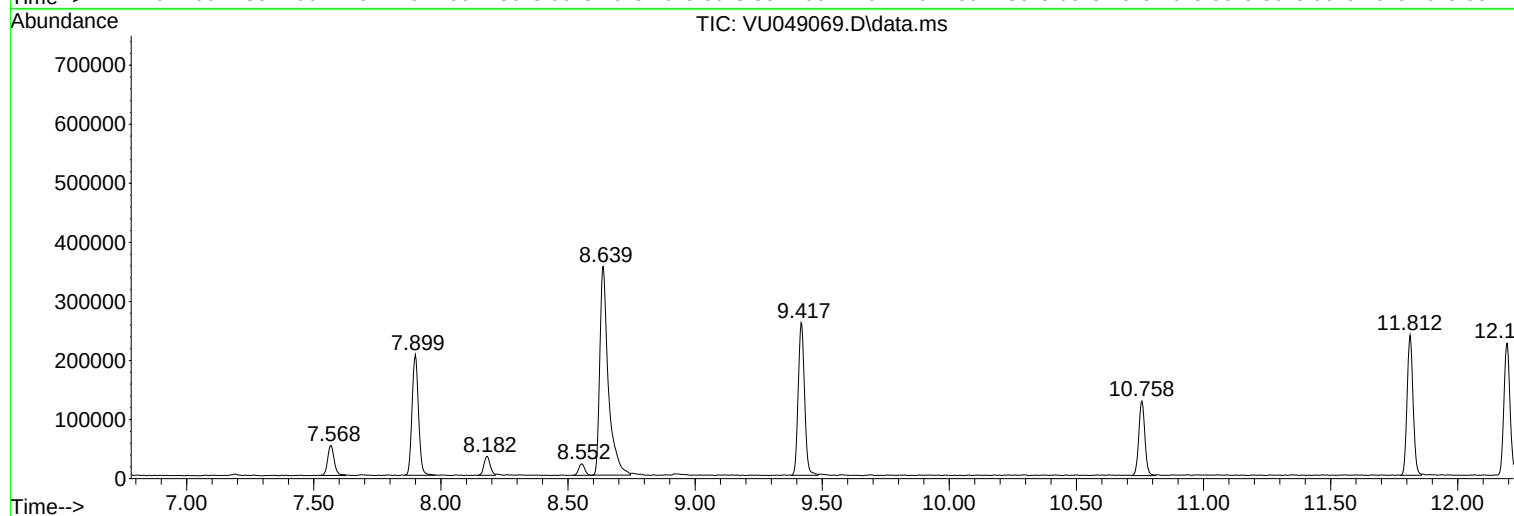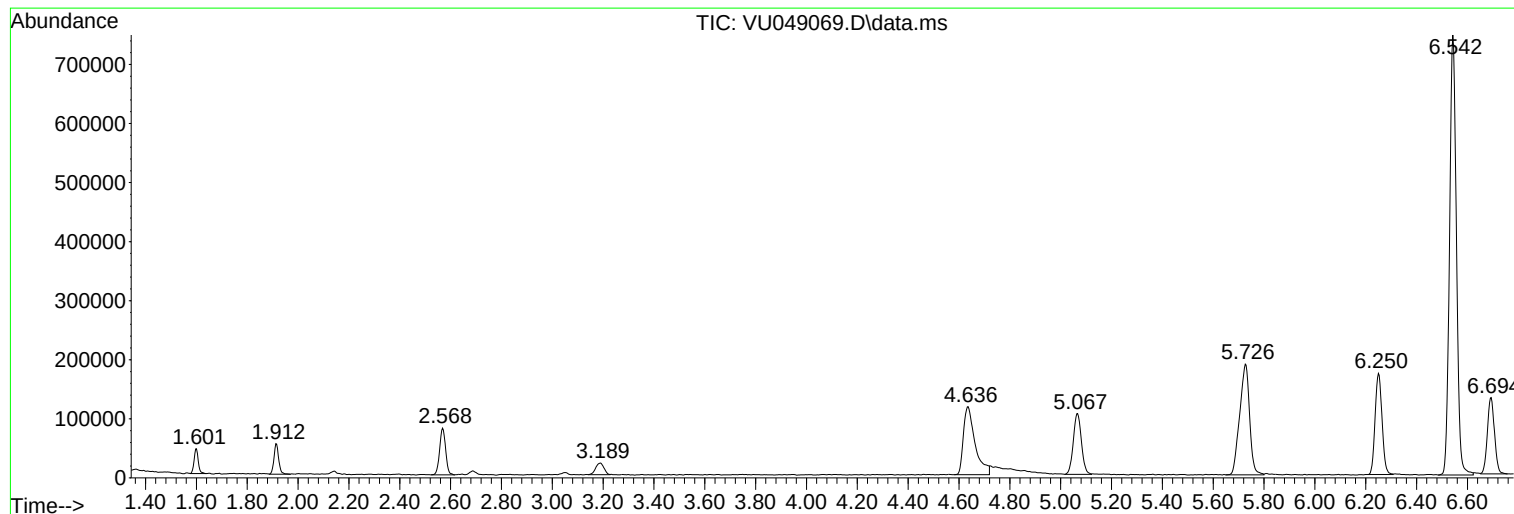

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049069.D
Acq On : 11 Jun 2022 21:54
Operator : SY/MD
Sample : N3277-05 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049069.D
Acq On : 11 Jun 2022 21:54
Operator : SY/MD
Sample : N3277-05 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc