

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049071.D
 Acq On : 11 Jun 2022 22:41
 Operator : SY/MD
 Sample : N3277-11 2000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BB0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	70	80	90	rVB	42002	46355	1.20%	0.512%
2	1.916	165	179	191	rVB	49391	64612	1.67%	0.714%
3	2.568	368	382	396	rBV2	80789	131061	3.40%	1.449%
4	3.186	560	574	587	rBV	20262	42025	1.09%	0.464%
5	4.639	1011	1026	1062	rBV3	114749	424891	11.01%	4.696%
6	5.067	1144	1159	1188	rBV2	107850	243101	6.30%	2.687%
7	5.726	1343	1364	1388	rBV2	202782	535033	13.87%	5.913%
8	6.250	1511	1527	1547	rBV	178523	343712	8.91%	3.799%
9	6.543	1603	1618	1651	rBV	2048722	3858519	100.00%	42.645%
10	6.690	1651	1664	1689	rVB	141841	289006	7.49%	3.194%
11	7.565	1925	1936	1953	rBV2	53877	95320	2.47%	1.053%
12	7.899	2027	2040	2060	rBV	217350	381111	9.88%	4.212%
13	8.182	2116	2128	2140	rBV	35389	60780	1.58%	0.672%
14	8.552	2227	2243	2257	rBV	176378	297911	7.72%	3.293%
15	8.639	2258	2270	2313	rVB2	372481	840214	21.78%	9.286%
16	9.417	2498	2512	2537	rBV	250831	428353	11.10%	4.734%
17	10.758	2917	2929	2943	rBV2	123739	200347	5.19%	2.214%
18	11.812	3246	3257	3275	rBV	232924	378175	9.80%	4.180%
19	12.192	3364	3375	3395	rBV	233379	387473	10.04%	4.282%




Sum of corrected areas: 9047999

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049071.D
Acq On : 11 Jun 2022 22:41
Operator : SY/MD
Sample : N3277-11 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

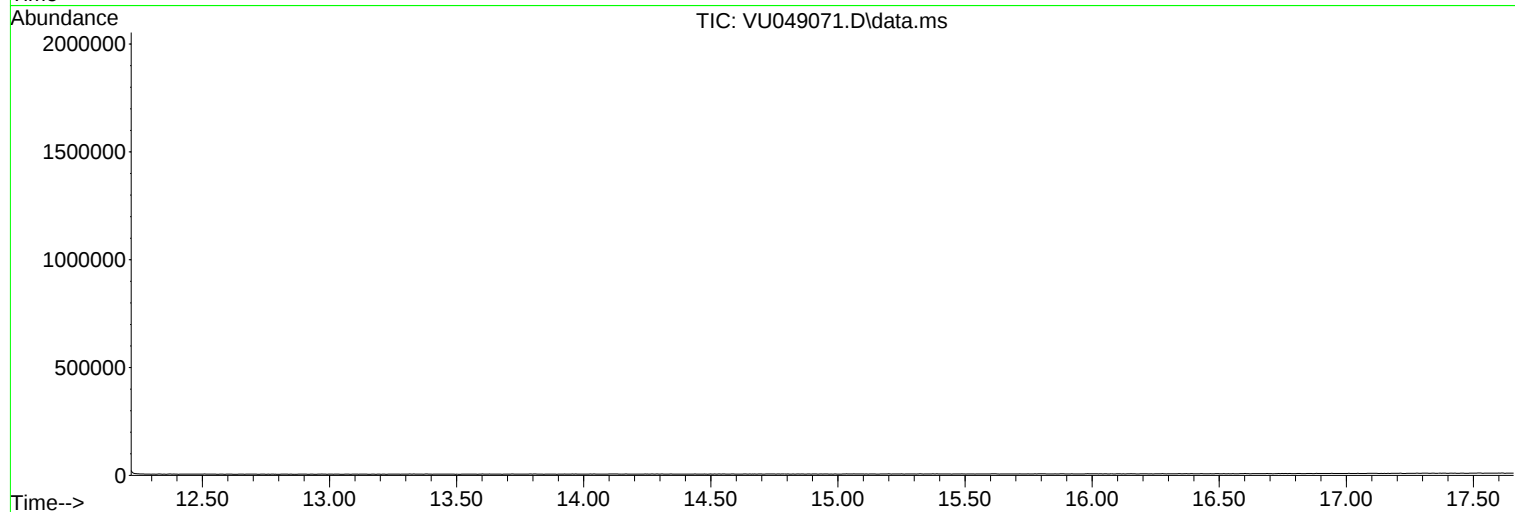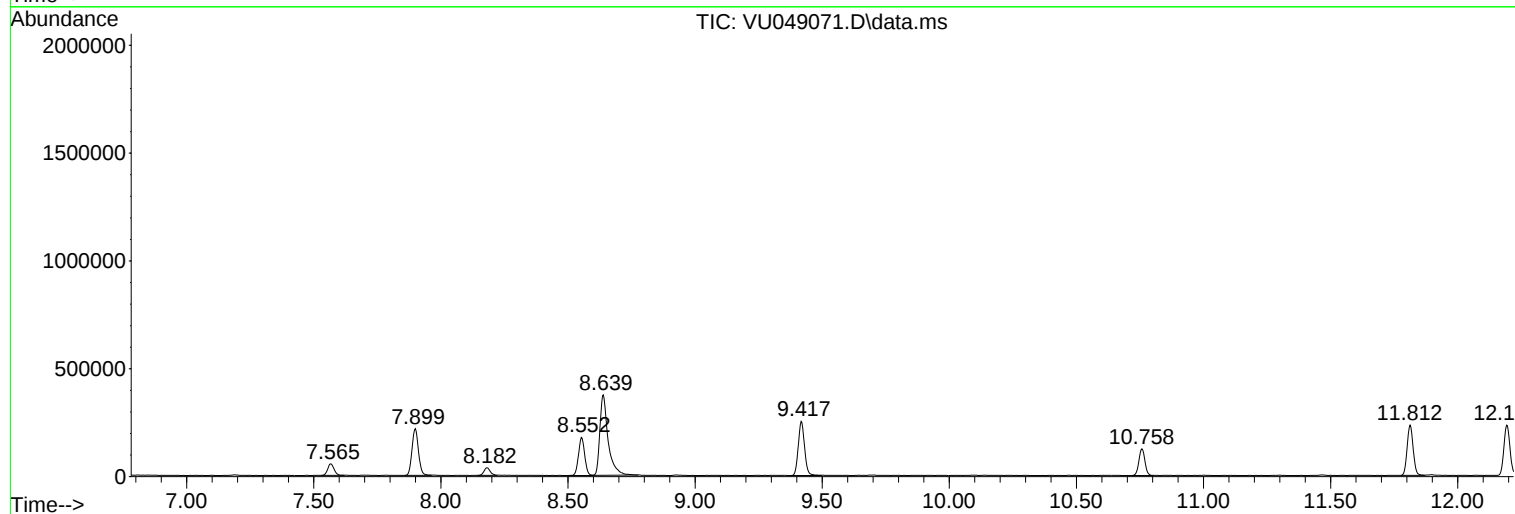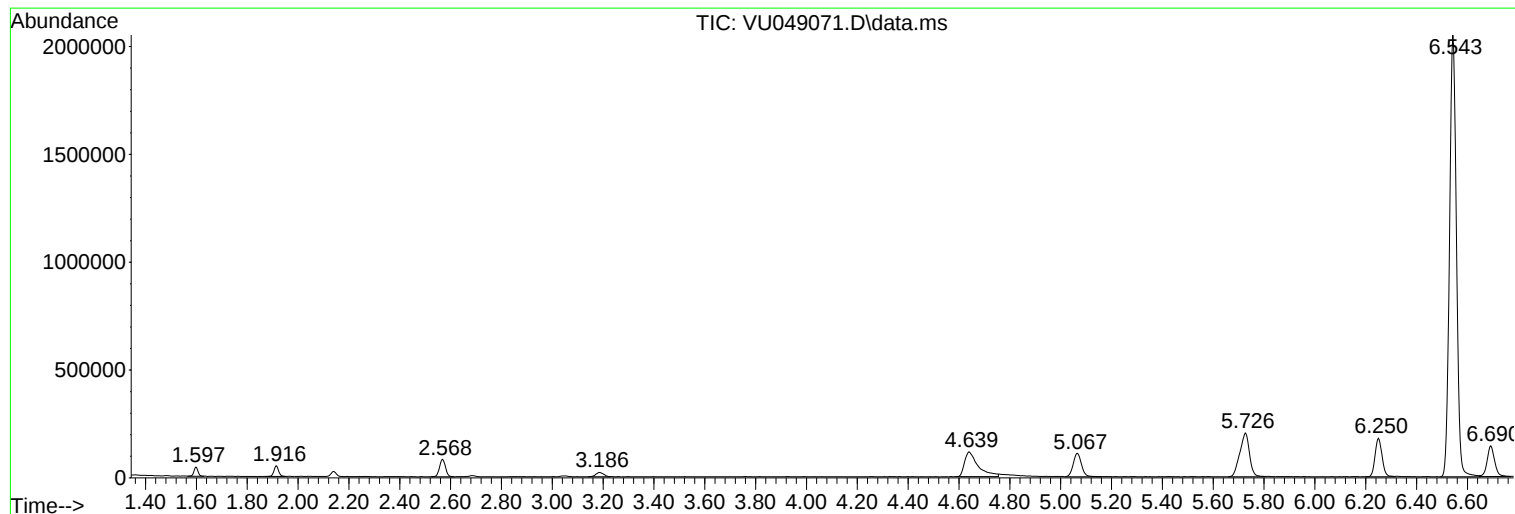

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049071.D
Acq On : 11 Jun 2022 22:41
Operator : SY/MD
Sample : N3277-11 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049071.D
Acq On : 11 Jun 2022 22:41
Operator : SY/MD
Sample : N3277-11 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc