

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049072.D
 Acq On : 11 Jun 2022 23:05
 Operator : SY/MD
 Sample : N3277-13 2000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BB2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	89	rBV	41106	45655	2.09%	0.639%
2	1.916	170	179	188	rBV	50082	63581	2.92%	0.889%
3	2.568	370	382	400	rVB	74036	124051	5.69%	1.735%
4	3.186	555	574	591	rBV	23333	53065	2.43%	0.742%
5	4.639	1009	1026	1067	rBV4	132745	484547	22.22%	6.777%
6	5.067	1142	1159	1175	rBV	103100	225987	10.36%	3.161%
7	5.726	1344	1364	1386	rBV2	187147	498516	22.86%	6.972%
8	6.250	1510	1527	1546	rBV2	174298	329084	15.09%	4.602%
9	6.543	1599	1618	1645	rBV	1164671	2180530	100.00%	30.496%
10	6.694	1652	1665	1685	rVB	137380	272627	12.50%	3.813%
11	7.565	1925	1936	1953	rBV	51108	90150	4.13%	1.261%
12	7.899	2027	2040	2055	rBV	208781	363005	16.65%	5.077%
13	8.182	2116	2128	2144	rBV2	33445	58032	2.66%	0.812%
14	8.552	2231	2243	2258	rBV	128276	219546	10.07%	3.071%
15	8.639	2258	2270	2302	rBV2	377389	808499	37.08%	11.307%
16	9.417	2500	2512	2528	rBV	247021	412168	18.90%	5.764%
17	10.758	2914	2929	2941	rBV	122259	196425	9.01%	2.747%
18	11.812	3245	3257	3277	rBV	223581	364154	16.70%	5.093%
19	12.195	3364	3376	3392	rBV	219369	360539	16.53%	5.042%




Sum of corrected areas: 7150161

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049072.D
Acq On : 11 Jun 2022 23:05
Operator : SY/MD
Sample : N3277-13 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

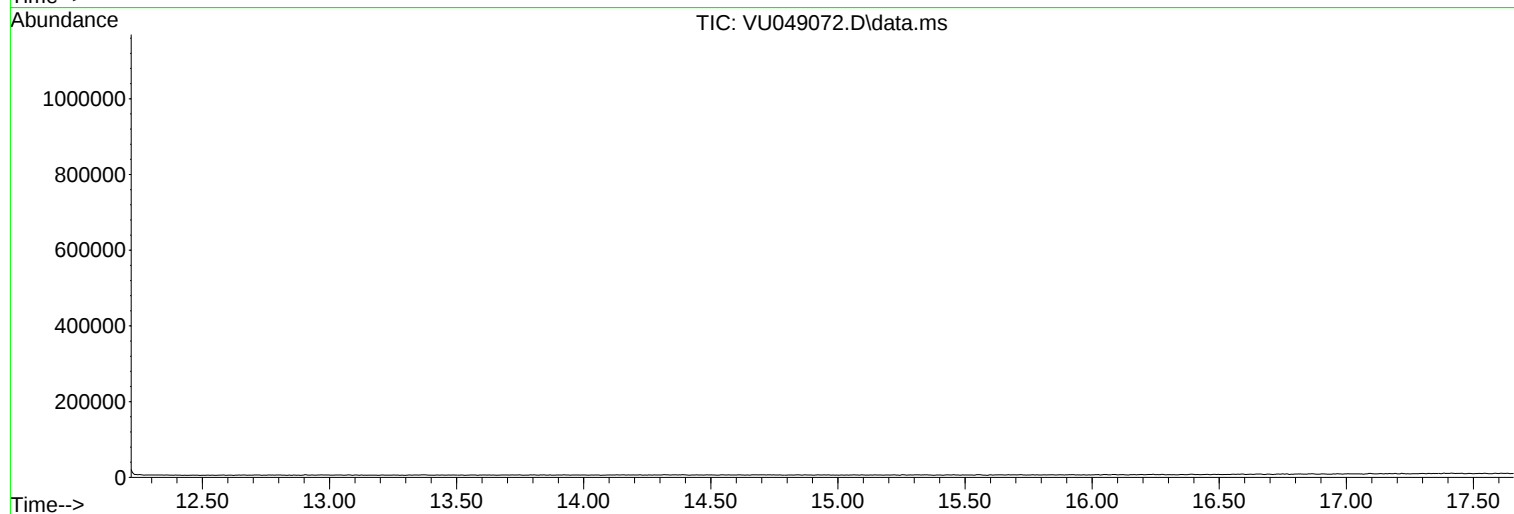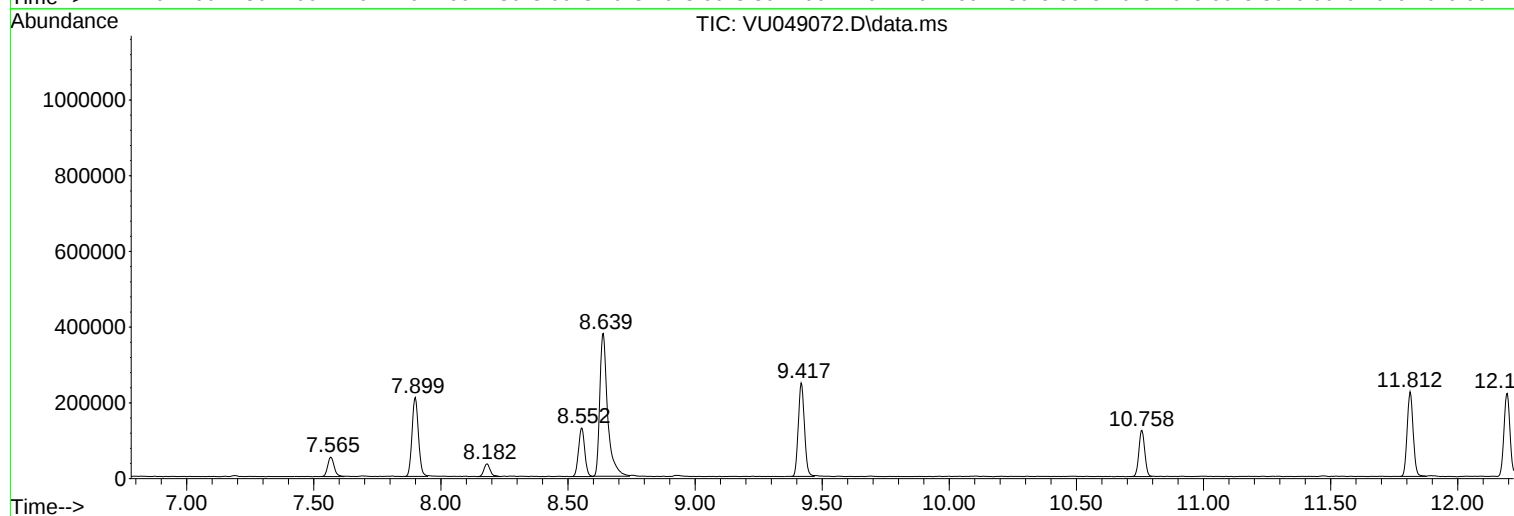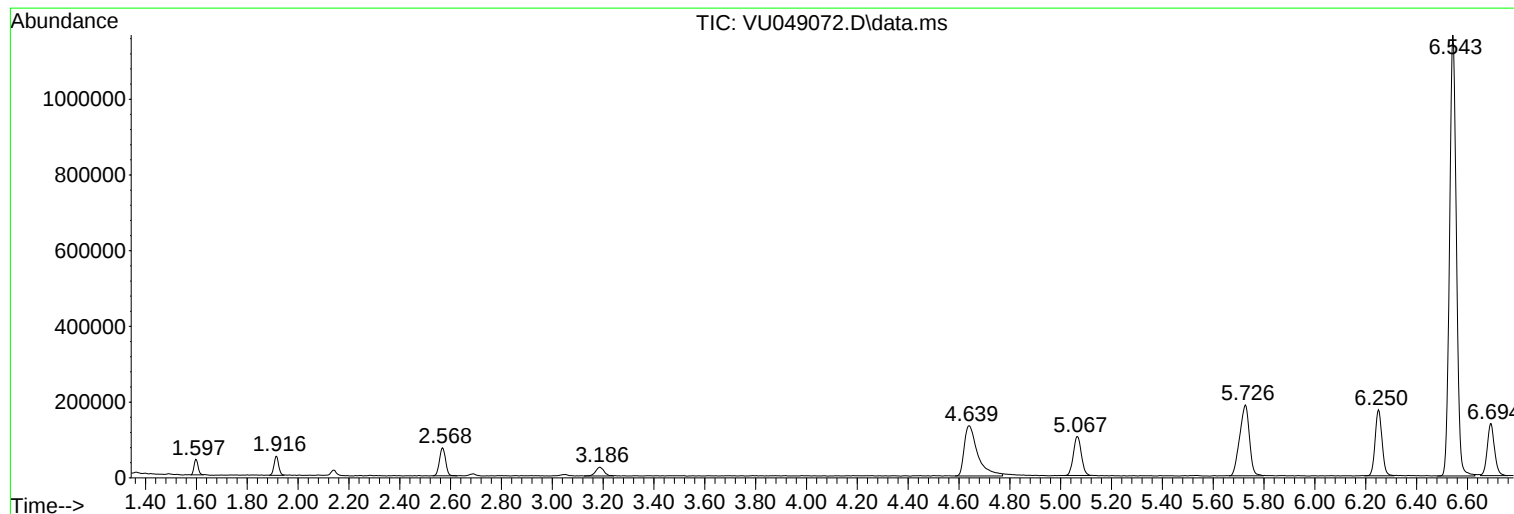

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049072.D
Acq On : 11 Jun 2022 23:05
Operator : SY/MD
Sample : N3277-13 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049072.D
Acq On : 11 Jun 2022 23:05
Operator : SY/MD
Sample : N3277-13 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc