

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049073.D
 Acq On : 11 Jun 2022 23:29
 Operator : SY/MD
 Sample : N3277-14 2000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BB3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049073.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	68	80	90	rBV	42486	48923	5.25%	0.870%
2	1.916	170	179	189	rBV	50061	64720	6.95%	1.151%
3	2.141	239	249	260	rVB2	8737	12033	1.29%	0.214%
4	2.568	371	382	398	rVB	77944	127799	13.72%	2.274%
5	3.189	559	575	592	rBV	19325	45604	4.90%	0.811%
6	4.639	1009	1026	1071	rBV3	115195	436030	46.81%	7.757%
7	5.063	1141	1158	1175	rBV	103438	228577	24.54%	4.066%
8	5.726	1339	1364	1382	rBV2	188609	501041	53.79%	8.913%
9	6.250	1511	1527	1548	rBV	161199	313160	33.62%	5.571%
10	6.542	1601	1618	1646	rBV	488842	931466	100.00%	16.571%
11	6.690	1651	1664	1688	rVB	127344	253406	27.21%	4.508%
12	7.568	1925	1937	1953	rBV2	48169	86661	9.30%	1.542%
13	7.899	2027	2040	2058	rBV	193240	339552	36.45%	6.041%
14	8.182	2116	2128	2144	rBV2	32137	56812	6.10%	1.011%
15	8.552	2231	2243	2257	rBV2	61604	102818	11.04%	1.829%
16	8.639	2257	2270	2307	rBV2	342332	776605	83.37%	13.816%
17	9.417	2500	2512	2534	rBV	238676	398714	42.80%	7.093%
18	10.758	2916	2929	2943	rBV	118681	190149	20.41%	3.383%
19	11.812	3241	3257	3272	rBV	213466	351302	37.71%	6.250%
20	12.192	3363	3375	3391	rBV	214537	355776	38.20%	6.329%




Sum of corrected areas: 5621148

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049073.D
Acq On : 11 Jun 2022 23:29
Operator : SY/MD
Sample : N3277-14 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

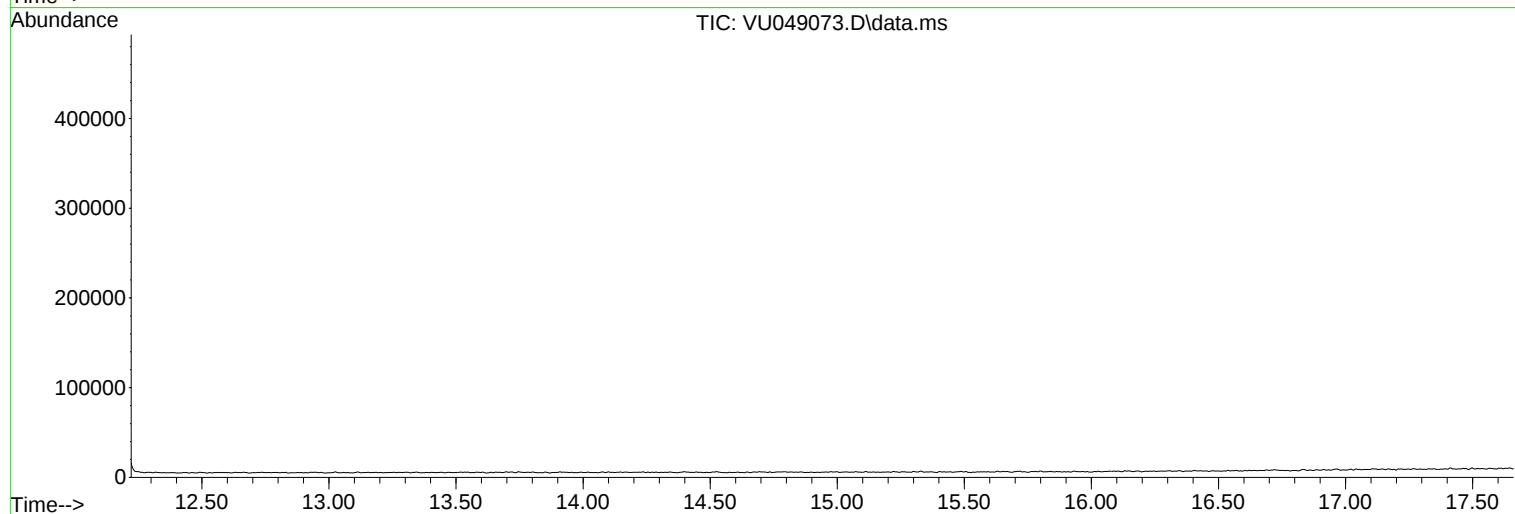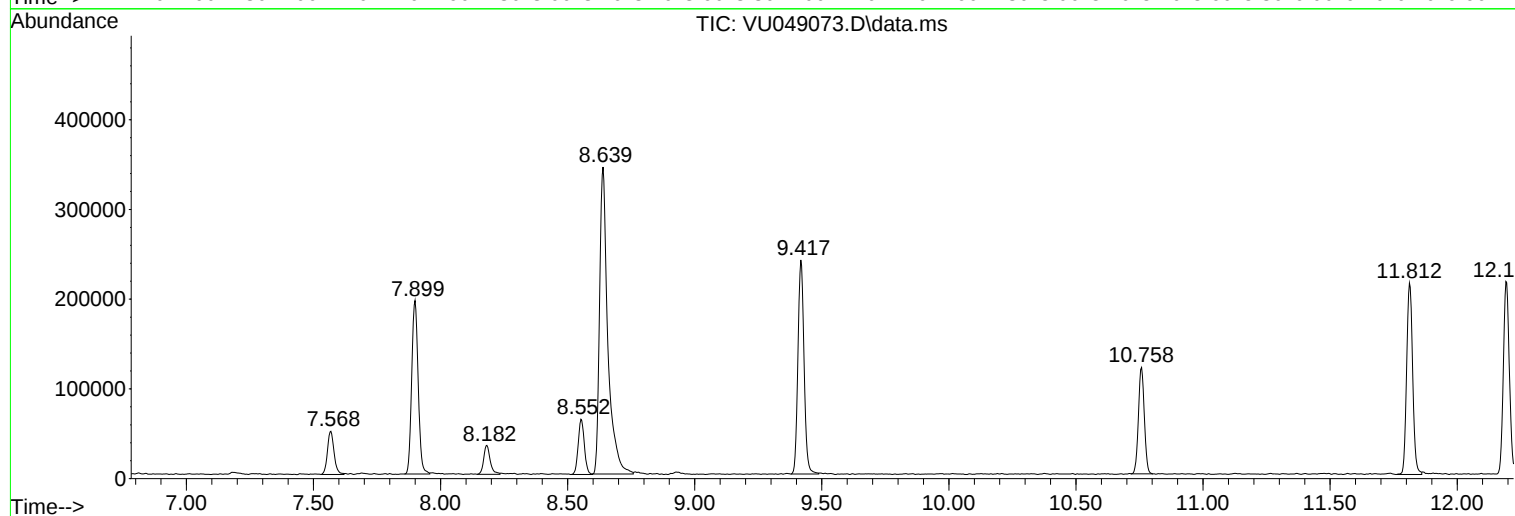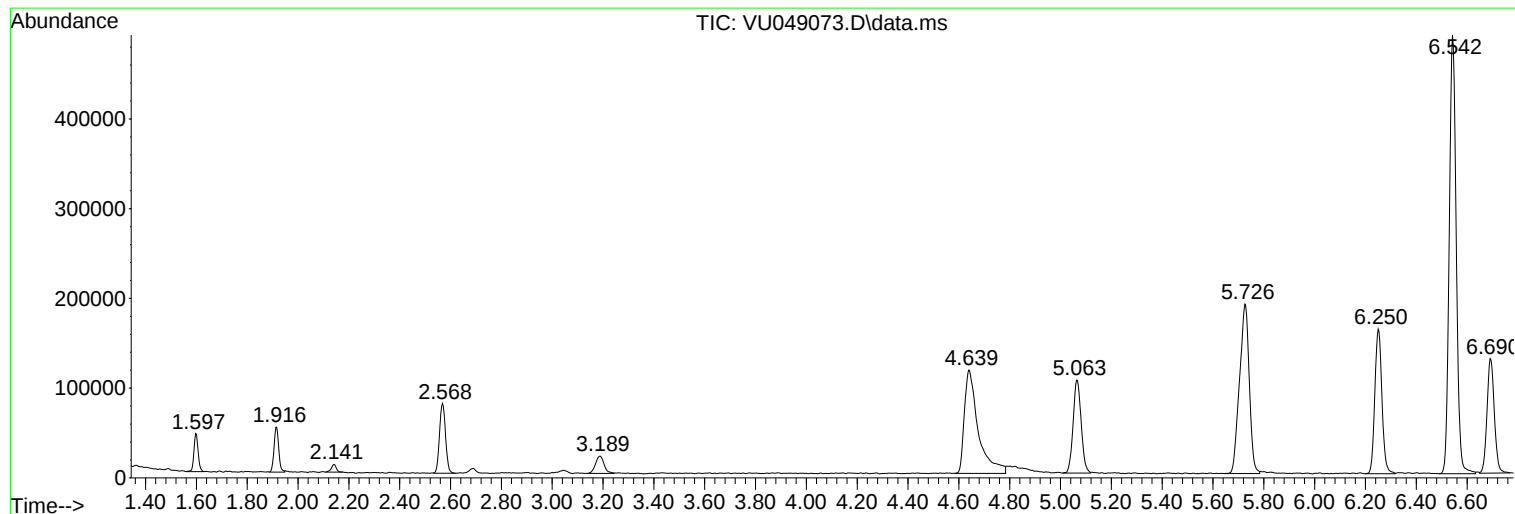

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049073.D
Acq On : 11 Jun 2022 23:29
Operator : SY/MD
Sample : N3277-14 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049073.D
Acq On : 11 Jun 2022 23:29
Operator : SY/MD
Sample : N3277-14 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc