

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049074.D
 Acq On : 11 Jun 2022 23:53
 Operator : SY/MD
 Sample : N3277-18 2000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rVB	46228	50057	6.09%	0.975%
2	1.916	170	179	190	rBV	51638	66088	8.04%	1.287%
3	2.568	369	382	395	rBV	82873	133957	16.29%	2.608%
4	2.687	411	419	431	rVB2	5906	9637	1.17%	0.188%
5	3.051	522	532	542	rVB5	4040	8317	1.01%	0.162%
6	3.186	558	574	594	rBV	19135	44850	5.45%	0.873%
7	4.639	1009	1026	1057	rBV3	124087	438003	53.26%	8.528%
8	5.063	1143	1158	1179	rBV	109399	242275	29.46%	4.717%
9	5.726	1334	1364	1389	rBV4	195857	527930	64.19%	10.279%
10	6.250	1512	1527	1552	rBV	161712	307159	37.35%	5.980%
11	6.543	1604	1618	1639	rBV	203780	385770	46.91%	7.511%
12	6.694	1650	1665	1690	rBV2	131150	263641	32.06%	5.133%
13	7.568	1923	1937	1955	rBV	48294	87856	10.68%	1.711%
14	7.899	2026	2040	2057	rBV	205656	358974	43.65%	6.989%
15	8.182	2117	2128	2141	rBV3	32881	57355	6.97%	1.117%
16	8.552	2232	2243	2253	rBV3	11596	20087	2.44%	0.391%
17	8.639	2256	2270	2308	rBV2	373662	822402	100.00%	16.012%
18	9.417	2500	2512	2528	rBV	228792	388838	47.28%	7.571%
19	10.758	2913	2929	2944	rBV	124869	203622	24.76%	3.965%
20	11.812	3244	3257	3274	rBV2	212351	347099	42.21%	6.758%
21	12.195	3359	3376	3391	rBV	227427	372111	45.25%	7.245%




Sum of corrected areas: 5136028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049074.D
Acq On : 11 Jun 2022 23:53
Operator : SY/MD
Sample : N3277-18 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

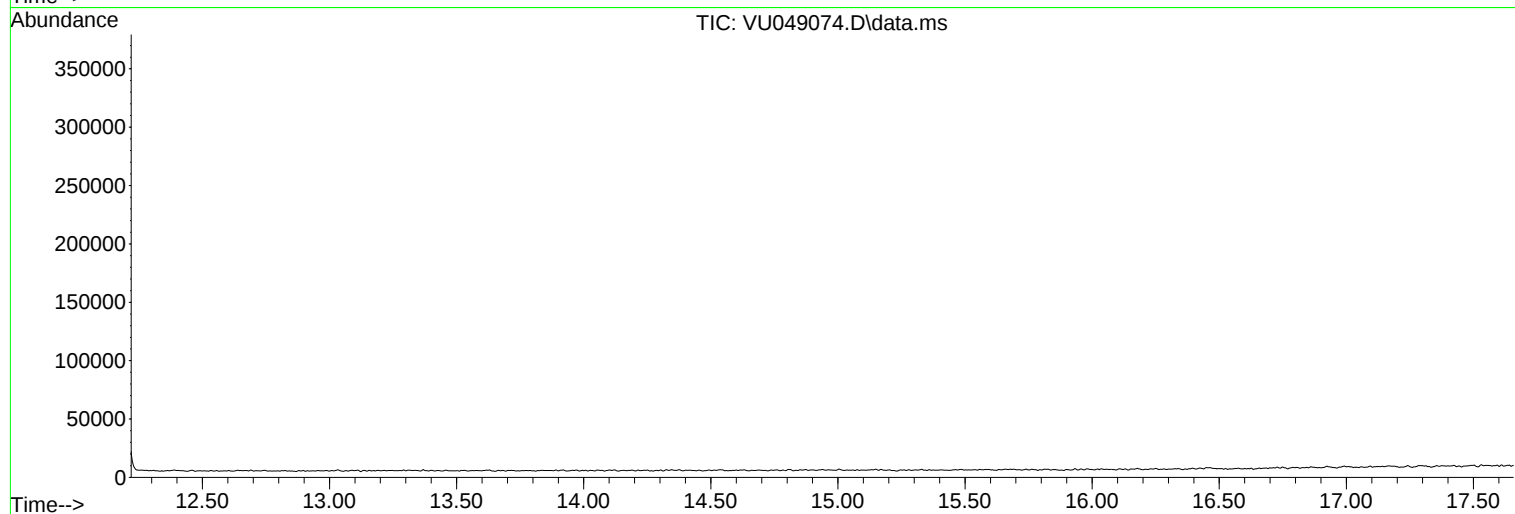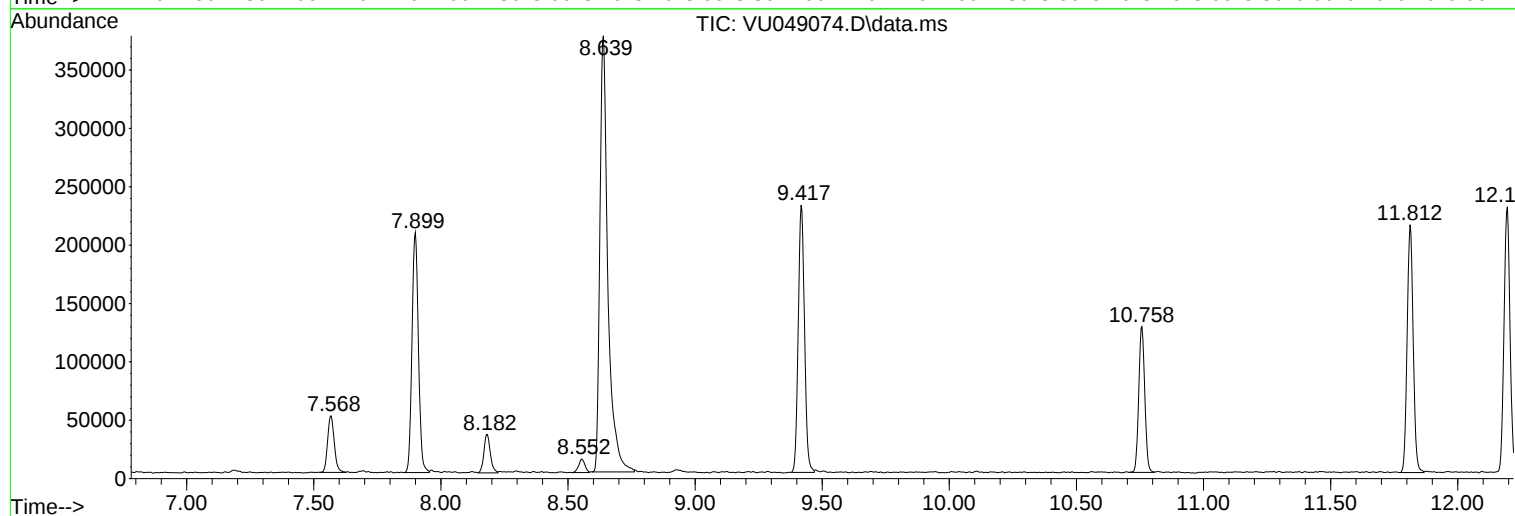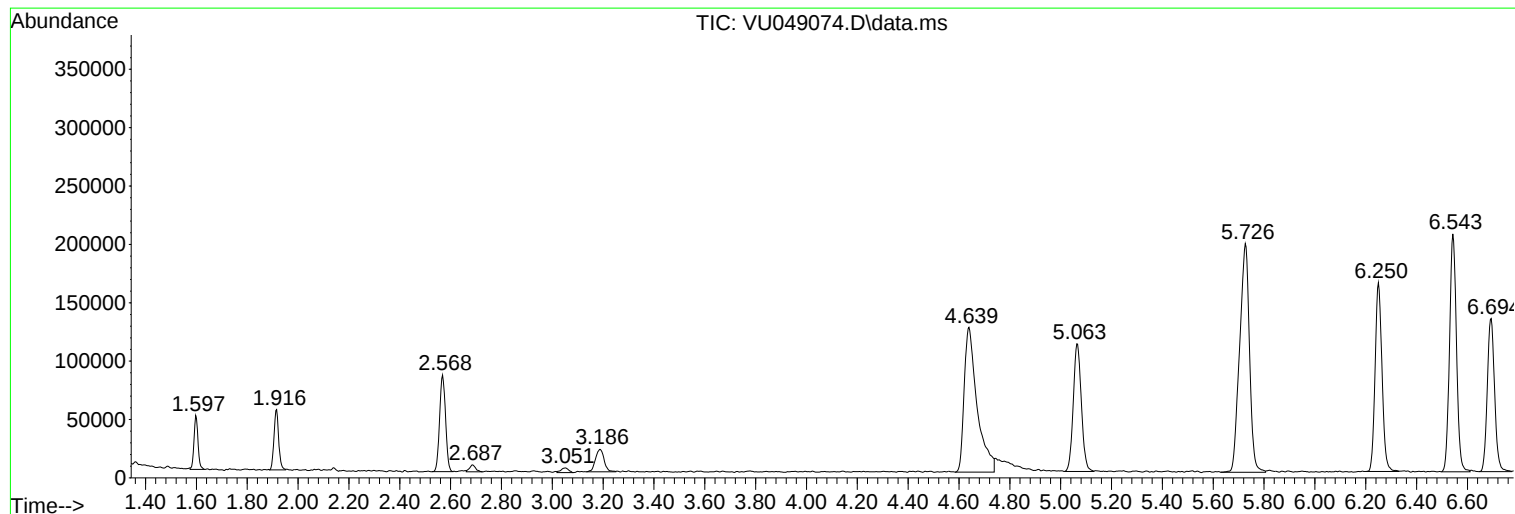

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049074.D
Acq On : 11 Jun 2022 23:53
Operator : SY/MD
Sample : N3277-18 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049074.D
Acq On : 11 Jun 2022 23:53
Operator : SY/MD
Sample : N3277-18 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc