

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049075.D
 Acq On : 12 Jun 2022 00:16
 Operator : SY/MD
 Sample : N3277-19 2000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	92	rVB	42622	46682	5.95%	0.954%
2	1.915	170	179	189	rBV	53109	64595	8.23%	1.321%
3	2.568	370	382	399	rVB	78700	128816	16.42%	2.634%
4	2.684	410	418	429	rVB4	5387	8988	1.15%	0.184%
5	3.186	560	574	591	rBV2	16181	35625	4.54%	0.728%
6	4.639	1011	1026	1060	rBV2	103326	356011	45.38%	7.278%
7	5.066	1142	1159	1180	rBV	101337	224141	28.57%	4.582%
8	5.726	1341	1364	1389	rBV2	186020	501371	63.91%	10.250%
9	6.250	1514	1527	1544	rBV	163776	313076	39.91%	6.401%
10	6.542	1603	1618	1635	rBV	198497	378926	48.31%	7.747%
11	6.693	1652	1665	1682	rBV	128034	252217	32.15%	5.156%
12	7.568	1923	1937	1951	rBV3	46880	86489	11.03%	1.768%
13	7.899	2026	2040	2060	rBV	191707	337950	43.08%	6.909%
14	8.179	2117	2127	2143	rBV	31250	53552	6.83%	1.095%
15	8.555	2232	2244	2254	rVB5	11088	18170	2.32%	0.371%
16	8.639	2254	2270	2304	rBV3	326465	784440	100.00%	16.037%
17	9.420	2500	2513	2531	rBV	230570	398998	50.86%	8.157%
18	10.758	2910	2929	2945	rBV	117678	195468	24.92%	3.996%
19	11.812	3245	3257	3277	rBV	217496	350678	44.70%	7.169%
20	12.195	3361	3376	3393	rBV	214894	355156	45.28%	7.261%




Sum of corrected areas: 4891349

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049075.D
Acq On : 12 Jun 2022 00:16
Operator : SY/MD
Sample : N3277-19 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

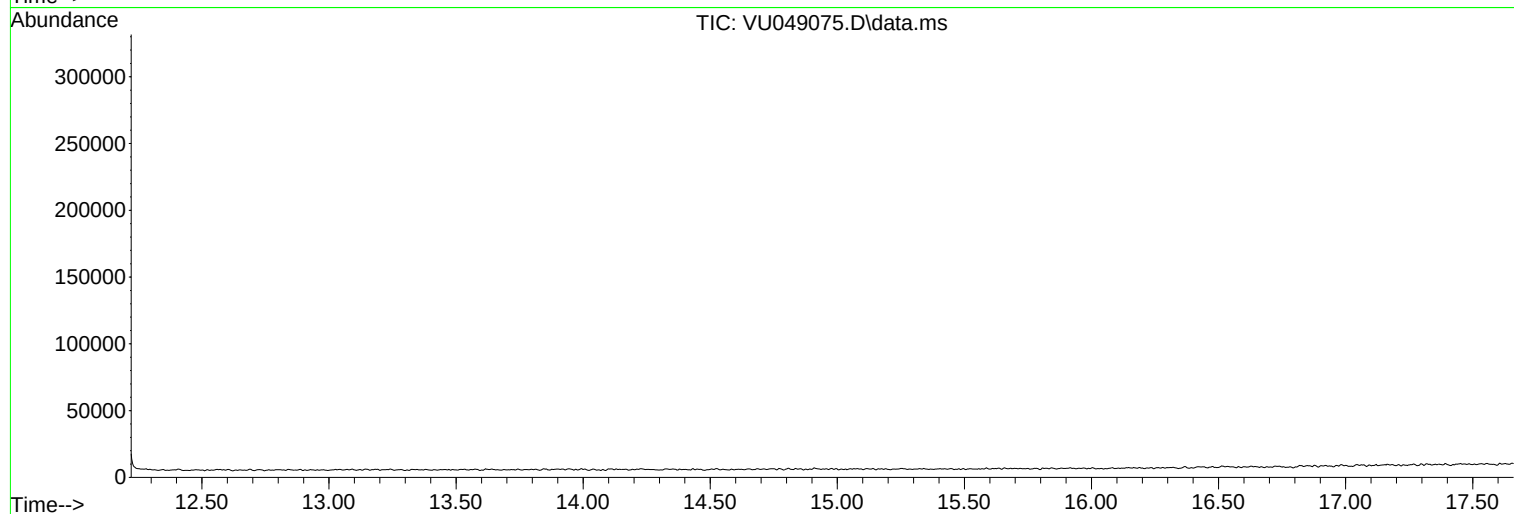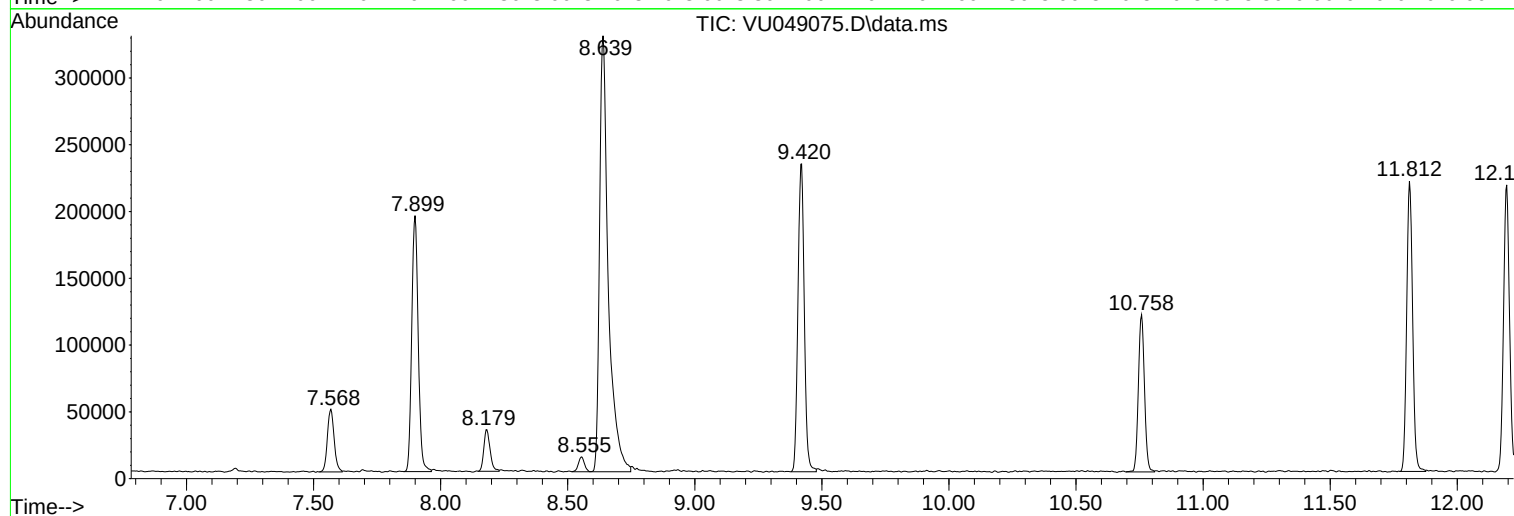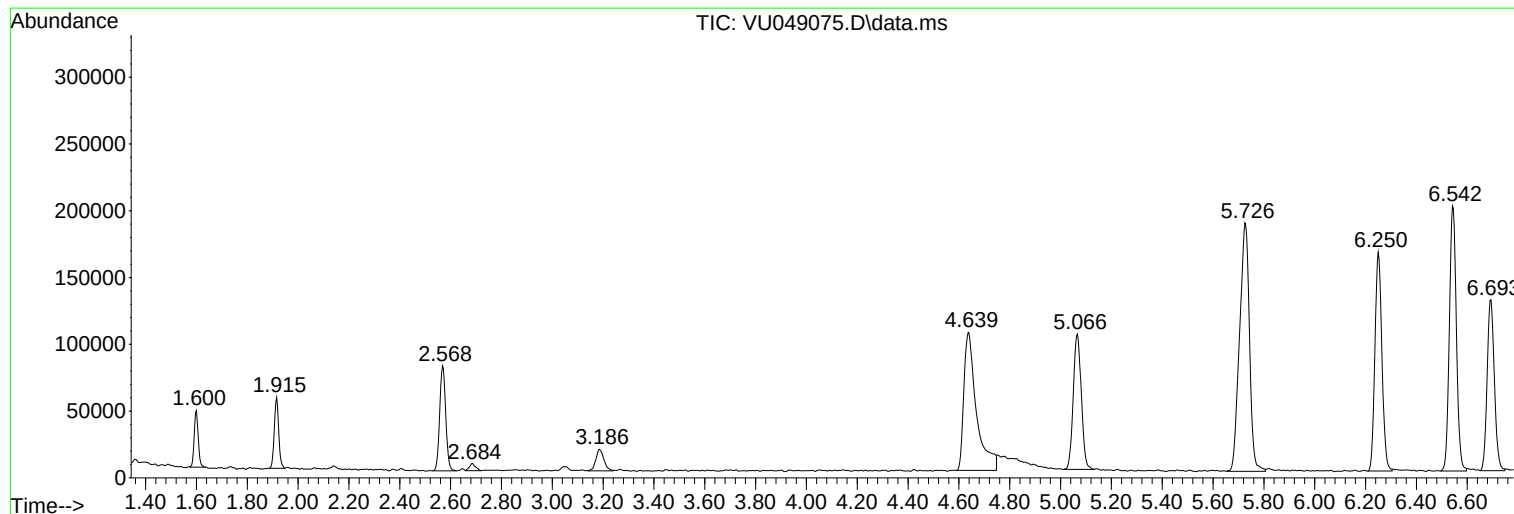

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049075.D
Acq On : 12 Jun 2022 00:16
Operator : SY/MD
Sample : N3277-19 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049075.D
Acq On : 12 Jun 2022 00:16
Operator : SY/MD
Sample : N3277-19 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------