

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049076.D
 Acq On : 12 Jun 2022 00:40
 Operator : SY/MD
 Sample : N3277-20 2000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	91	rVB	41716	47354	6.01%	1.015%
2	1.916	170	179	191	rVB	50279	65420	8.30%	1.402%
3	2.568	368	382	396	rBV	81058	129886	16.48%	2.783%
4	2.684	409	418	432	rVB5	5312	9536	1.21%	0.204%
5	3.189	560	575	591	rVB	21200	47936	6.08%	1.027%
6	4.642	1008	1027	1061	rBV2	122099	442985	56.21%	9.491%
7	5.063	1143	1158	1176	rBV2	105556	231902	29.42%	4.969%
8	5.726	1343	1364	1383	rBV2	186577	499173	63.34%	10.695%
9	6.250	1513	1527	1551	rBV	166653	320861	40.71%	6.875%
10	6.543	1607	1618	1631	rBV6	22275	43221	5.48%	0.926%
11	6.694	1650	1665	1685	rBV	127146	251620	31.93%	5.391%
12	7.568	1925	1937	1953	rBV2	48013	87113	11.05%	1.866%
13	7.899	2027	2040	2060	rBV	192558	336032	42.64%	7.200%
14	8.179	2117	2127	2142	rBV3	30590	52735	6.69%	1.130%
15	8.559	2235	2245	2253	rVB5	6339	10735	1.36%	0.230%
16	8.639	2256	2270	2301	rBV2	358804	788141	100.00%	16.886%
17	9.417	2500	2512	2533	rBV	237549	404303	51.30%	8.662%
18	10.758	2917	2929	2945	rBV	117036	193332	24.53%	4.142%
19	11.812	3245	3257	3274	rBV	216964	358136	45.44%	7.673%
20	12.192	3363	3375	3394	rBV	209556	346955	44.02%	7.434%




Sum of corrected areas: 4667376

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049076.D
Acq On : 12 Jun 2022 00:40
Operator : SY/MD
Sample : N3277-20 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

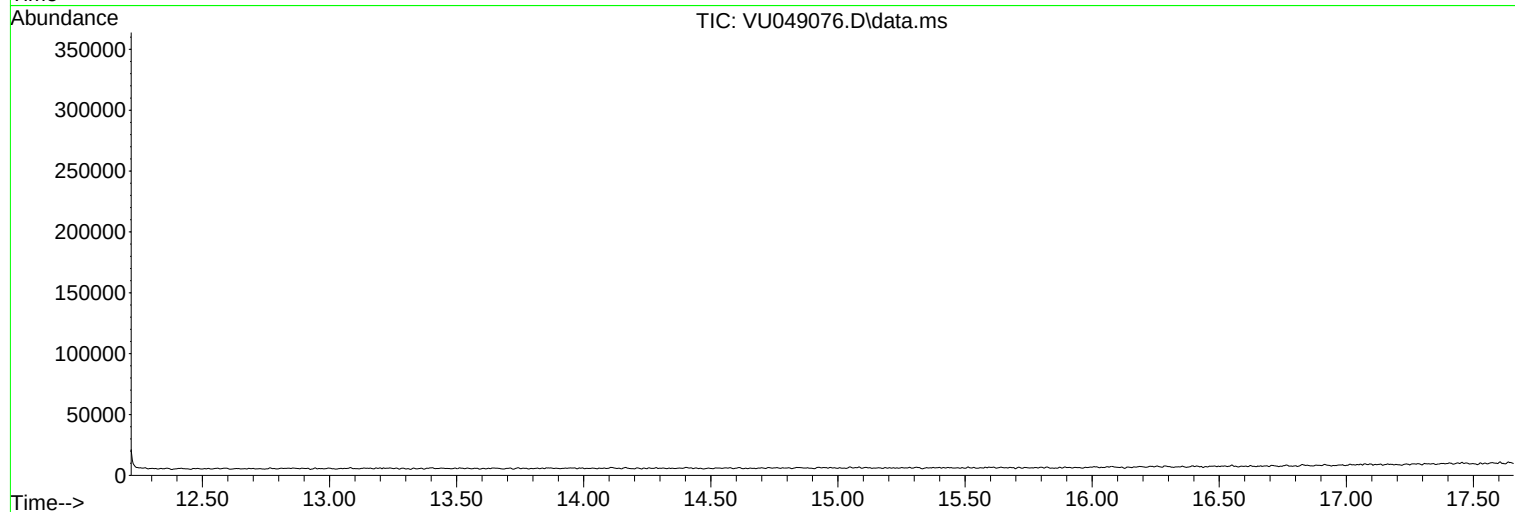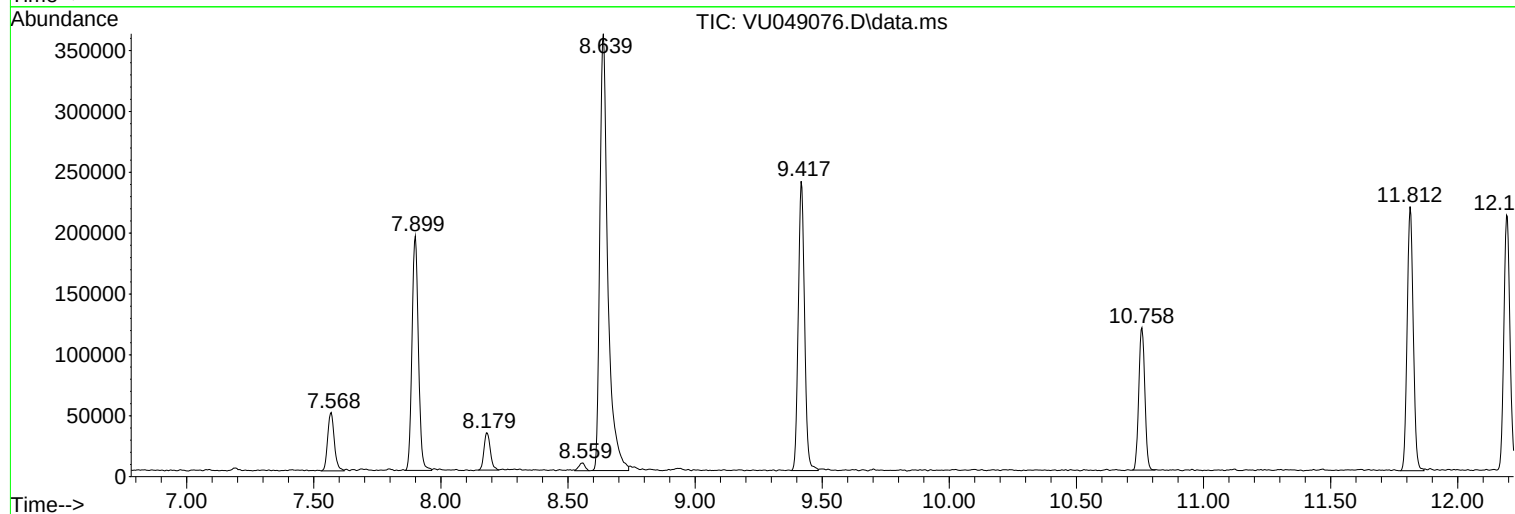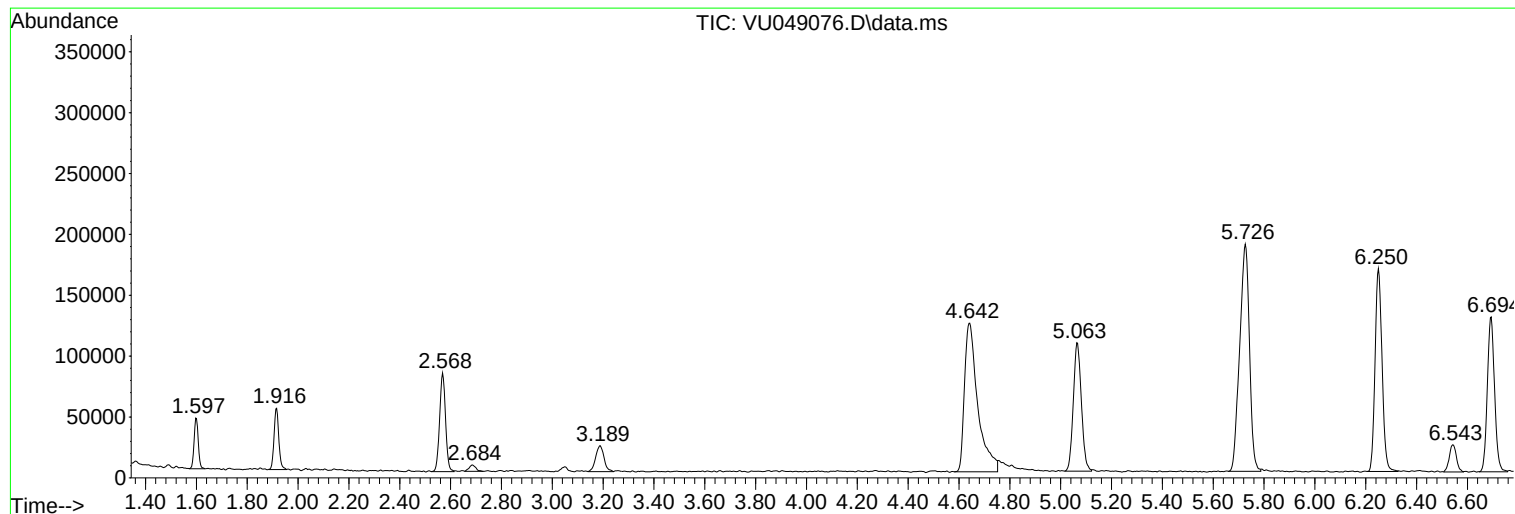

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049076.D
Acq On : 12 Jun 2022 00:40
Operator : SY/MD
Sample : N3277-20 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
Data File : VU049076.D
Acq On : 12 Jun 2022 00:40
Operator : SY/MD
Sample : N3277-20 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc