
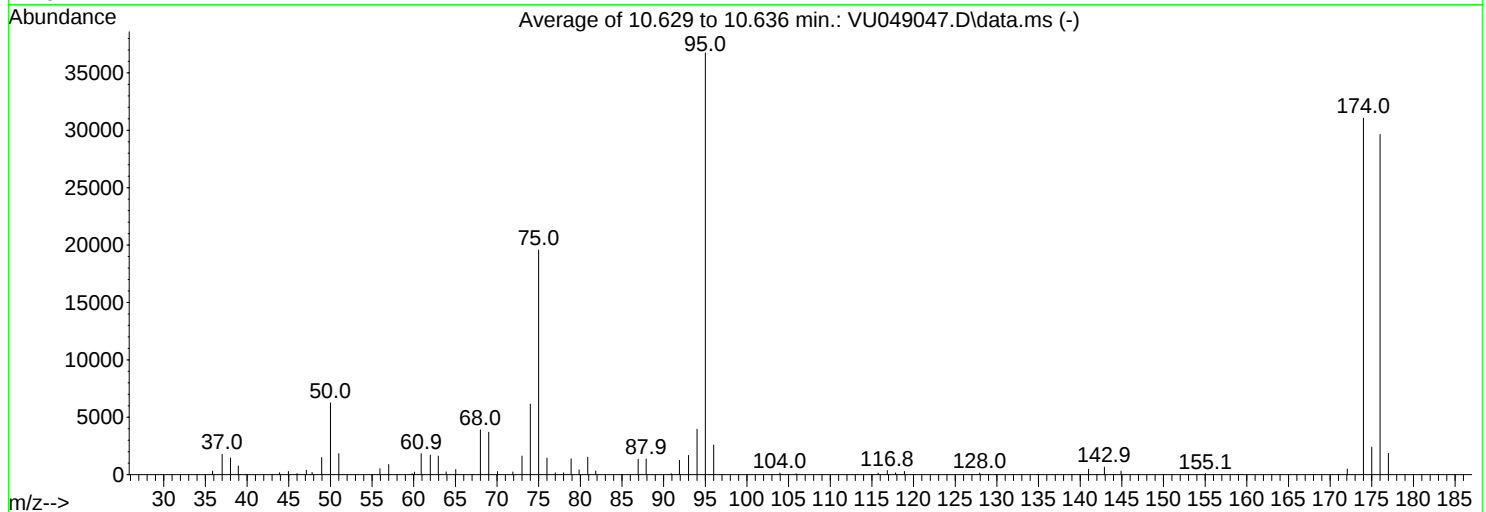


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061122\
 Data File : VU049047.D
 Acq On : 11 Jun 2022 11:29
 Operator : SY/MD
 Sample : BFB081
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB081

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jun 13 01:35:15 2022

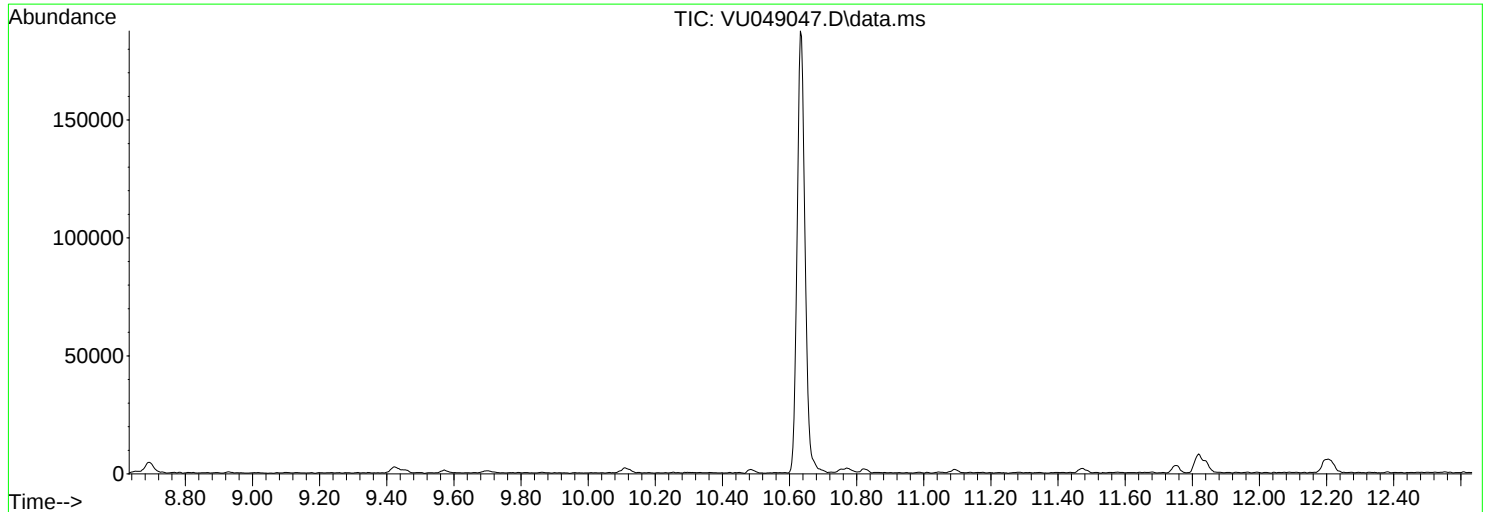

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	6266	PASS
75	95	30	80	53.3	19571	PASS
95	95	100	100	100.0	36747	PASS
96	95	5	9	7.0	2583	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.5	31053	PASS
175	174	5	9	7.7	2400	PASS
176	174	95	101	95.4	29637	PASS
177	176	5	9	6.3	1857	PASS

m/z	Abundance
39.90	153.0
44.00	302.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.80	250.0
37.00	1721.0
38.00	1341.0
39.00	820.0
39.80	187.0
43.80	448.0
44.90	260.0
47.10	382.0
47.80	167.0
49.00	1286.0
50.00	6056.0
51.00	1904.0
56.00	507.0
57.00	907.0
59.80	269.0
60.90	1733.0
62.00	1556.0
63.00	1496.0
63.90	283.0
65.00	385.0
68.00	3651.0
69.00	3596.0
70.10	263.0
71.90	223.0
73.00	1492.0
74.00	5892.0
75.00	18408.0
76.00	1403.0
76.90	136.0
78.00	126.0
78.90	1321.0
79.90	370.0
80.90	1384.0
81.80	270.0
87.00	1312.0
87.90	1343.0
91.90	1145.0
93.00	1598.0
94.00	3867.0
95.00	35064.0
96.00	2602.0
104.00	151.0
115.80	109.0
116.80	348.0
117.80	128.0
118.90	278.0
127.90	132.0
141.00	423.0
142.90	554.0
144.90	300.0
155.00	133.0
172.10	463.0
174.00	28904.0
175.00	2171.0
176.00	27352.0
177.00	1773.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.90	312.0
37.00	1873.0
38.00	1528.0
38.90	773.0
39.90	218.0
43.80	485.0
44.90	309.0
46.00	122.0
47.10	384.0
47.80	226.0
48.90	1537.0
50.00	6472.0
51.00	1873.0
56.00	513.0
57.00	904.0
60.10	297.0
60.90	1908.0
62.00	1804.0
63.00	1654.0
63.90	240.0
65.10	448.0
68.00	4053.0
69.00	3828.0
70.00	284.0
71.90	259.0
73.00	1673.0
74.00	6348.0
75.00	20184.0
76.00	1499.0
77.00	162.0
78.00	174.0
78.90	1468.0
79.80	421.0
80.90	1635.0
81.90	340.0
87.00	1347.0
87.90	1415.0
90.90	116.0
91.90	1316.0
93.00	1741.0
94.00	4021.0
95.00	38168.0
96.00	2674.0
103.90	135.0
105.90	101.0
115.70	139.0
116.90	388.0
117.90	164.0
118.90	267.0
127.90	157.0
141.00	480.0
142.90	676.0
144.90	301.0
155.10	117.0
172.00	495.0
174.00	32096.0
175.00	2458.0
176.00	30720.0
177.00	1965.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.90	346.0
37.00	1738.0
38.00	1498.0
38.90	669.0
39.90	198.0
43.90	472.0
45.00	260.0
46.00	188.0
47.10	411.0
47.80	199.0
48.90	1652.0
50.00	6271.0
51.00	1694.0
55.90	540.0
57.00	827.0
60.10	359.0
60.90	1839.0
62.00	1757.0
62.90	1695.0
63.90	209.0
65.10	493.0
68.00	3997.0
69.00	3650.0
70.00	272.0
71.90	233.0
73.00	1687.0
74.00	6225.0
75.00	20120.0
76.00	1467.0
77.10	217.0
78.00	206.0
78.90	1364.0
79.80	450.0
80.90	1557.0
81.80	370.0
86.90	1350.0
87.90	1322.0
90.90	120.0
91.90	1301.0
93.00	1699.0
94.00	4001.0
95.00	37008.0
96.00	2474.0
103.90	125.0
105.90	144.0
115.70	175.0
116.90	371.0
117.90	189.0
118.90	289.0
128.00	126.0
129.80	103.0
141.00	473.0
142.90	744.0
144.90	325.0
172.00	502.0
174.00	32160.0
175.00	2571.0
176.00	30840.0
177.00	1832.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081