

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061124\
 Data File : VU059210.D
 Acq On : 11 Jun 2024 10:48
 Operator : MD/SY
 Sample : P2798-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB66

Quant Time: Jun 12 04:25:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 12 04:24:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	173633	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	174095	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	75429	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	38698	3.679	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.600%
7) Chloroethane-d5	1.907	69	42991	4.522	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.400%
11) 1,1-Dichloroethene-d2	2.560	65	17341	4.046	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.000%
20) 2-Butanone-d5	4.621	46	139716	51.094	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.180%
24) Chloroform-d	5.055	84	104079	4.900	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.000%
26) 1,2-Dichloroethane-d4	5.695	65	54844	5.024	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	5.721	84	195809	4.900	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.000%
36) 1,2-Dichloropropane-d6	6.682	67	66651	5.006	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.200%
41) Toluene-d8	7.894	98	156172	4.294	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.800%
43) trans-1,3-Dichloroprop...	8.177	79	20578	4.503	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.000%
46) 2-Hexanone-d5	8.627	63	98942	45.120	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.240%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	57781	5.025	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	61100	5.386	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.800%
Target Compounds						
					Qvalue	
13) Acetone	2.637	43	13568	7.179	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061124\
Data File : VU059210.D
Acq On : 11 Jun 2024 10:48
Operator : MD/SY
Sample : P2798-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB66

Quant Time: Jun 12 04:25:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 12 04:24:49 2024
Response via : Initial Calibration

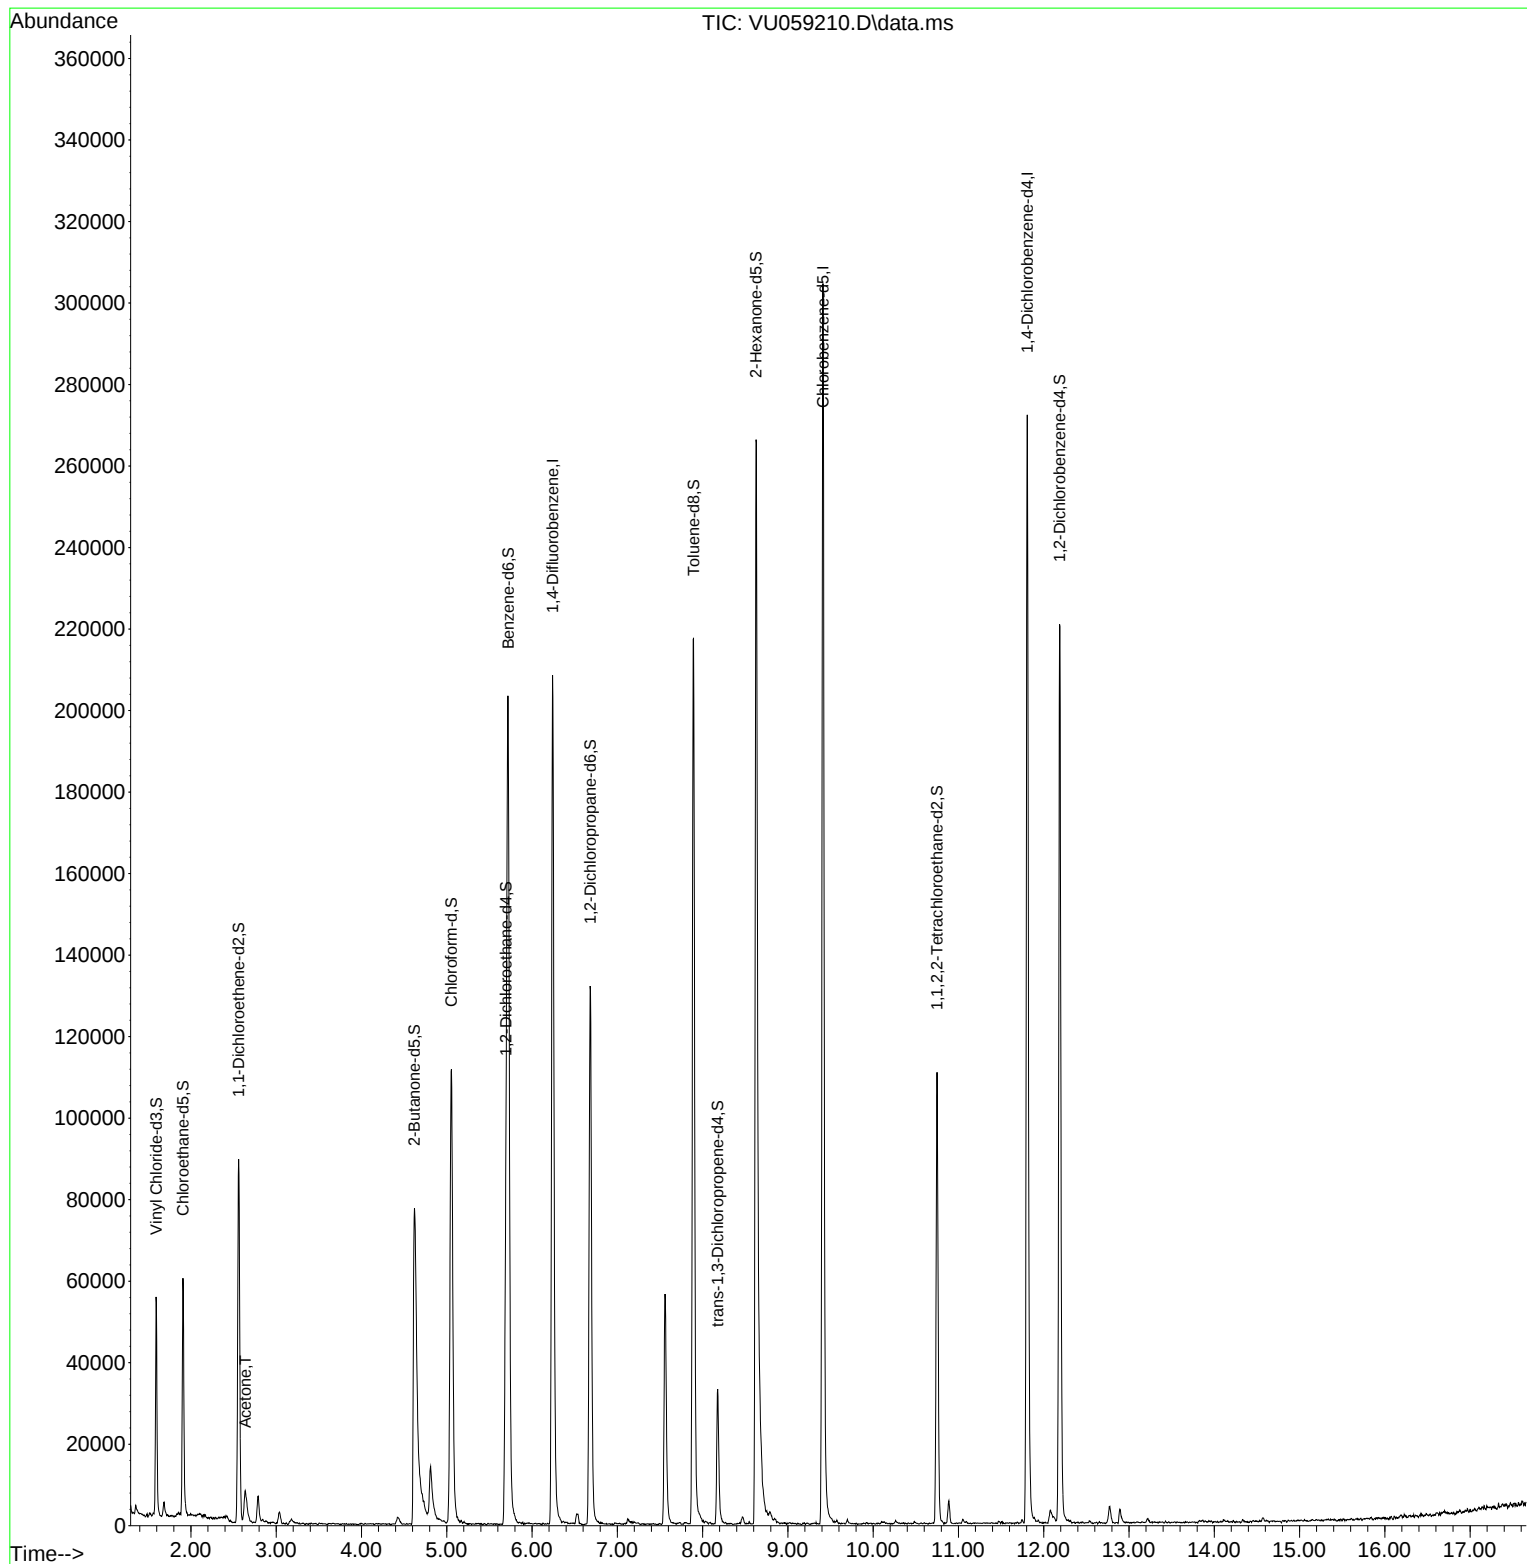

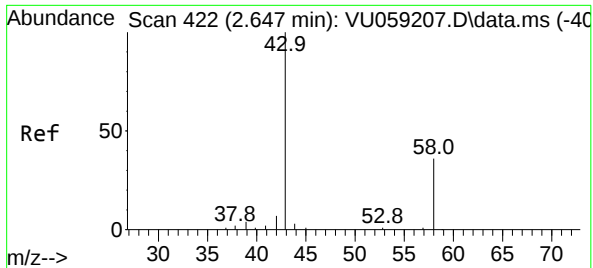

#13
 Acetone
 Concen: 7.179 ug/L
 RT: 2.637 min Scan# 41
 Delta R.T. -0.010 min
 Lab File: VU059210.D
 Acq: 11 Jun 2024 10:48

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB66

Tgt Ion: 43 Resp: 13568
 Ion Ratio Lower Upper
 43 100
 58 35.3 0.0 68.0

