


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061124\
Data File : VU059206.D
Acq On : 11 Jun 2024 08:13
Operator : MD/SY
Sample : BFB160
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB160

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Jun 12 04:24:49 2024

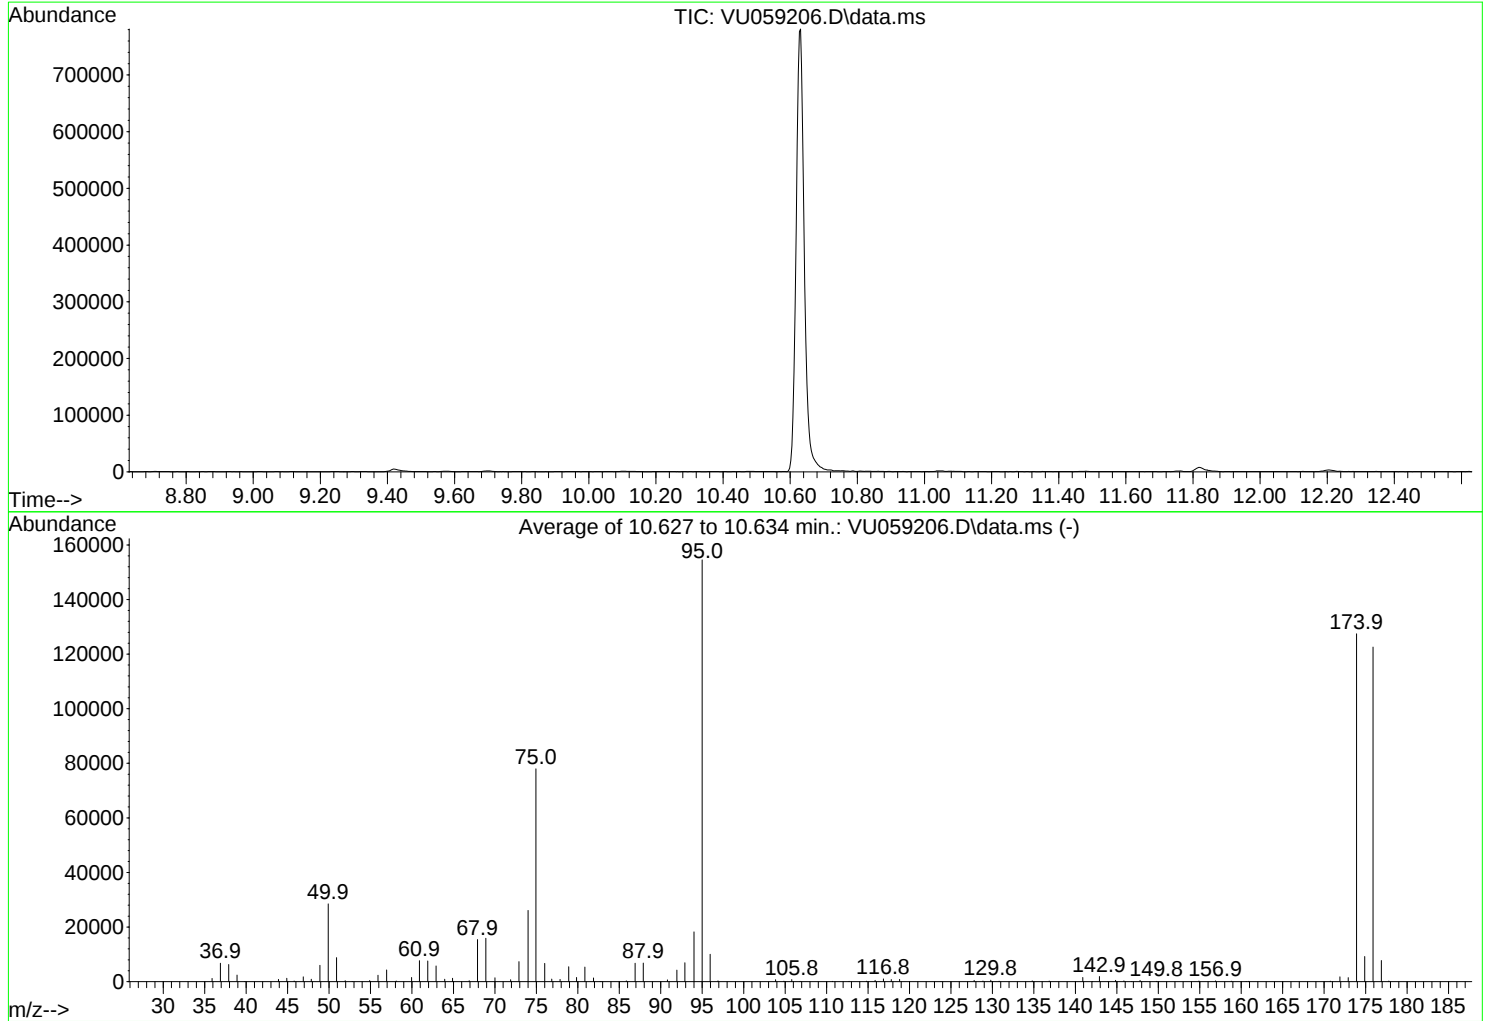

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	28467	PASS
75	95	30	80	50.5	77979	PASS
95	95	100	100	100.0	154539	PASS
96	95	5	9	6.5	10016	PASS
173	174	0.00	2	1.1	1443	PASS
174	95	50	120	82.5	127453	PASS
175	174	5	9	7.2	9198	PASS
176	174	95	101	96.2	122555	PASS
177	176	5	9	6.3	7769	PASS

m/z	Abundance
39.90	124.0
43.90	356.0

Instrument :
MSVOA_U
ClientSampleId :
BFB160

m/z	Abundance
35.90	1348.0
36.90	7144.0
37.90	6615.0
38.90	2482.0
39.90	172.0
43.90	1209.0
44.90	1371.0
45.80	265.0
46.90	1824.0
47.80	1060.0
48.90	6266.0
49.90	30144.0
50.90	8909.0
51.90	350.0
52.80	141.0
54.90	444.0
55.90	2640.0
57.00	4566.0
58.10	291.0
60.00	1580.0
60.90	7766.0
61.90	8033.0
62.90	5955.0
63.90	968.0
64.90	1263.0
66.90	347.0
67.90	16392.0
68.90	16696.0
70.00	1456.0
71.90	808.0
72.90	7366.0
74.00	26848.0
75.00	81688.0
76.00	6891.0
76.90	1076.0
77.80	856.0
78.90	5643.0
79.80	1494.0
80.80	5621.0
81.90	1406.0
85.80	325.0
86.90	7223.0
87.90	6868.0
90.80	568.0
92.00	4500.0
92.90	7170.0
94.00	19080.0
95.00	158784.0
96.00	10333.0
96.90	369.0
103.90	715.0
104.90	205.0
105.80	772.0
106.80	187.0
110.70	156.0
112.70	128.0
114.80	173.0
115.90	563.0
116.90	1034.0
117.80	685.0
118.80	803.0
123.80	110.0
127.80	499.0
128.90	271.0
129.80	472.0
130.80	139.0
134.80	265.0
136.80	285.0
140.90	1496.0
142.90	2060.0
144.00	135.0
144.90	501.0
145.80	286.0
147.80	402.0
149.80	166.0
154.90	297.0
156.90	325.0
158.80	101.0
160.60	102.0
170.80	168.0
171.90	1693.0
172.90	1396.0
173.90	127776.0
174.90	9525.0
175.90	122016.0
176.90	7813.0
177.80	227.0

Instrument :
MSVOA_U
ClientSampleId :
BFB160

m/z	Abundance
35.90	1239.0
36.90	6967.0
37.90	6507.0
38.90	2453.0
39.90	175.0
43.90	1200.0
44.90	1268.0
45.80	267.0
46.90	1851.0
47.90	933.0
48.90	6139.0
49.90	29248.0
50.90	9109.0
52.00	363.0
54.90	423.0
55.90	2419.0
56.90	4400.0
58.10	251.0
59.90	1608.0
60.90	7937.0
61.90	7778.0
62.90	5969.0
63.90	881.0
64.90	1265.0
66.90	337.0
67.90	15813.0
68.90	16488.0
70.00	1488.0
71.90	705.0
72.90	7560.0
74.00	26952.0
75.00	80224.0
76.00	6896.0
76.90	994.0
77.80	846.0
78.90	5621.0
79.90	1577.0
80.90	5455.0
81.90	1425.0
82.70	107.0
82.90	108.0
85.90	295.0
86.90	6951.0
87.90	6944.0
90.80	660.0
92.00	4303.0
92.90	7120.0
94.00	18704.0
95.00	159168.0
96.00	10327.0
96.90	326.0
103.80	720.0
104.90	192.0
105.80	819.0
106.80	118.0
110.70	144.0
112.70	142.0
114.80	194.0
115.80	486.0
116.90	1040.0
117.80	821.0
118.80	859.0
127.80	501.0
128.90	272.0
129.80	523.0
130.80	168.0
134.80	337.0
136.90	282.0
140.90	1583.0
142.10	136.0
142.90	1912.0
143.90	119.0
144.90	483.0
145.80	324.0
146.80	101.0
147.80	499.0
149.80	132.0
154.90	271.0
156.90	304.0
158.80	184.0
160.90	127.0
170.70	172.0
171.90	1837.0
172.90	1538.0
173.90	131456.0
174.90	9459.0
175.90	126400.0
176.90	8019.0
177.80	240.0

Instrument :
MSVOA_U
ClientSampleId :
BFB160

m/z	Abundance
35.90	1002.0
36.90	6188.0
37.90	5738.0
38.90	2212.0
39.80	204.0
43.90	1117.0
44.90	1060.0
45.80	211.0
46.90	1656.0
47.90	732.0
48.90	5479.0
49.90	26008.0
50.90	8396.0
52.00	358.0
54.90	408.0
55.90	2025.0
56.90	3853.0
58.00	131.0
59.90	1469.0
60.90	7276.0
61.90	6922.0
62.90	5366.0
64.00	754.0
64.90	1170.0
66.90	370.0
67.90	13983.0
68.90	14528.0
70.00	1258.0
71.90	625.0
72.90	7031.0
74.00	24536.0
74.90	72024.0
76.00	6200.0
76.80	811.0
77.90	748.0
78.90	5044.0
79.90	1481.0
80.90	4965.0
81.90	1276.0
85.80	245.0
86.90	6066.0
87.90	6575.0
90.80	647.0
91.90	3796.0
92.90	6404.0
94.00	16944.0
95.00	145664.0
95.90	9387.0
96.90	266.0
103.80	715.0
104.80	144.0
105.80	793.0
110.70	134.0
112.70	118.0
114.80	170.0
115.80	439.0
116.80	1000.0
117.80	841.0
118.80	814.0
127.80	488.0
128.80	257.0
129.80	554.0
130.80	184.0
134.80	350.0
136.80	245.0
140.90	1522.0
142.00	102.0
142.90	1727.0
144.80	410.0
145.90	318.0
146.80	100.0
147.80	480.0
149.80	122.0
154.90	237.0
156.90	255.0
158.80	239.0
160.90	162.0
170.70	162.0
171.90	1767.0
172.90	1396.0
173.90	123128.0
174.90	8611.0
175.90	119248.0
176.90	7474.0
177.80	200.0

Instrument :
MSVOA_U
ClientSampleId :
BFB160