

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
 Data File : VU063385.D
 Acq On : 11 Jun 2025 16:00
 Operator : MD/SY
 Sample : VU0611WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK118

Quant Time: Jun 11 16:21:14 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 11 13:45:27 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	142343	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	147069	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	63433	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	51423	47.855	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	95.700%	
7) Chloroethane-d5	1.901	69	51937	49.668	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	99.340%	
11) 1,1-Dichloroethene-d2	2.554	63	71641	35.088	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	70.180%	
21) 2-Butanone-d5	4.615	46	103862	111.386	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	111.390%	
24) Chloroform-d	5.052	84	110673	48.452	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.900%	
26) 1,2-Dichloroethane-d4	5.692	65	71698	51.253	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.500%	
32) Benzene-d6	5.714	84	222674	50.060	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	100.120%	
36) 1,2-Dichloropropane-d6	6.679	67	78611	52.107	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	104.220%	
41) Toluene-d8	7.891	98	185234	47.460	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	94.920%	
43) trans-1,3-Dichloroprop...	8.171	79	29031	47.819	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	95.640%	
47) 2-Hexanone-d5	8.624	63	55043	98.269	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	98.270%	
56) 1,1,2,2-Tetrachloroeth...	10.746	84	113271	49.159	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.320%	
66) 1,2-Dichlorobenzene-d4	12.187	152	65384	56.336	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	112.680%	
Target Compounds						
37) 1,2-Dichloropropane	6.679	63	7745	5.108	ug/L #	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063385.D
Acq On : 11 Jun 2025 16:00
Operator : MD/SY
Sample : VU0611WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK118

Quant Time: Jun 11 16:21:14 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:45:27 2025
Response via : Initial Calibration

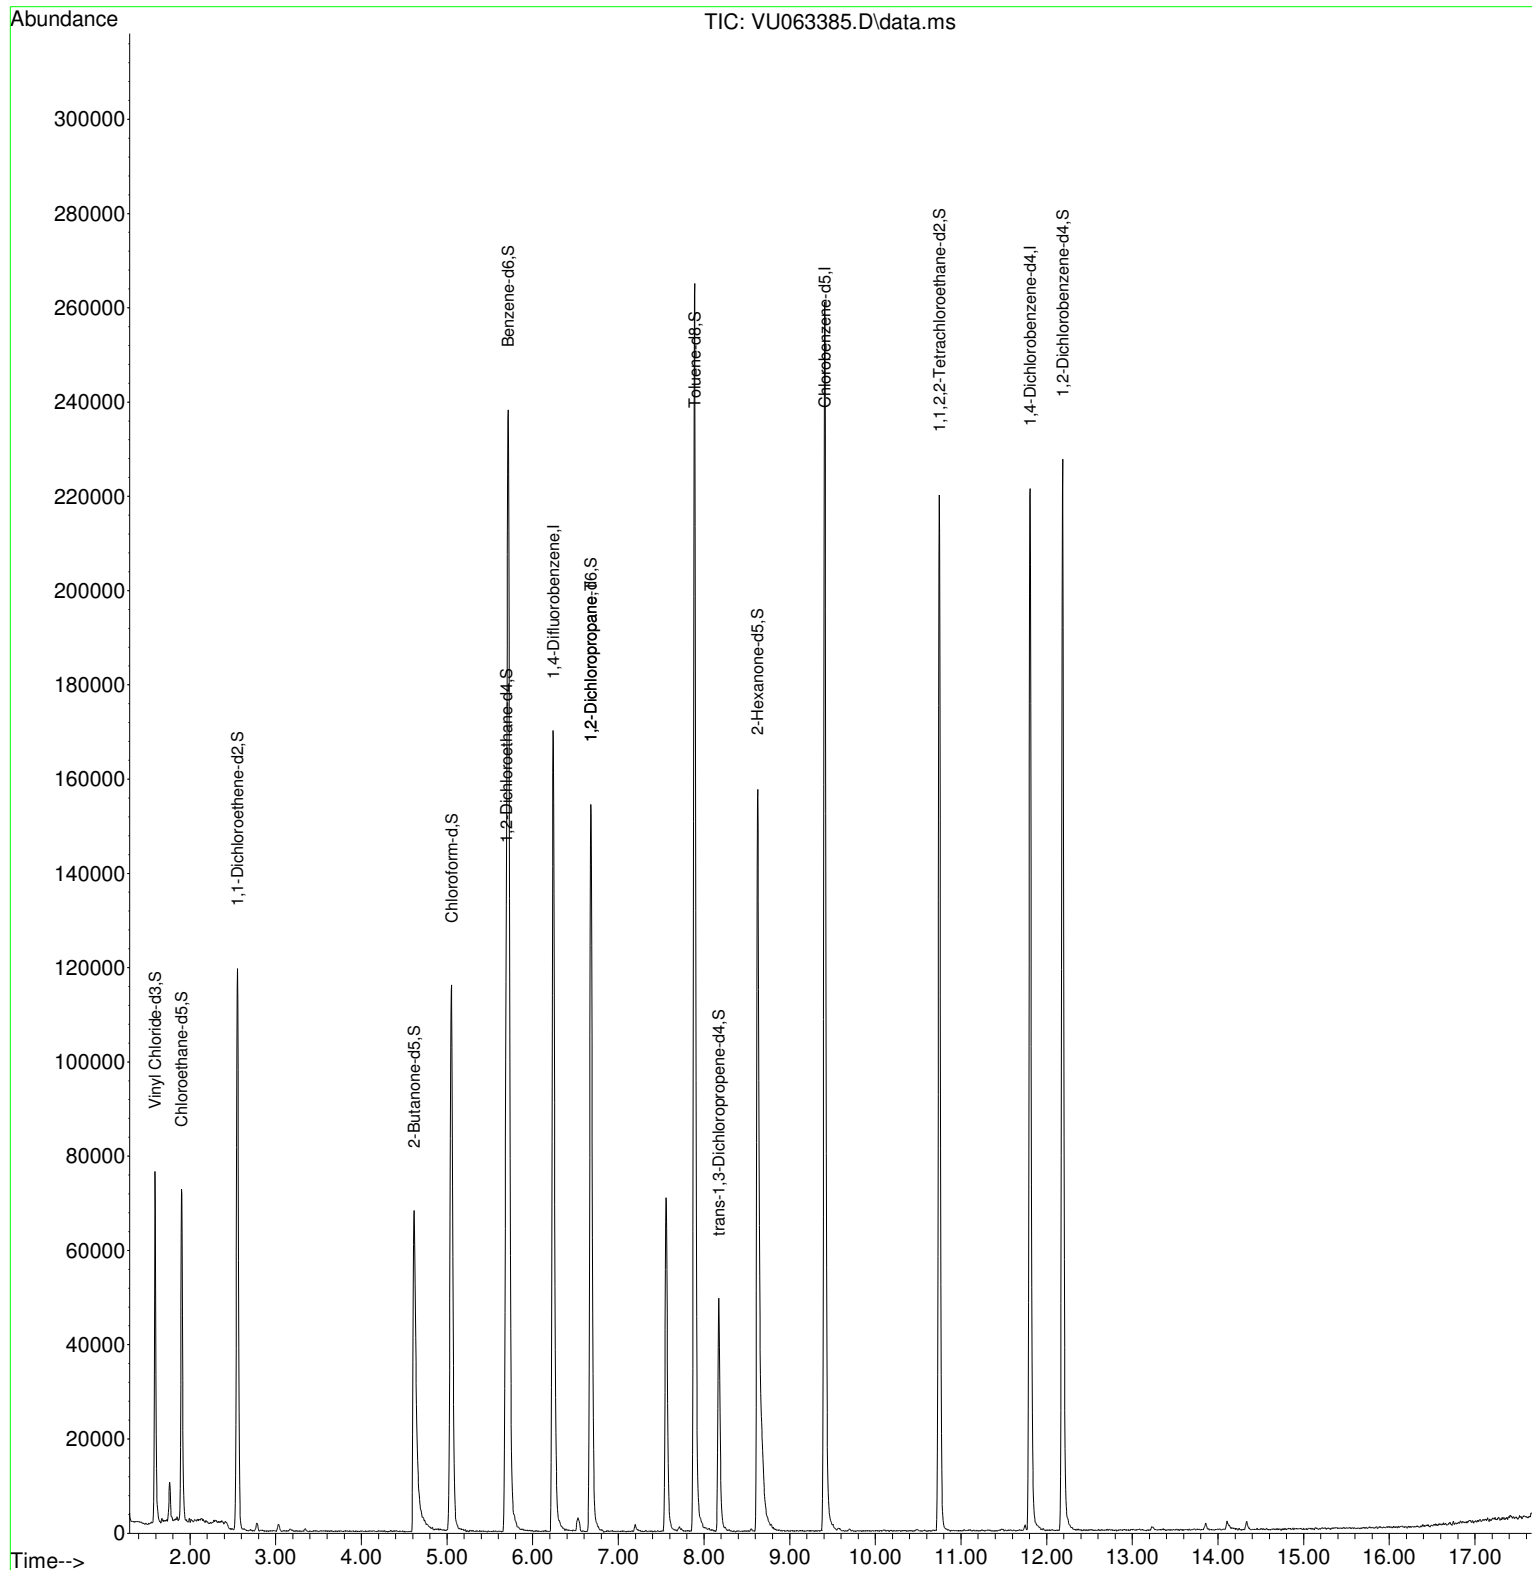

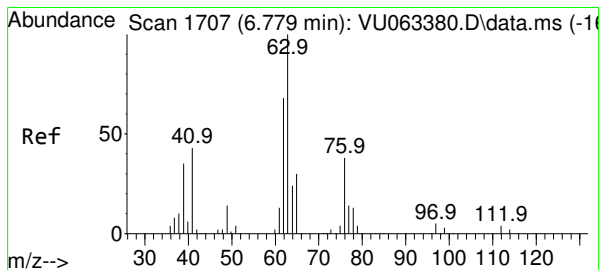

#37
 1,2-Dichloropropane
 Concen: 5.108 ug/L
 RT: 6.679 min Scan# 1
 Delta R.T. -0.100 min
 Lab File: VU063385.D
 Acq: 11 Jun 2025 16:00

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK118

Tgt Ion: 63 Resp: 7745
 Ion Ratio Lower Upper
 63 100
 112 0.0 2.9 4.3#

