




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063378.D
Acq On : 11 Jun 2025 11:23
Operator : MD/SY
Sample : VSTD00533
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD005033

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 11 13:20:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:19:23 2025
Response via : Initial Calibration

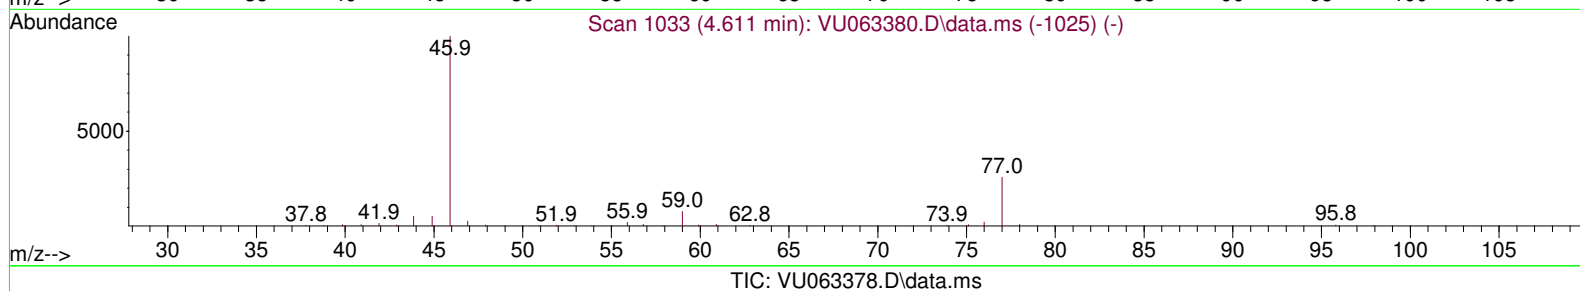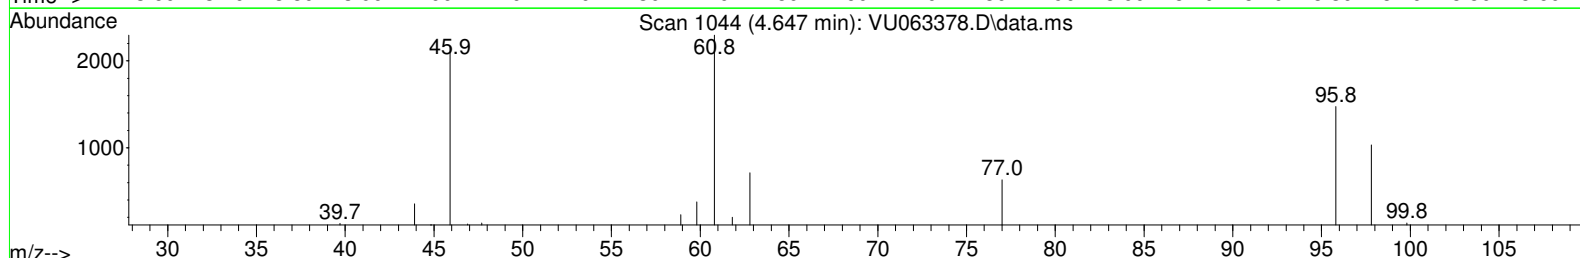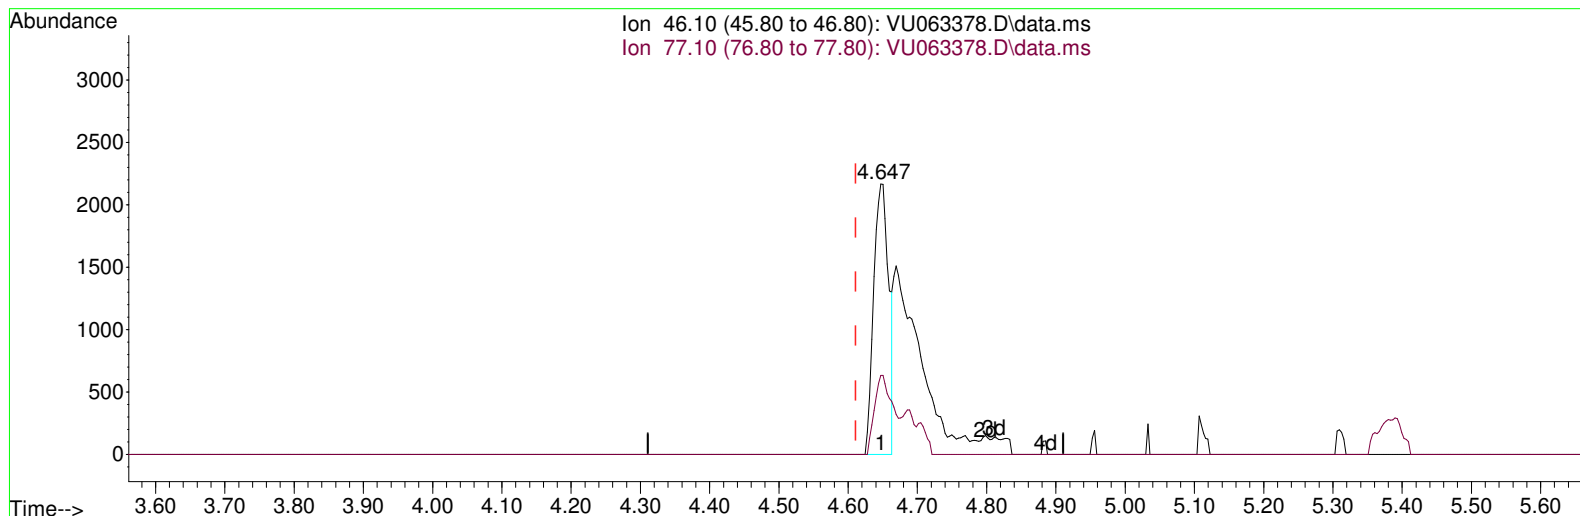

(21) 2-Butanone-d5 (S)

4.647min (+ 0.036) 4.13 ug/L

response 3312

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.30	34.57#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063378.D
Acq On : 11 Jun 2025 11:23
Operator : MD/SY
Sample : VSTD00533
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD005033

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 11 13:20:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:19:23 2025
Response via : Initial Calibration

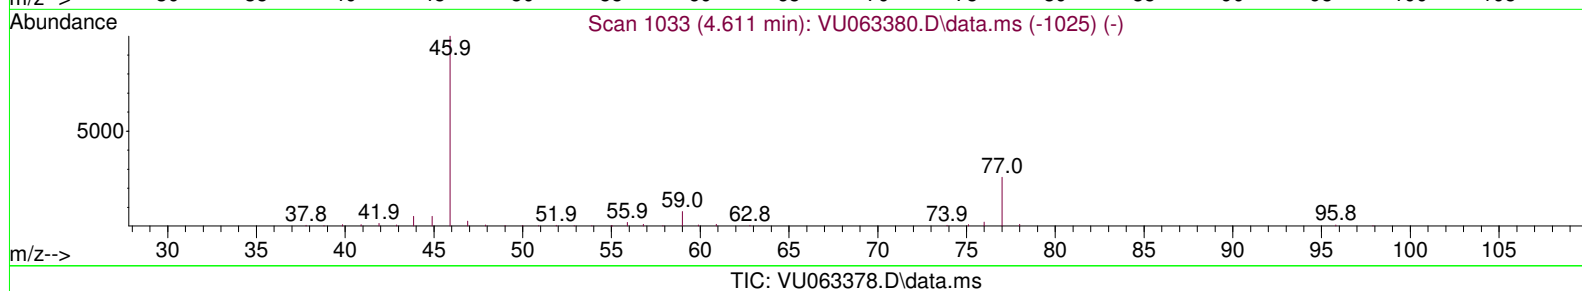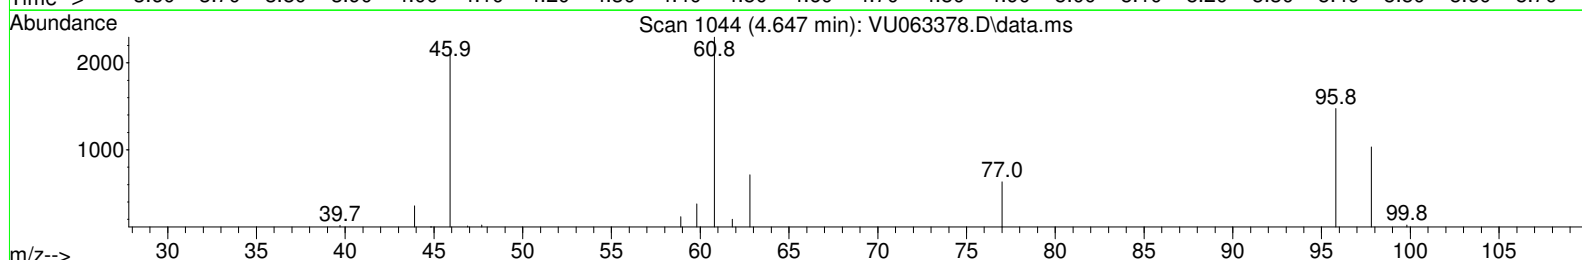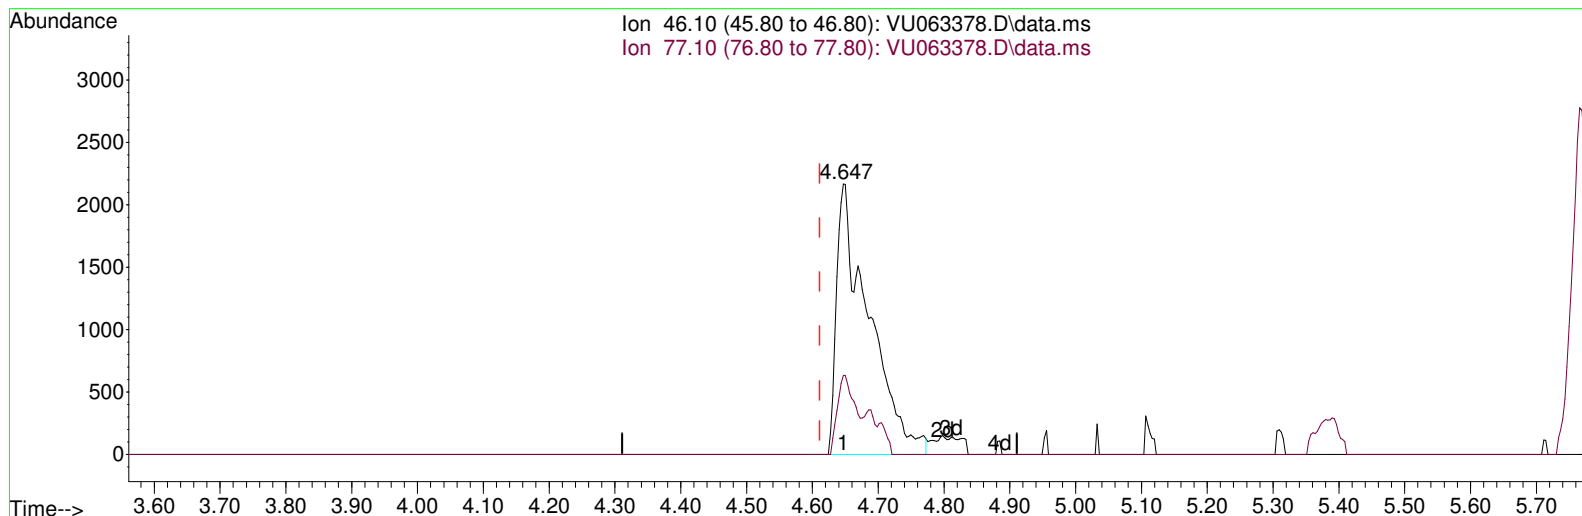

(21) 2-Butanone-d5 (S)

4.647min (+ 0.036) 9.16 ug/L m

response 7354

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.30	15.57#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063378.D
Acq On : 11 Jun 2025 11:23
Operator : MD/SY
Sample : VSTD00533
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD005033

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 11 13:20:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:19:23 2025
Response via : Initial Calibration

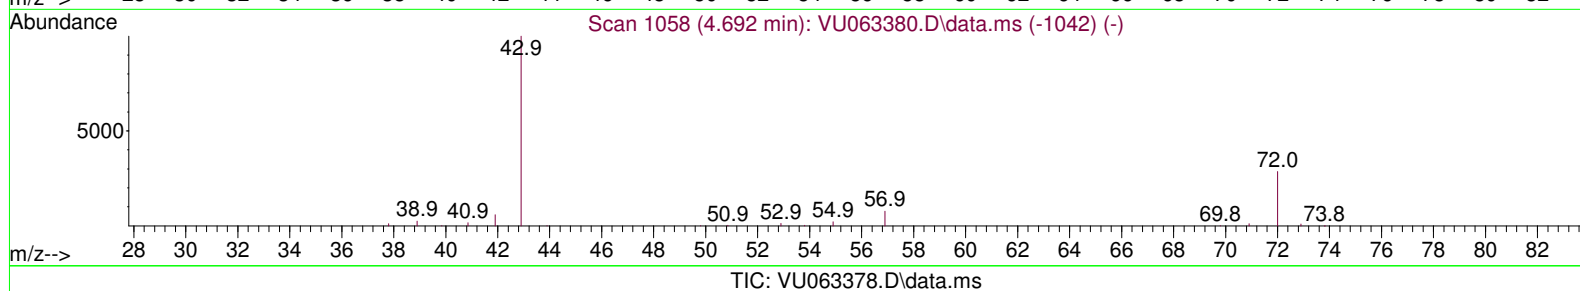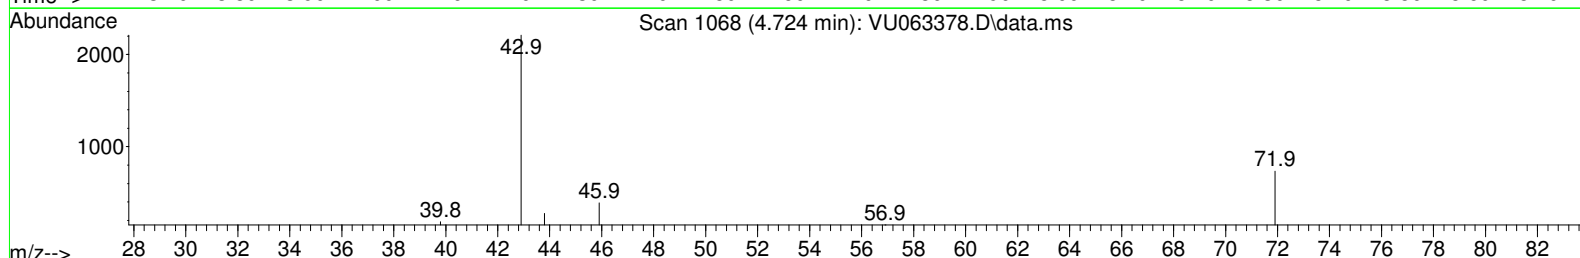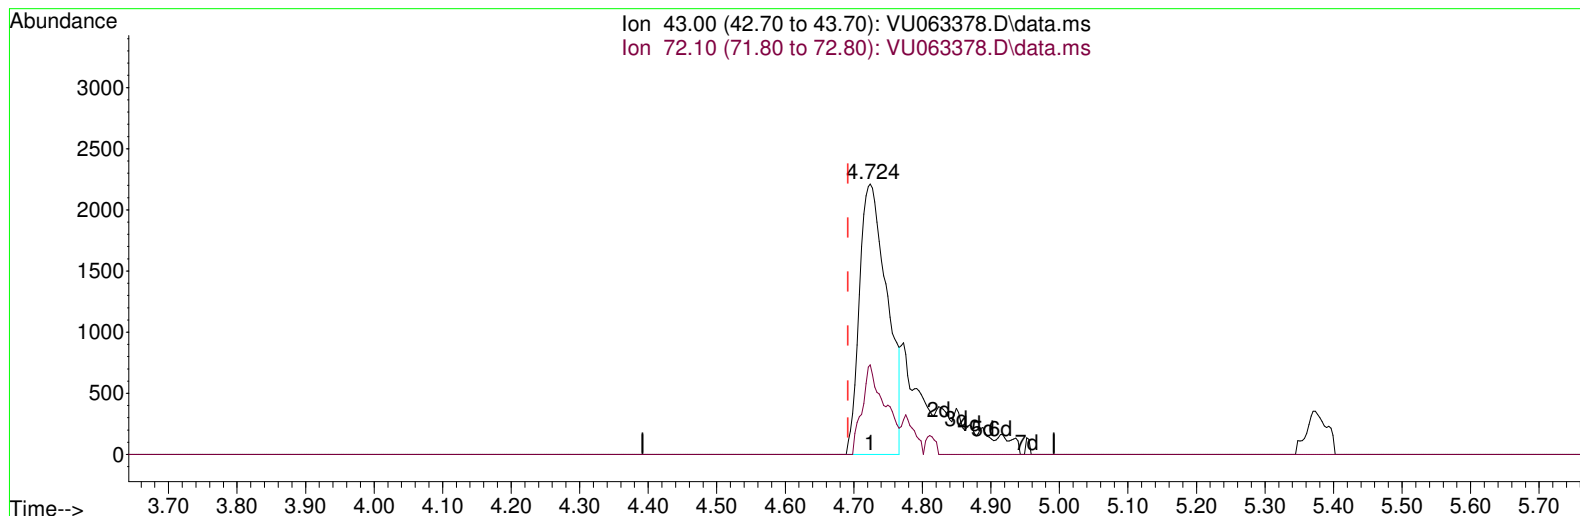

(22) 2-Butanone (T)

4.724min (+ 0.032) 7.82 ug/L

response 6186

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	30.90	21.73
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063378.D
Acq On : 11 Jun 2025 11:23
Operator : MD/SY
Sample : VSTD00533
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD005033

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 11 13:20:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:19:23 2025
Response via : Initial Calibration

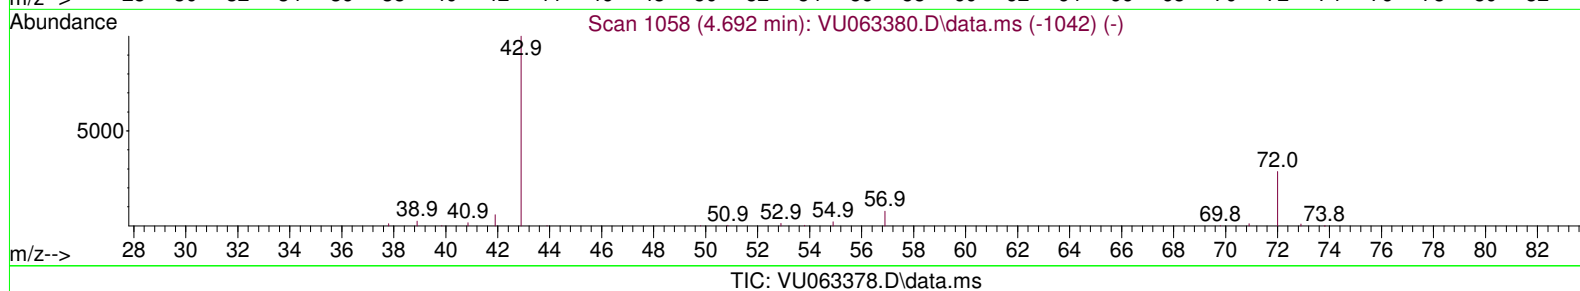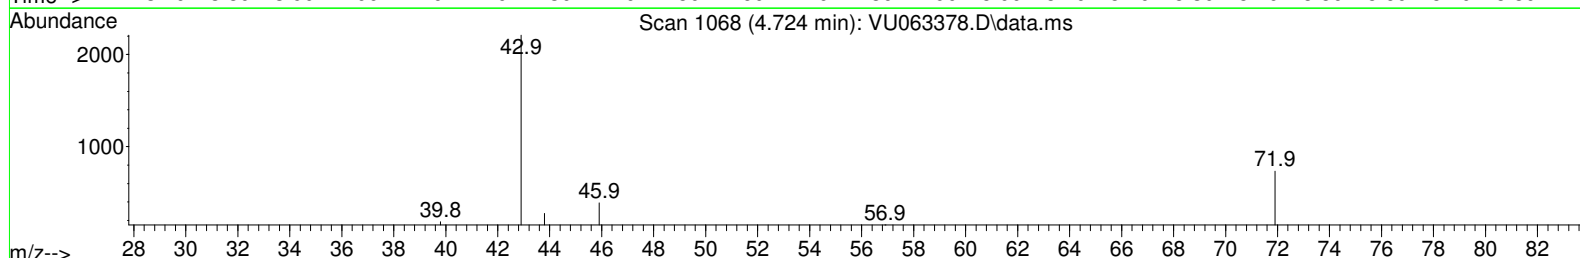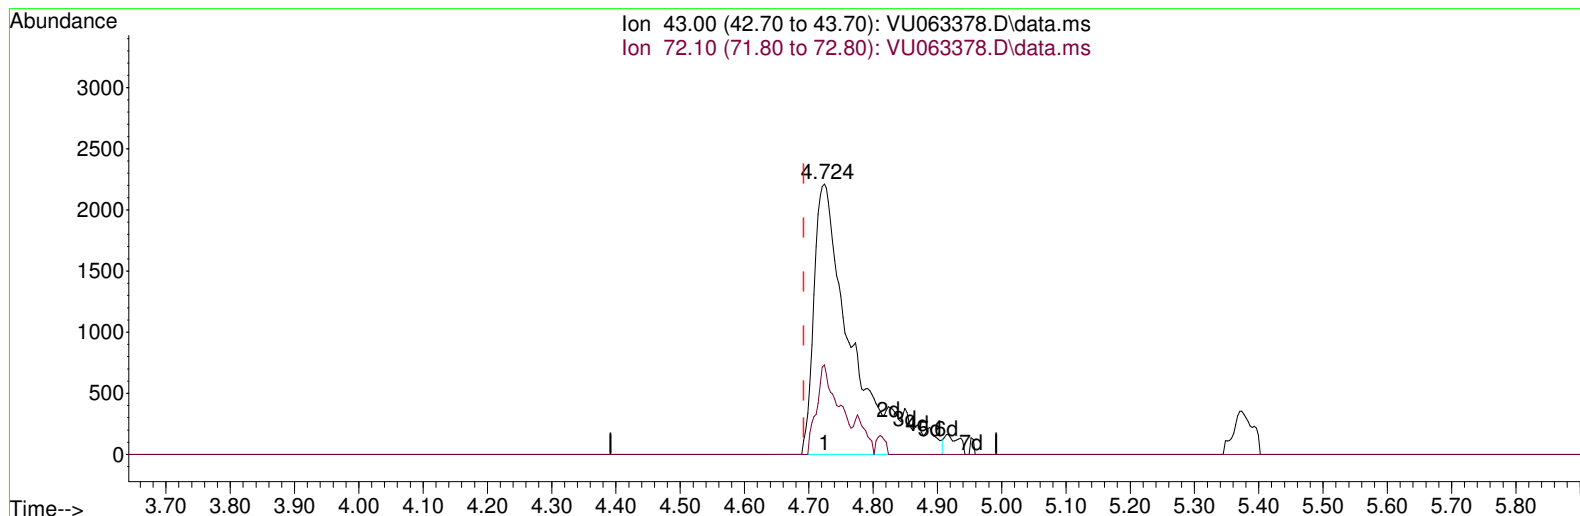

(22) 2-Butanone (T)

4.724min (+ 0.032) 11.62 ug/L m

response 9192

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	30.90	14.62#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063378.D
Acq On : 11 Jun 2025 11:23
Operator : MD/SY
Sample : VSTD00533
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD005033

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 11 13:20:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:19:23 2025
Response via : Initial Calibration

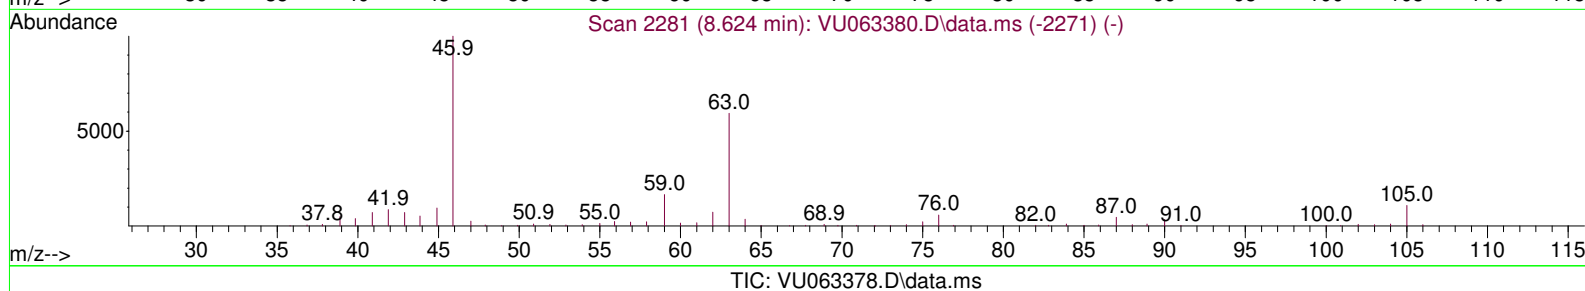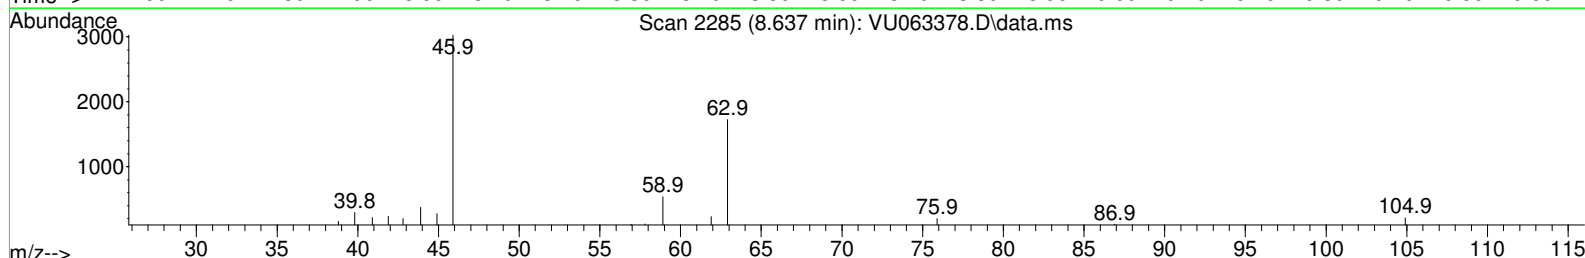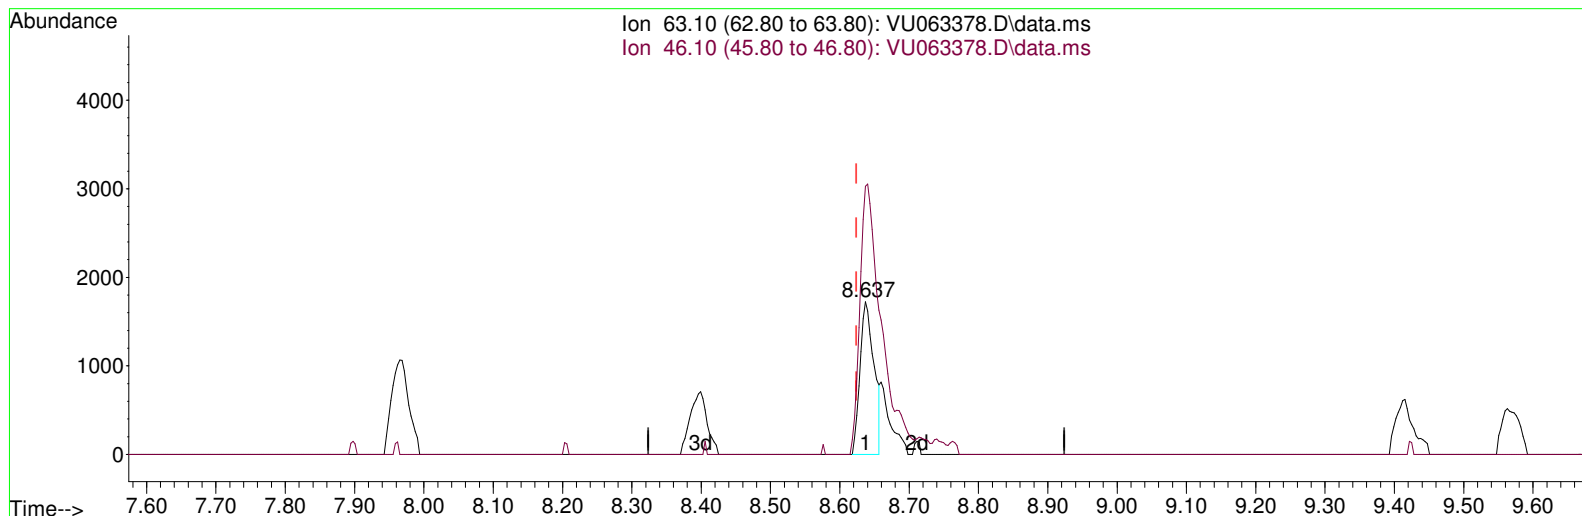

(47) 2-Hexanone-d5 (S)

8.637min (+ 0.013) 4.56 ug/L

response 2424

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	177.10	249.67#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063378.D
Acq On : 11 Jun 2025 11:23
Operator : MD/SY
Sample : VSTD00533
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD005033

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 11 13:20:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:19:23 2025
Response via : Initial Calibration

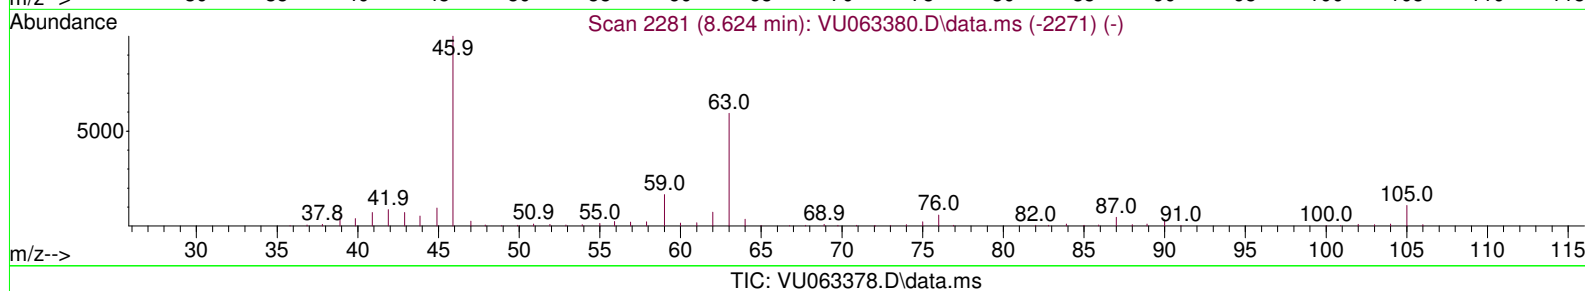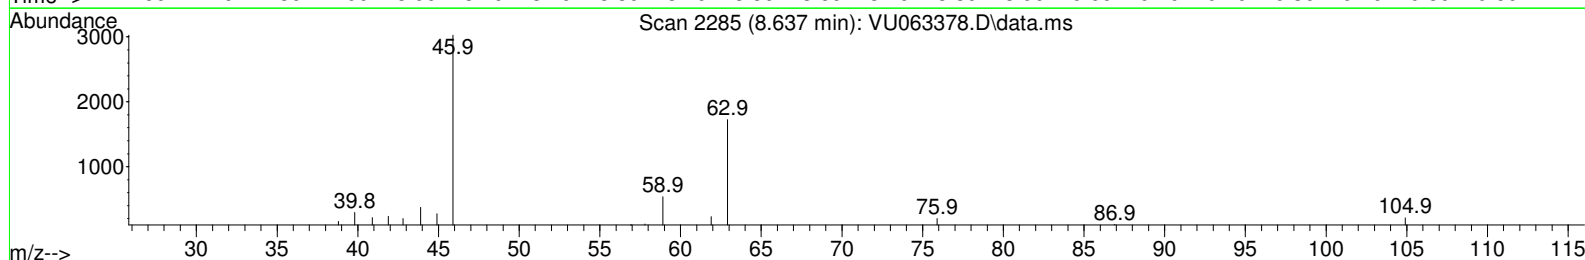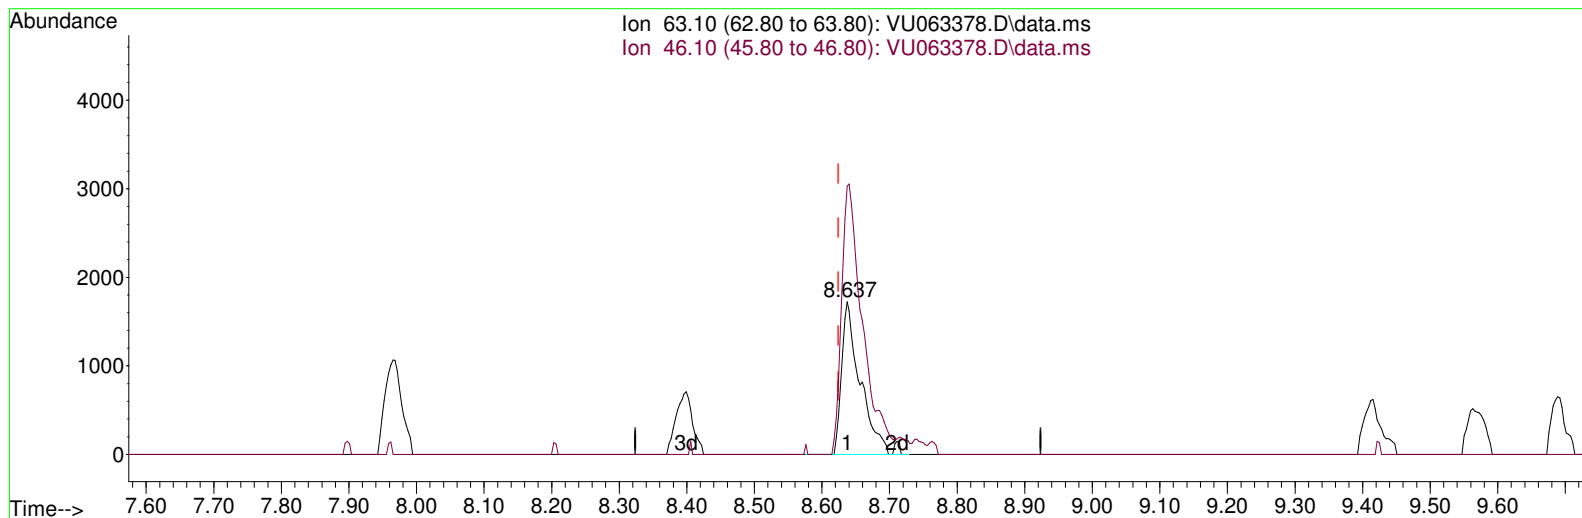

(47) 2-Hexanone-d5 (S)

8.637min (+ 0.013) 6.29 ug/L m

response 3340

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	177.10	181.20
0.00	0.00	0.00
0.00	0.00	0.00