




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063379.D
Acq On : 11 Jun 2025 11:48
Operator : MD/SY
Sample : VSTD01034
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD010034

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 11 13:21:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:19:23 2025
Response via : Initial Calibration

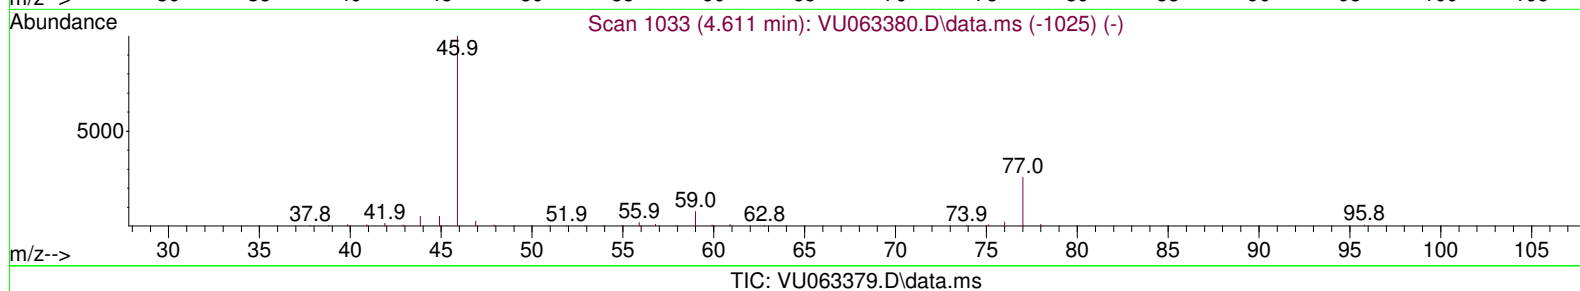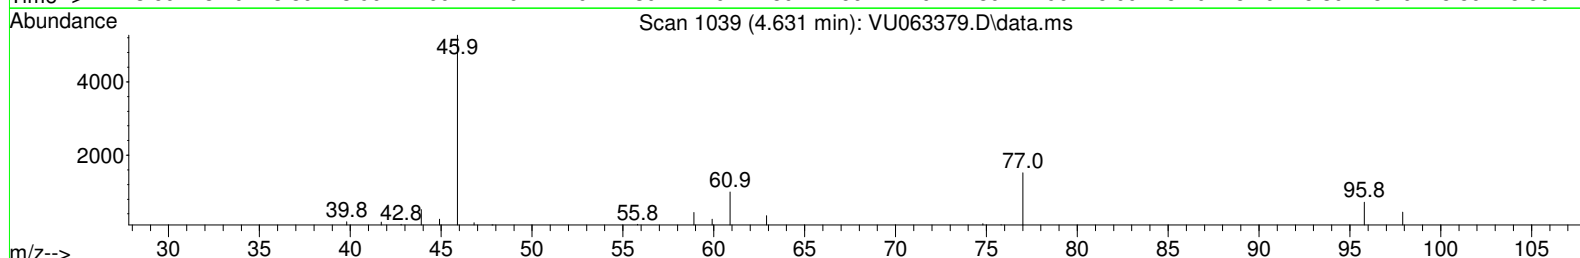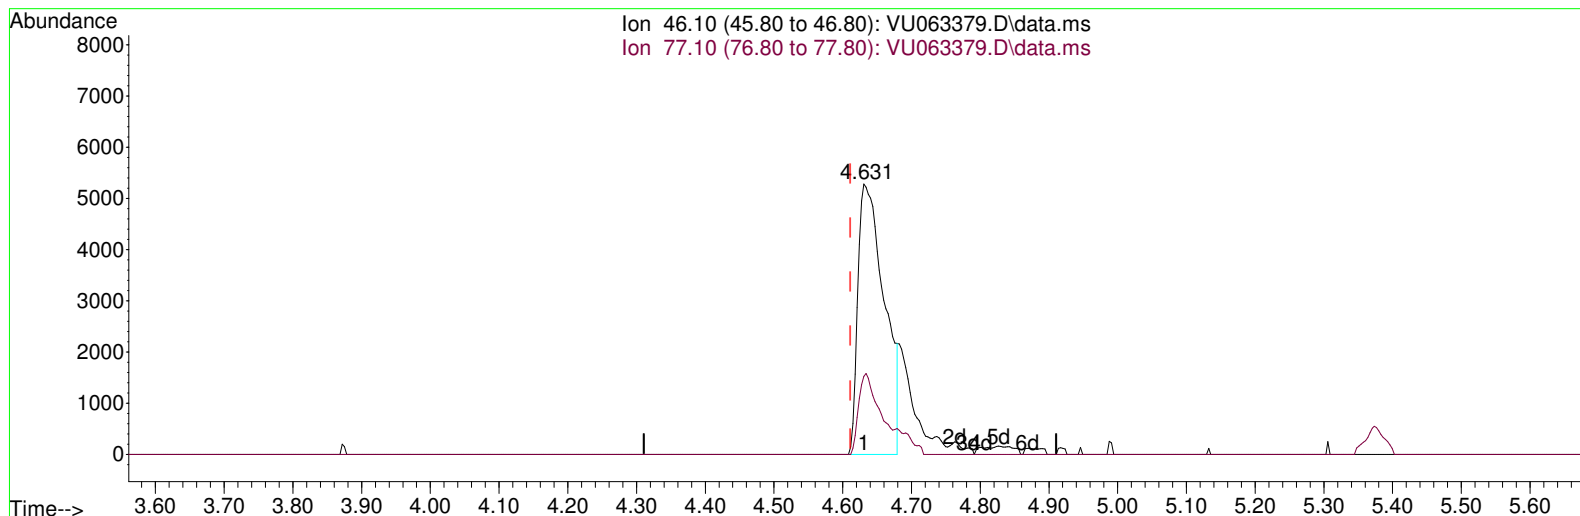

(21) 2-Butanone-d5 (S)

4.631min (+ 0.020) 15.97 ug/L

response 14035

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.30	23.69
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063379.D
Acq On : 11 Jun 2025 11:48
Operator : MD/SY
Sample : VSTD01034
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD010034

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 11 13:21:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:19:23 2025
Response via : Initial Calibration

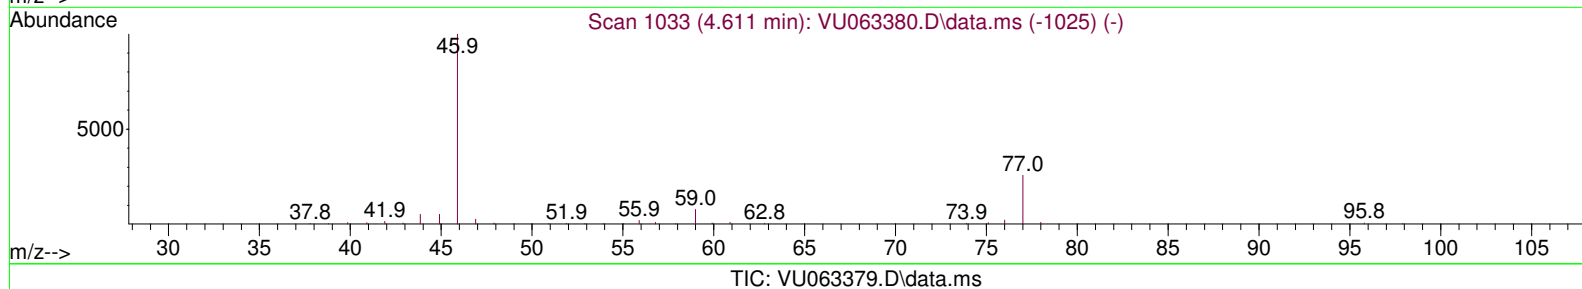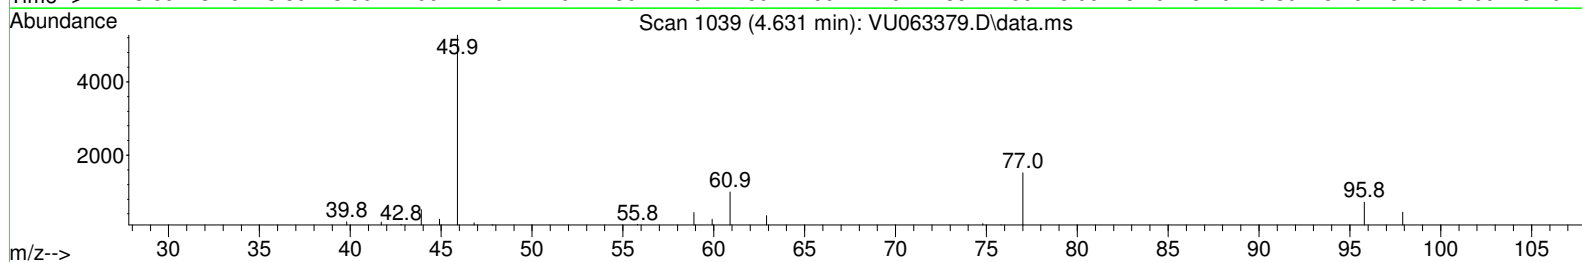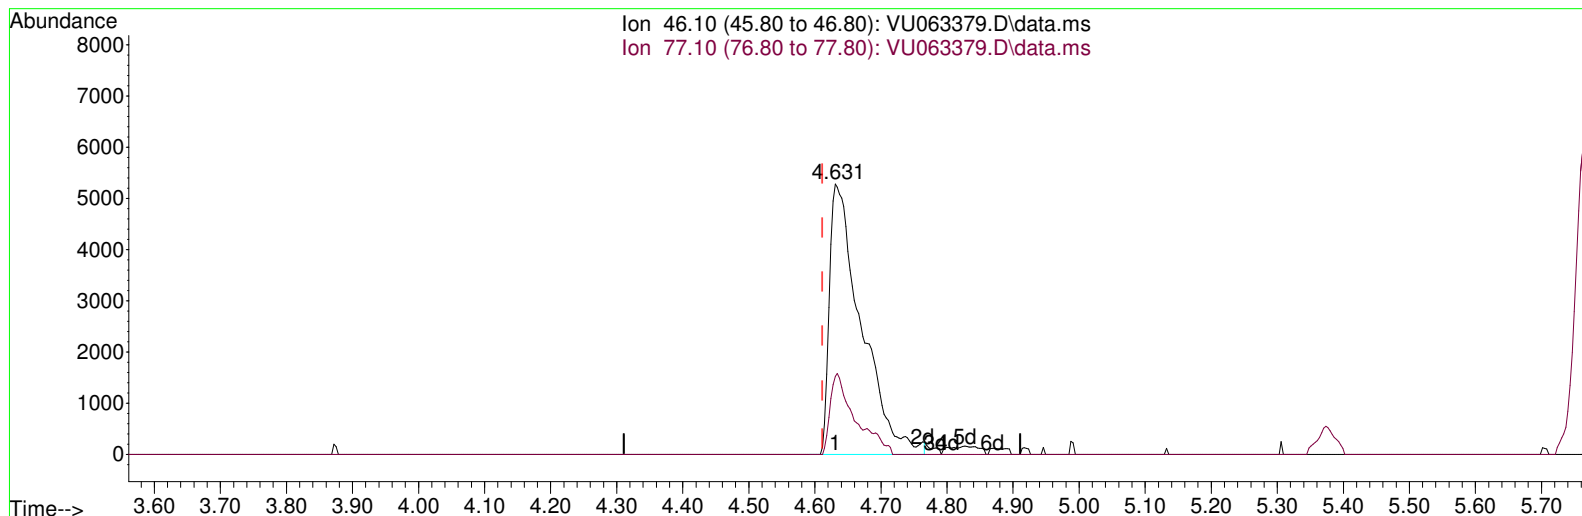

(21) 2-Butanone-d5 (S)

4.631min (+ 0.020) 20.03 ug/L m

response 17605

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.30	18.89
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063379.D
Acq On : 11 Jun 2025 11:48
Operator : MD/SY
Sample : VSTD01034
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD010034

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 11 13:21:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:19:23 2025
Response via : Initial Calibration

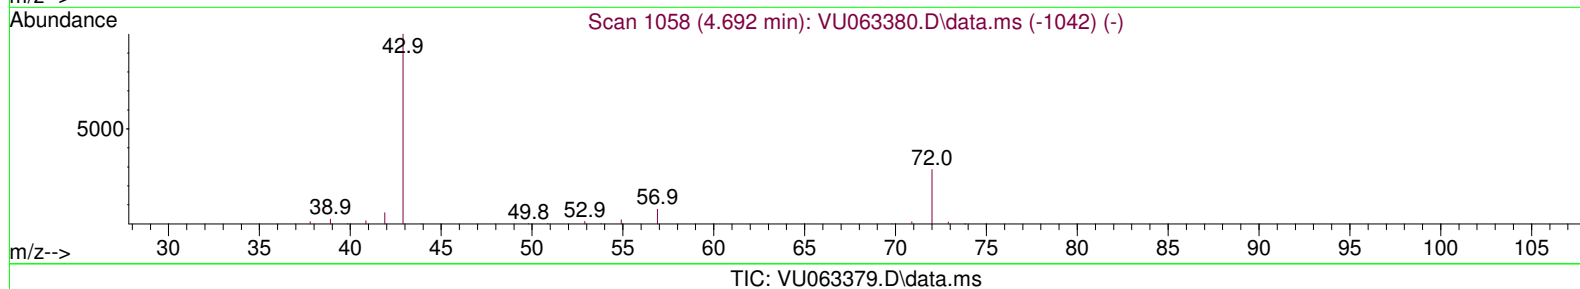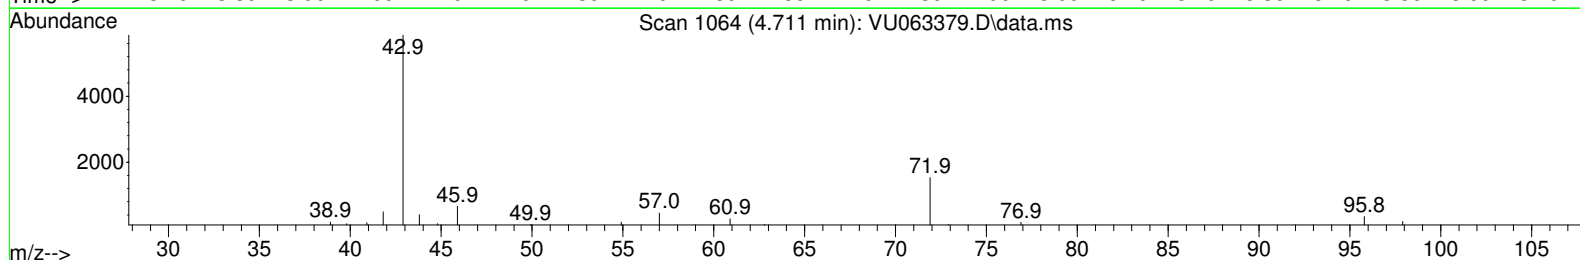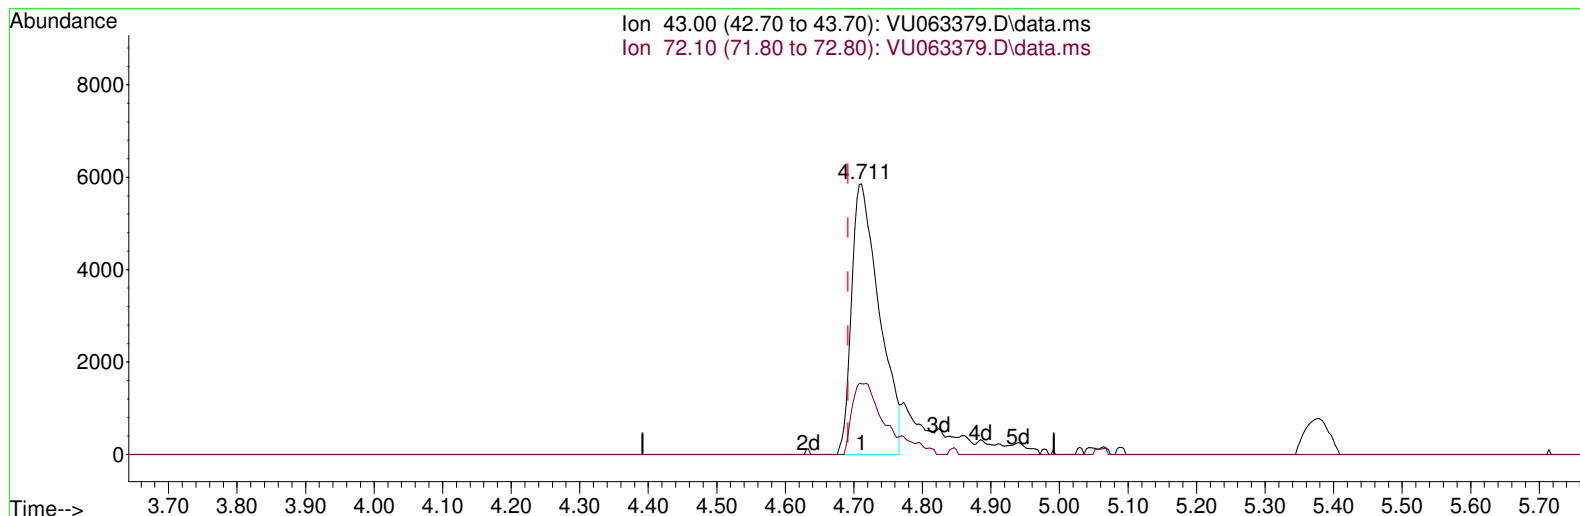

(22) 2-Butanone (T)

4.711min (+ 0.019) 18.97 ug/L

response 16431

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	30.90	11.59#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063379.D
Acq On : 11 Jun 2025 11:48
Operator : MD/SY
Sample : VSTD01034
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD010034

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 11 13:21:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:19:23 2025
Response via : Initial Calibration

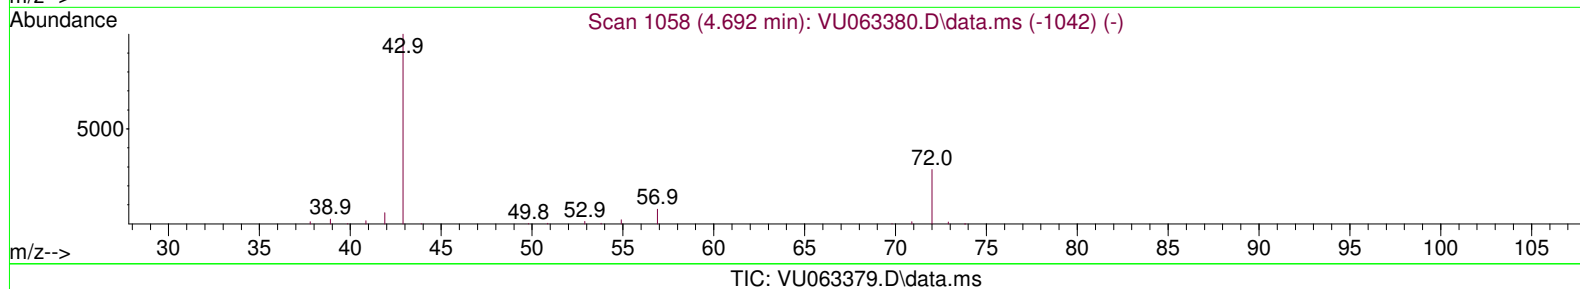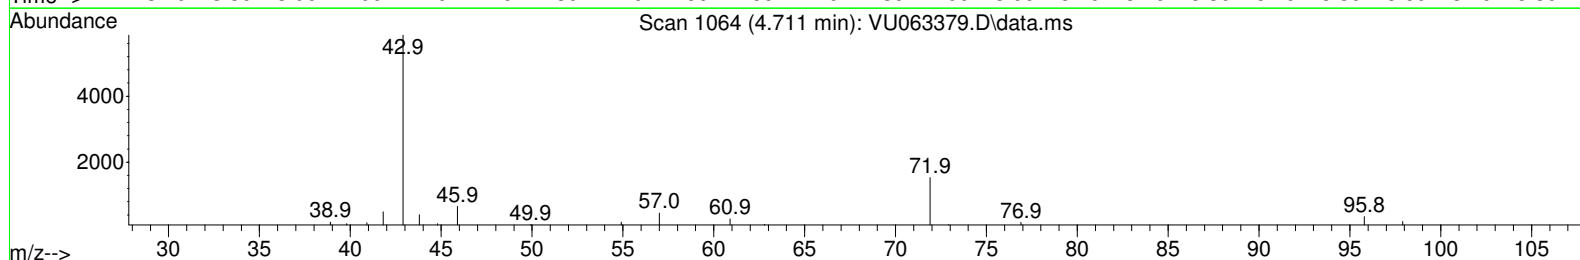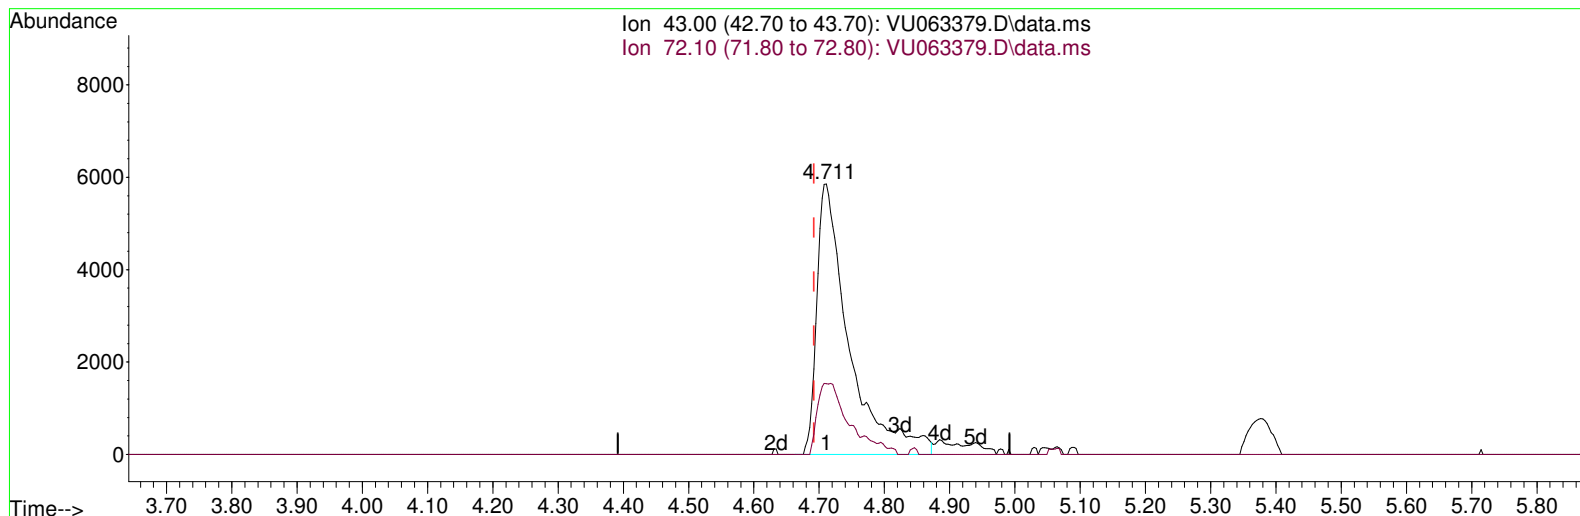

(22) 2-Butanone (T)

4.711min (+ 0.019) 23.06 ug/L m

response 19972

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	30.90	9.54#
0.00	0.00	0.00
0.00	0.00	0.00