




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063386.D
Acq On : 11 Jun 2025 16:24
Operator : MD/SY
Sample : Q2117-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 12 08:31:51 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:45:27 2025
Response via : Initial Calibration

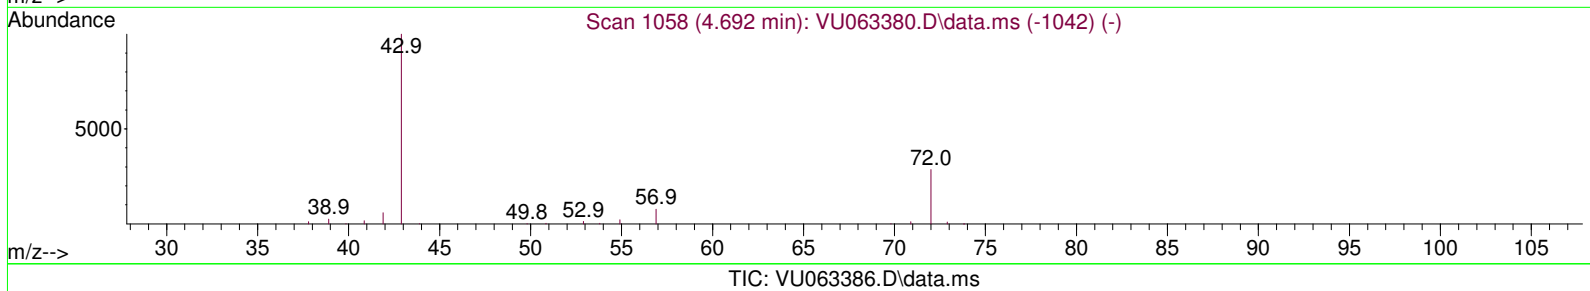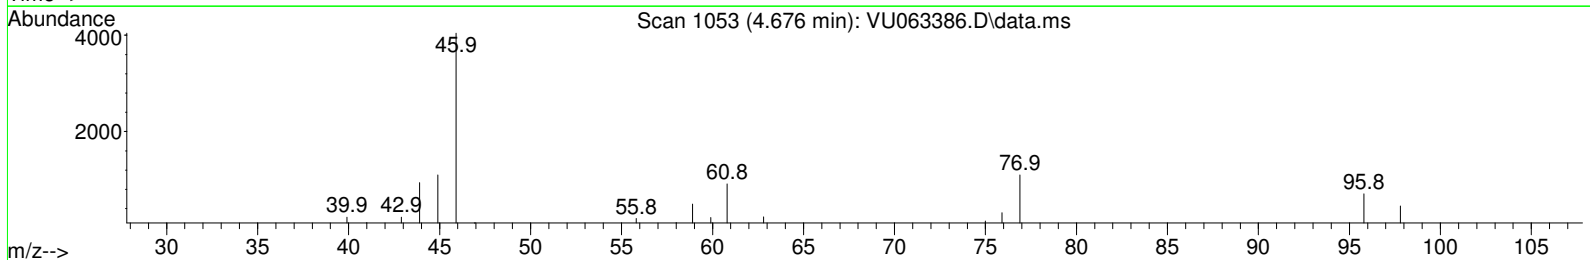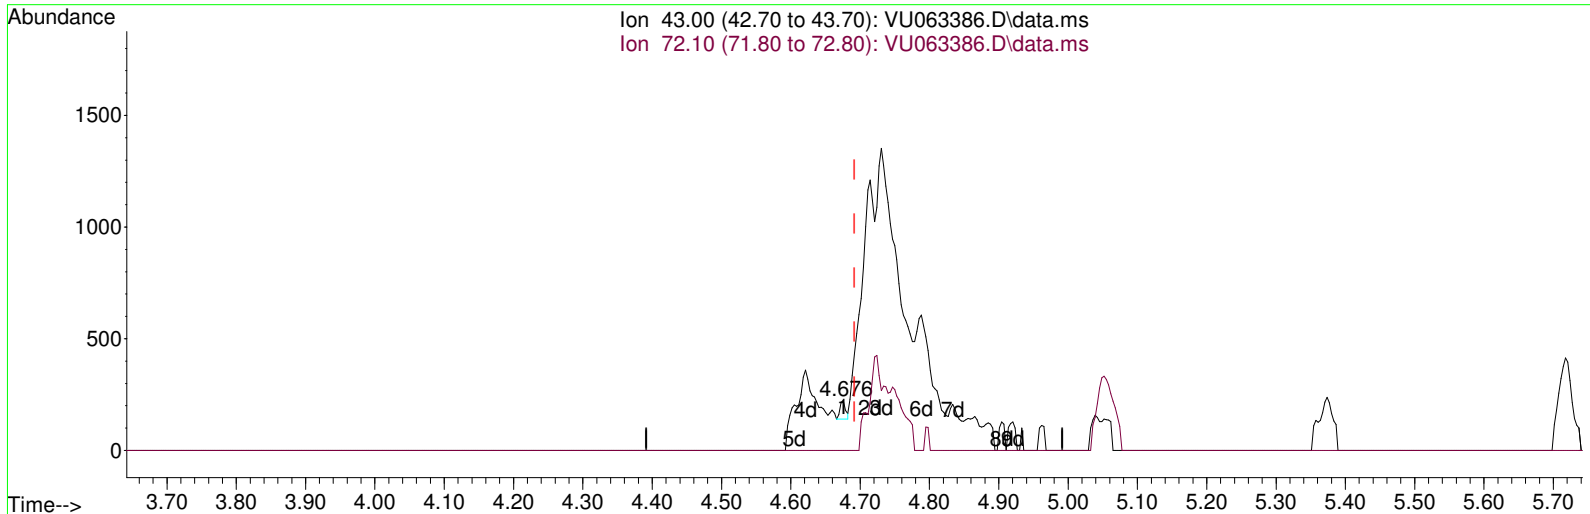

(22) 2-Butanone (T)

4.676min (-0.016) 0.04 ug/L

response 46

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	30.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063386.D
Acq On : 11 Jun 2025 16:24
Operator : MD/SY
Sample : Q2117-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 12 08:31:51 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:45:27 2025
Response via : Initial Calibration

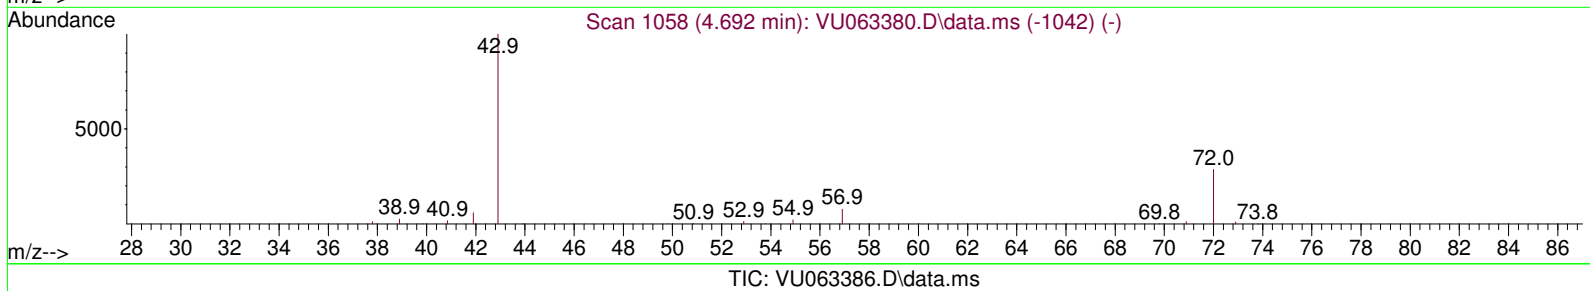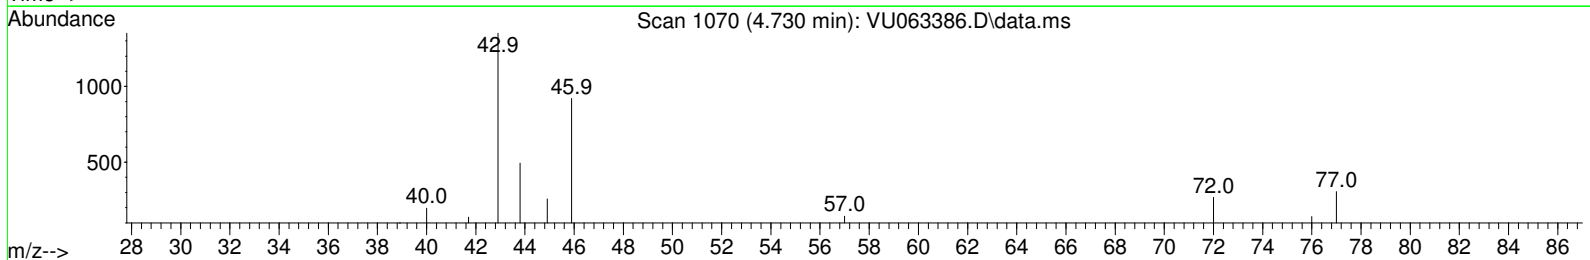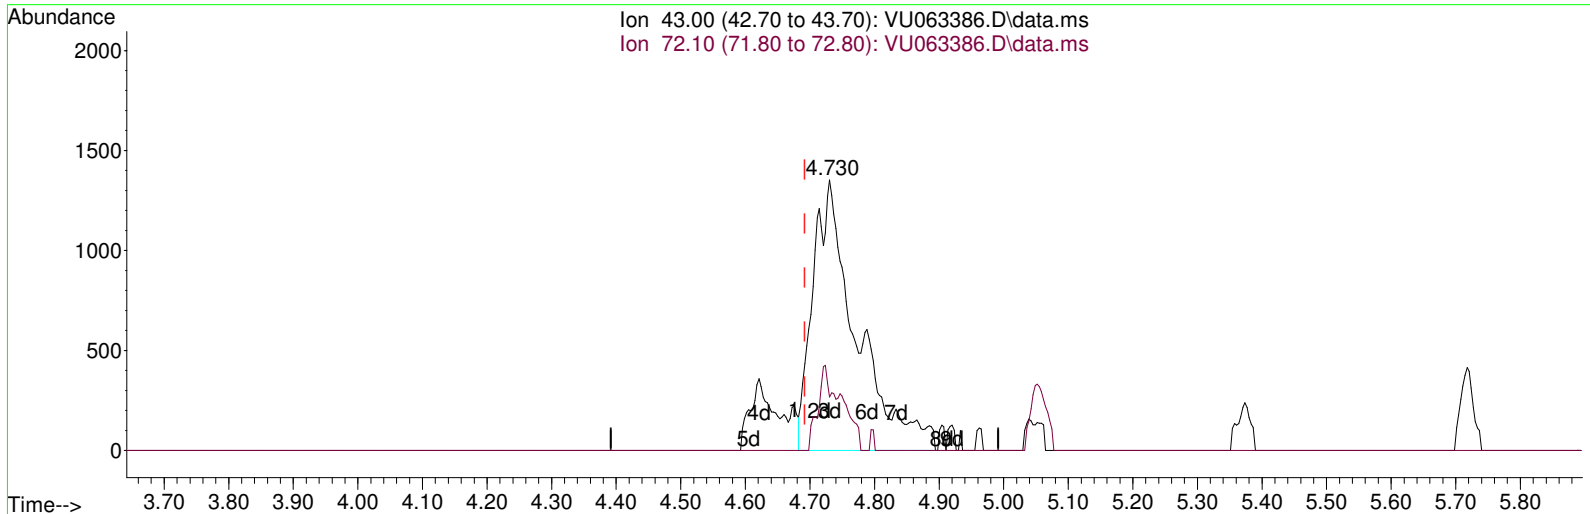

(22) 2-Butanone (T)

4.730min (+ 0.039) 6.15 ug/L m

response 6347

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	30.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063386.D
Acq On : 11 Jun 2025 16:24
Operator : MD/SY
Sample : Q2117-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 12 08:31:51 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:45:27 2025
Response via : Initial Calibration

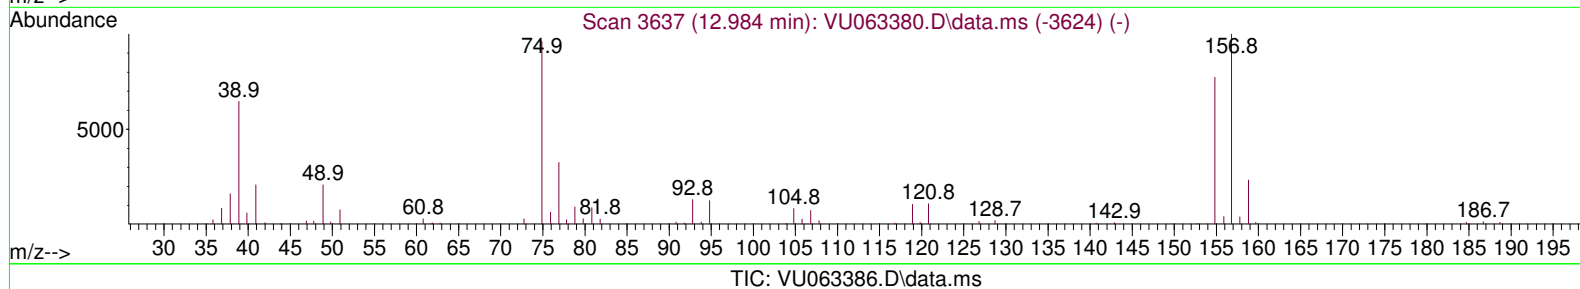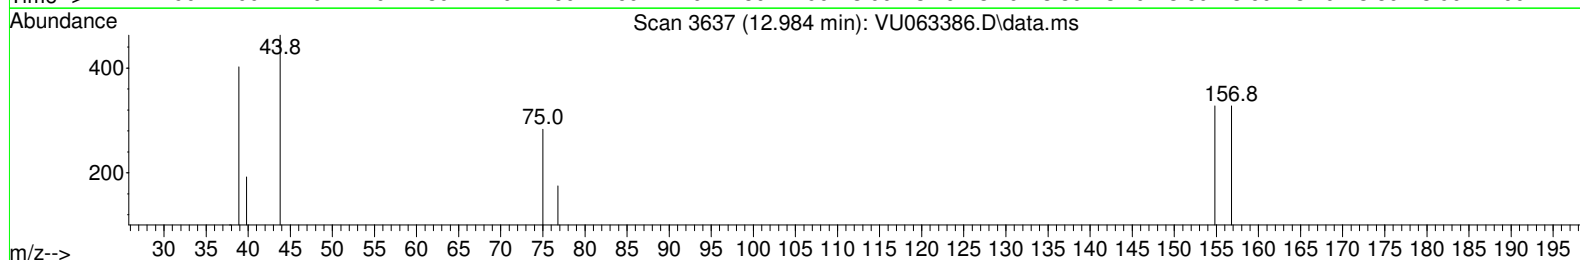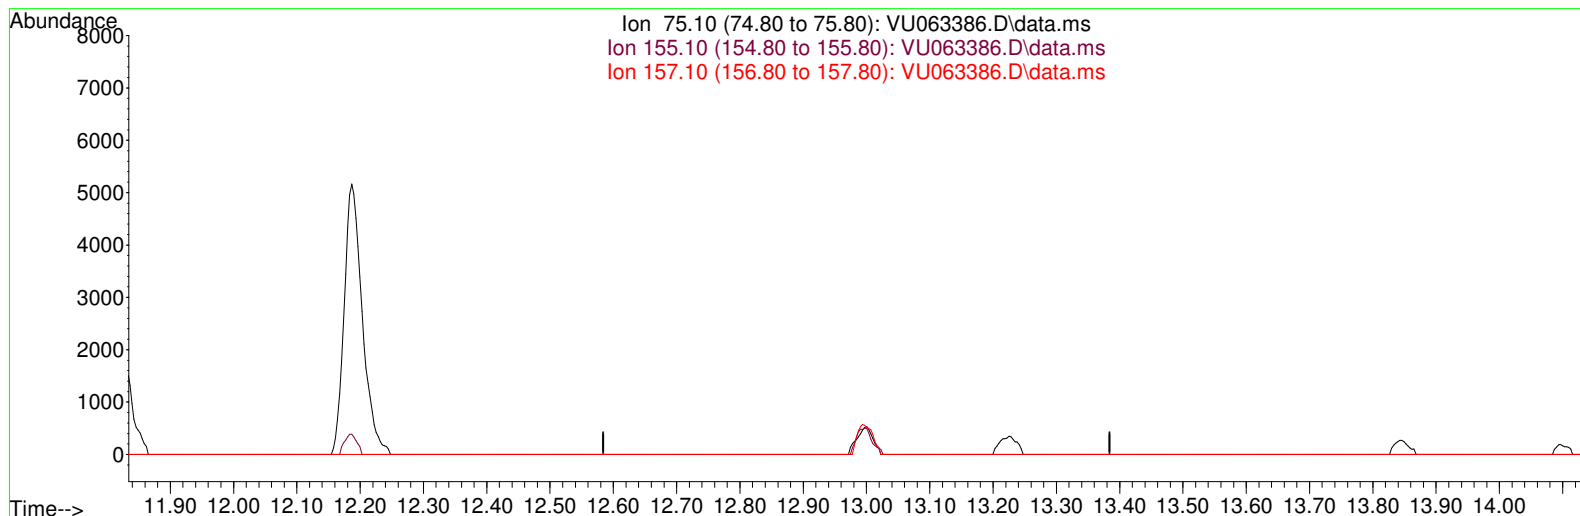

(68) 1,2-Dibromo-3-chloropropane (T)

12.984min (-12.984) 0.00 ug/L

response 0

Ion	Exp%	Act%
75.10	100.00	0.00
155.10	85.50	0.00#
157.10	105.30	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063386.D
Acq On : 11 Jun 2025 16:24
Operator : MD/SY
Sample : Q2117-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/12/2025
Supervised By :Mahesh Dadoda 06/12/2025

Quant Time: Jun 12 08:31:51 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 11 13:45:27 2025
Response via : Initial Calibration

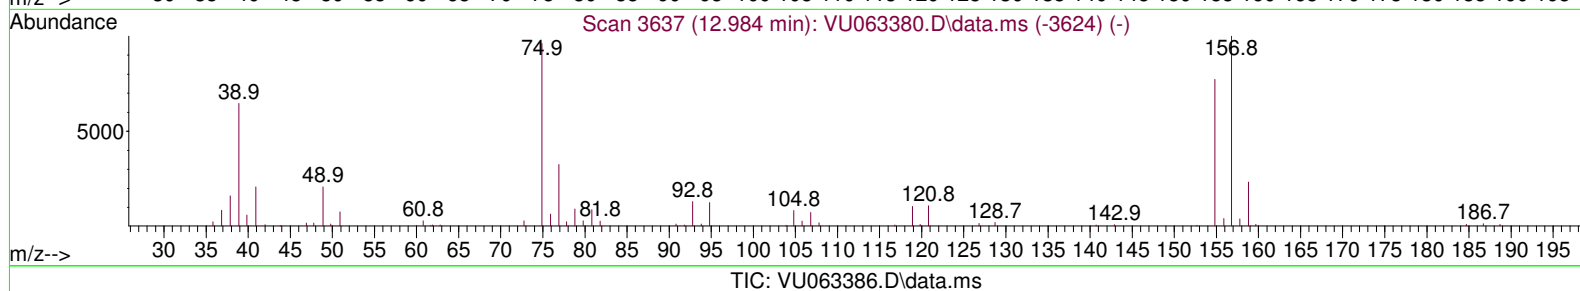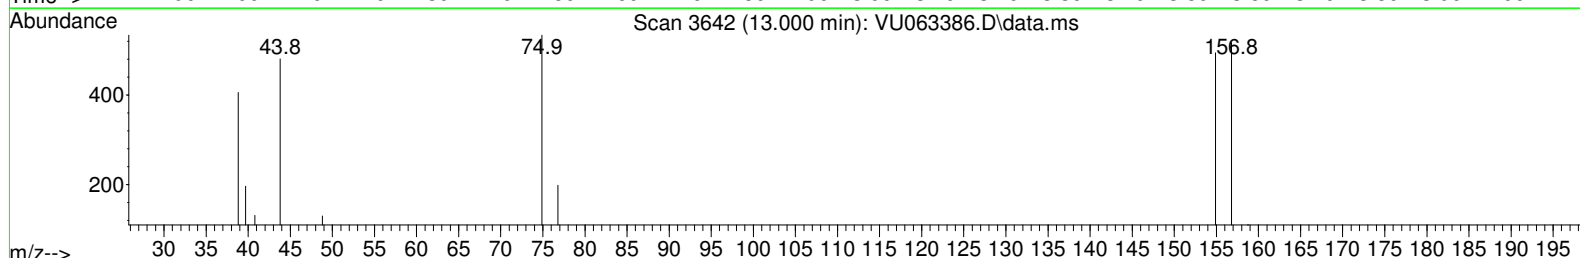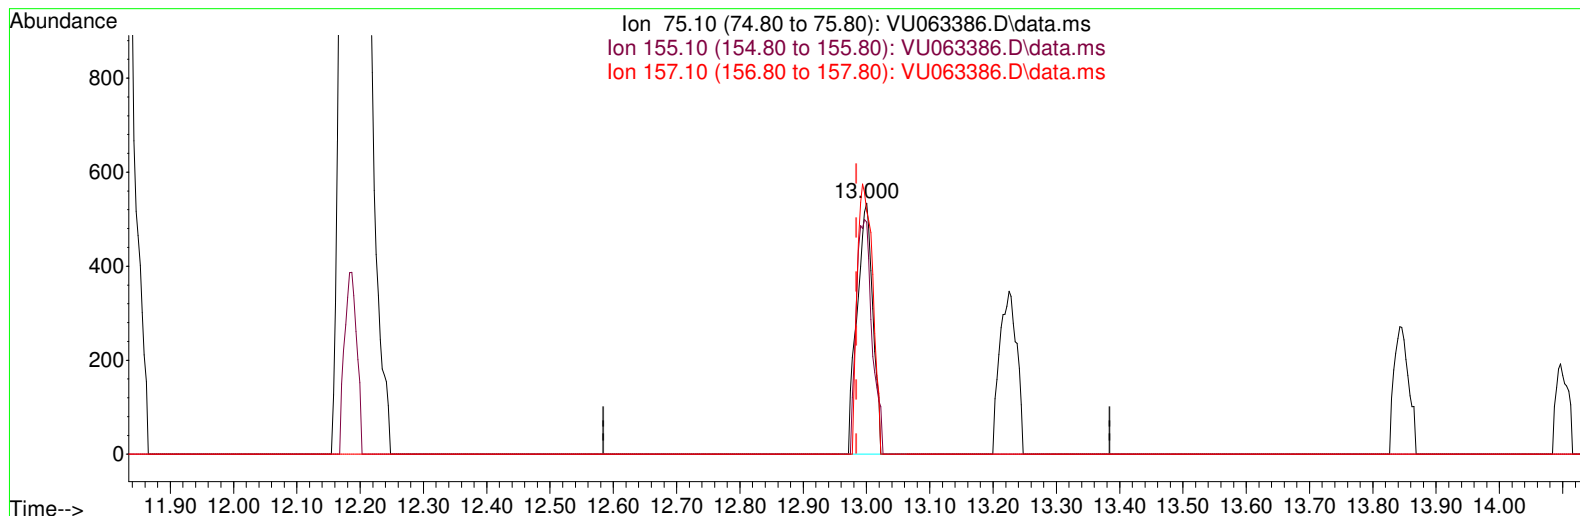

(68) 1,2-Dibromo-3-chloropropane (T)

13.000min (+ 0.016) 2.13 ug/L m

response 926

Ion	Exp%	Act%
75.10	100.00	100.00
155.10	85.50	92.51
157.10	105.30	96.82
0.00	0.00	0.00