
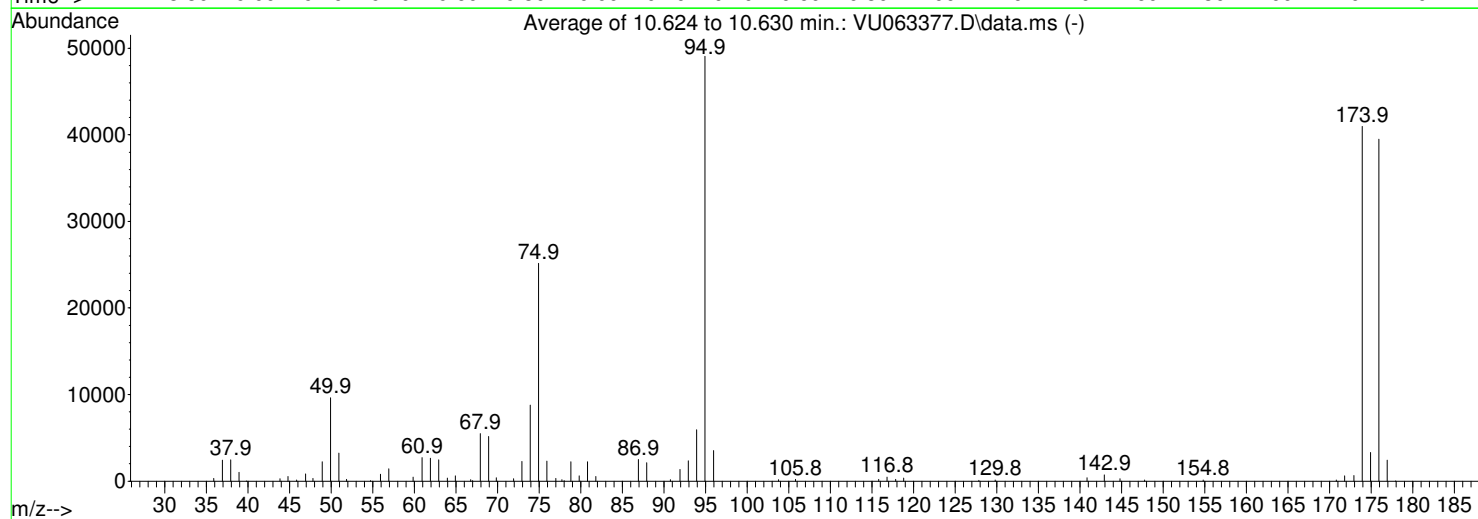


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061125\
Data File : VU063377.D
Acq On : 11 Jun 2025 10:49
Operator : MD/SY
Sample : BFB086
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB086

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061125WMA.M
Title : VOC Analysis
Last Update : Wed Jun 11 13:45:27 2025

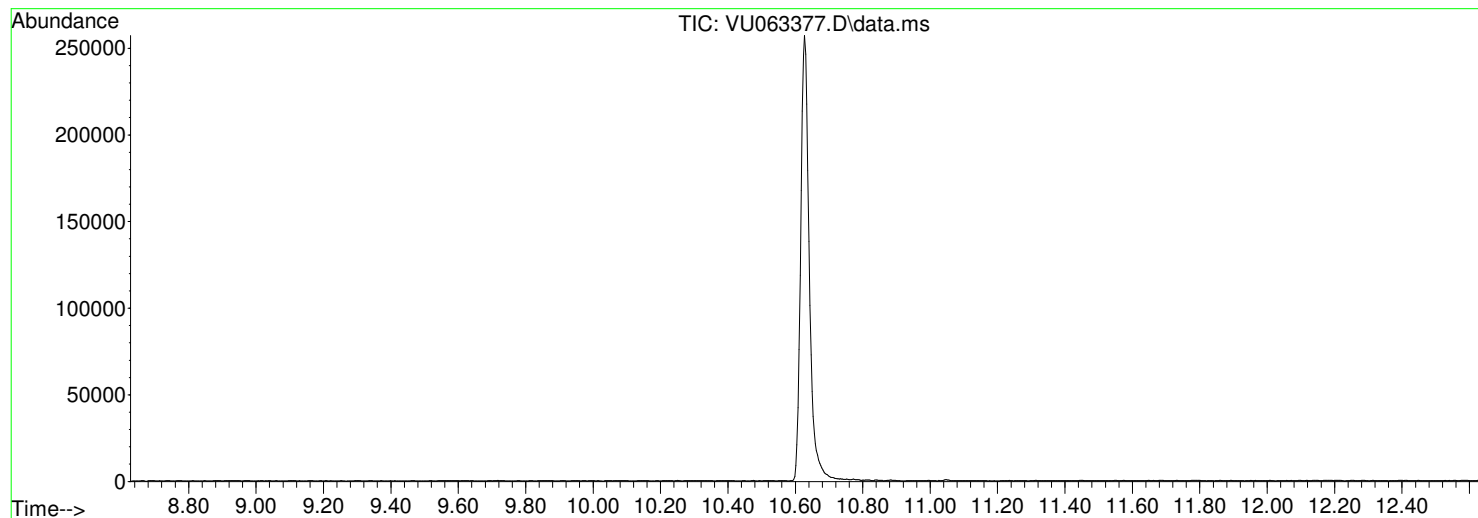

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	9619	PASS
75	95	30	80	51.3	25171	PASS
95	95	100	100	100.0	49075	PASS
96	95	5	9	7.2	3546	PASS
173	174	0.00	2	1.5	634	PASS
174	95	50	120	83.5	40960	PASS
175	174	5	9	8.1	3308	PASS
176	174	95	101	96.4	39491	PASS
177	176	5	9	6.2	2433	PASS

m/z	Abundance
39.80	153.0
43.90	303.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086

m/z	Abundance
35.90	296.0
36.90	2388.0
37.90	2539.0
38.90	1003.0
39.80	216.0
43.80	633.0
44.80	515.0
45.80	108.0
46.90	806.0
47.80	364.0
48.90	2288.0
49.90	9612.0
50.90	3176.0
51.80	206.0
55.90	789.0
56.90	1316.0
59.90	432.0
60.90	2656.0
61.90	2741.0
62.90	2404.0
63.90	315.0
64.90	617.0
66.70	156.0
67.00	145.0
67.90	5512.0
68.90	5208.0
69.80	400.0
71.90	268.0
72.90	2257.0
73.90	8621.0
74.90	24992.0
75.90	2326.0
77.00	281.0
77.70	267.0
78.80	2256.0
79.80	519.0
80.80	2236.0
81.80	593.0
86.90	2491.0
87.90	2172.0
90.70	182.0
91.90	1201.0
92.90	2294.0
93.90	5780.0
94.90	48248.0
96.00	3587.0
103.80	170.0
105.80	201.0
115.80	204.0
116.80	478.0
117.90	186.0
118.80	309.0
129.80	122.0
140.90	353.0
142.90	730.0
144.80	304.0
147.80	131.0
154.80	131.0
170.80	148.0
171.80	551.0
172.90	590.0
173.90	39896.0
174.90	3173.0
175.90	38296.0
176.90	2331.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086

m/z	Abundance
35.80	338.0
36.90	2506.0
37.90	2552.0
38.90	1062.0
39.80	179.0
43.80	587.0
44.80	583.0
45.90	117.0
46.90	848.0
47.80	301.0
48.90	2271.0
49.90	9846.0
50.90	3342.0
51.80	228.0
55.90	796.0
56.90	1468.0
59.80	462.0
60.90	2829.0
61.90	2712.0
62.90	2517.0
64.00	329.0
64.90	620.0
66.70	150.0
67.90	5725.0
68.90	5300.0
69.90	409.0
71.90	294.0
72.90	2354.0
73.90	8996.0
74.90	26000.0
75.90	2412.0
77.00	316.0
77.70	246.0
78.80	2317.0
79.80	628.0
80.80	2291.0
81.80	533.0
86.90	2570.0
87.90	2217.0
90.70	178.0
91.90	1405.0
92.90	2387.0
93.90	6103.0
94.90	50456.0
95.90	3670.0
103.80	170.0
105.80	222.0
115.80	191.0
116.80	467.0
117.90	212.0
118.80	360.0
127.90	120.0
129.80	119.0
140.80	381.0
142.90	752.0
144.80	284.0
147.70	125.0
154.80	157.0
170.80	148.0
171.80	642.0
172.90	652.0
173.90	42176.0
174.90	3475.0
175.90	40704.0
176.90	2504.0
177.90	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086

m/z	Abundance
35.80	340.0
36.90	2407.0
37.90	2308.0
38.90	978.0
39.80	153.0
43.90	572.0
44.80	518.0
45.90	118.0
46.90	793.0
47.80	247.0
48.90	2114.0
49.90	9400.0
50.90	3152.0
51.90	216.0
54.70	129.0
55.90	755.0
56.90	1450.0
59.80	498.0
60.90	2631.0
61.90	2530.0
62.90	2414.0
64.00	359.0
64.90	592.0
66.80	147.0
67.90	5271.0
68.90	5018.0
69.90	369.0
71.90	279.0
72.90	2193.0
73.90	8681.0
74.90	24520.0
75.90	2233.0
77.00	377.0
78.00	222.0
78.80	2123.0
79.80	650.0
80.80	2231.0
81.80	434.0
86.90	2445.0
87.90	2033.0
90.80	163.0
91.90	1439.0
92.90	2337.0
93.90	5900.0
94.90	48520.0
95.90	3381.0
103.70	166.0
105.80	222.0
115.80	178.0
116.80	418.0
117.80	205.0
118.80	337.0
127.80	135.0
129.80	118.0
140.80	424.0
142.90	718.0
144.80	269.0
147.70	103.0
154.80	142.0
170.80	134.0
171.80	680.0
172.90	661.0
173.90	40808.0
174.90	3277.0
175.90	39472.0
176.90	2465.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086