

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061219\
 Data File : VU032667.D
 Acq On : 12 Jun 2019 21:05
 Operator : JC/SP
 Sample : K3313-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLY9

Quant Time: Jun 13 07:01:31 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 13 05:57:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	167427	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	160502	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	78294	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	50055	46.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.16%
7) Chloroethane-d5	1.68	69	41463	47.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.00%
11) 1,1-Dichloroethene-d2	2.27	63	76204	35.83	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.66%
21) 2-Butanone-d5	4.17	46	88057	96.87	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.87%
24) Chloroform-d	4.64	84	96789	47.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.56%
26) 1,2-Dichloroethane-d4	5.30	65	64969	50.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.82%
32) Benzene-d6	5.33	84	193733	46.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.98%
36) 1,2-Dichloropropane-d6	6.32	67	61861	47.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.70%
41) Toluene-d8	7.56	98	176577	44.69	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.38%
43) trans-1,3-Dichloropropene-	7.85	79	27336	43.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.44%
47) 2-Hexanone-d5	8.31	63	49828	78.62	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	78.62%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	86384	45.63	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.26%
64) 1,2-Dichlorobenzene-d4	11.86	152	72493	48.34	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.68%


Target Compounds					Ovalue
13) Acetone	2.32	43	2584	2.755 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061219\
Data File : VU032667.D
Acq On : 12 Jun 2019 21:05
Operator : JC/SP
Sample : K3313-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LY9

Quant Time: Jun 13 07:01:31 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 13 05:57:37 2019
Response via : Initial Calibration

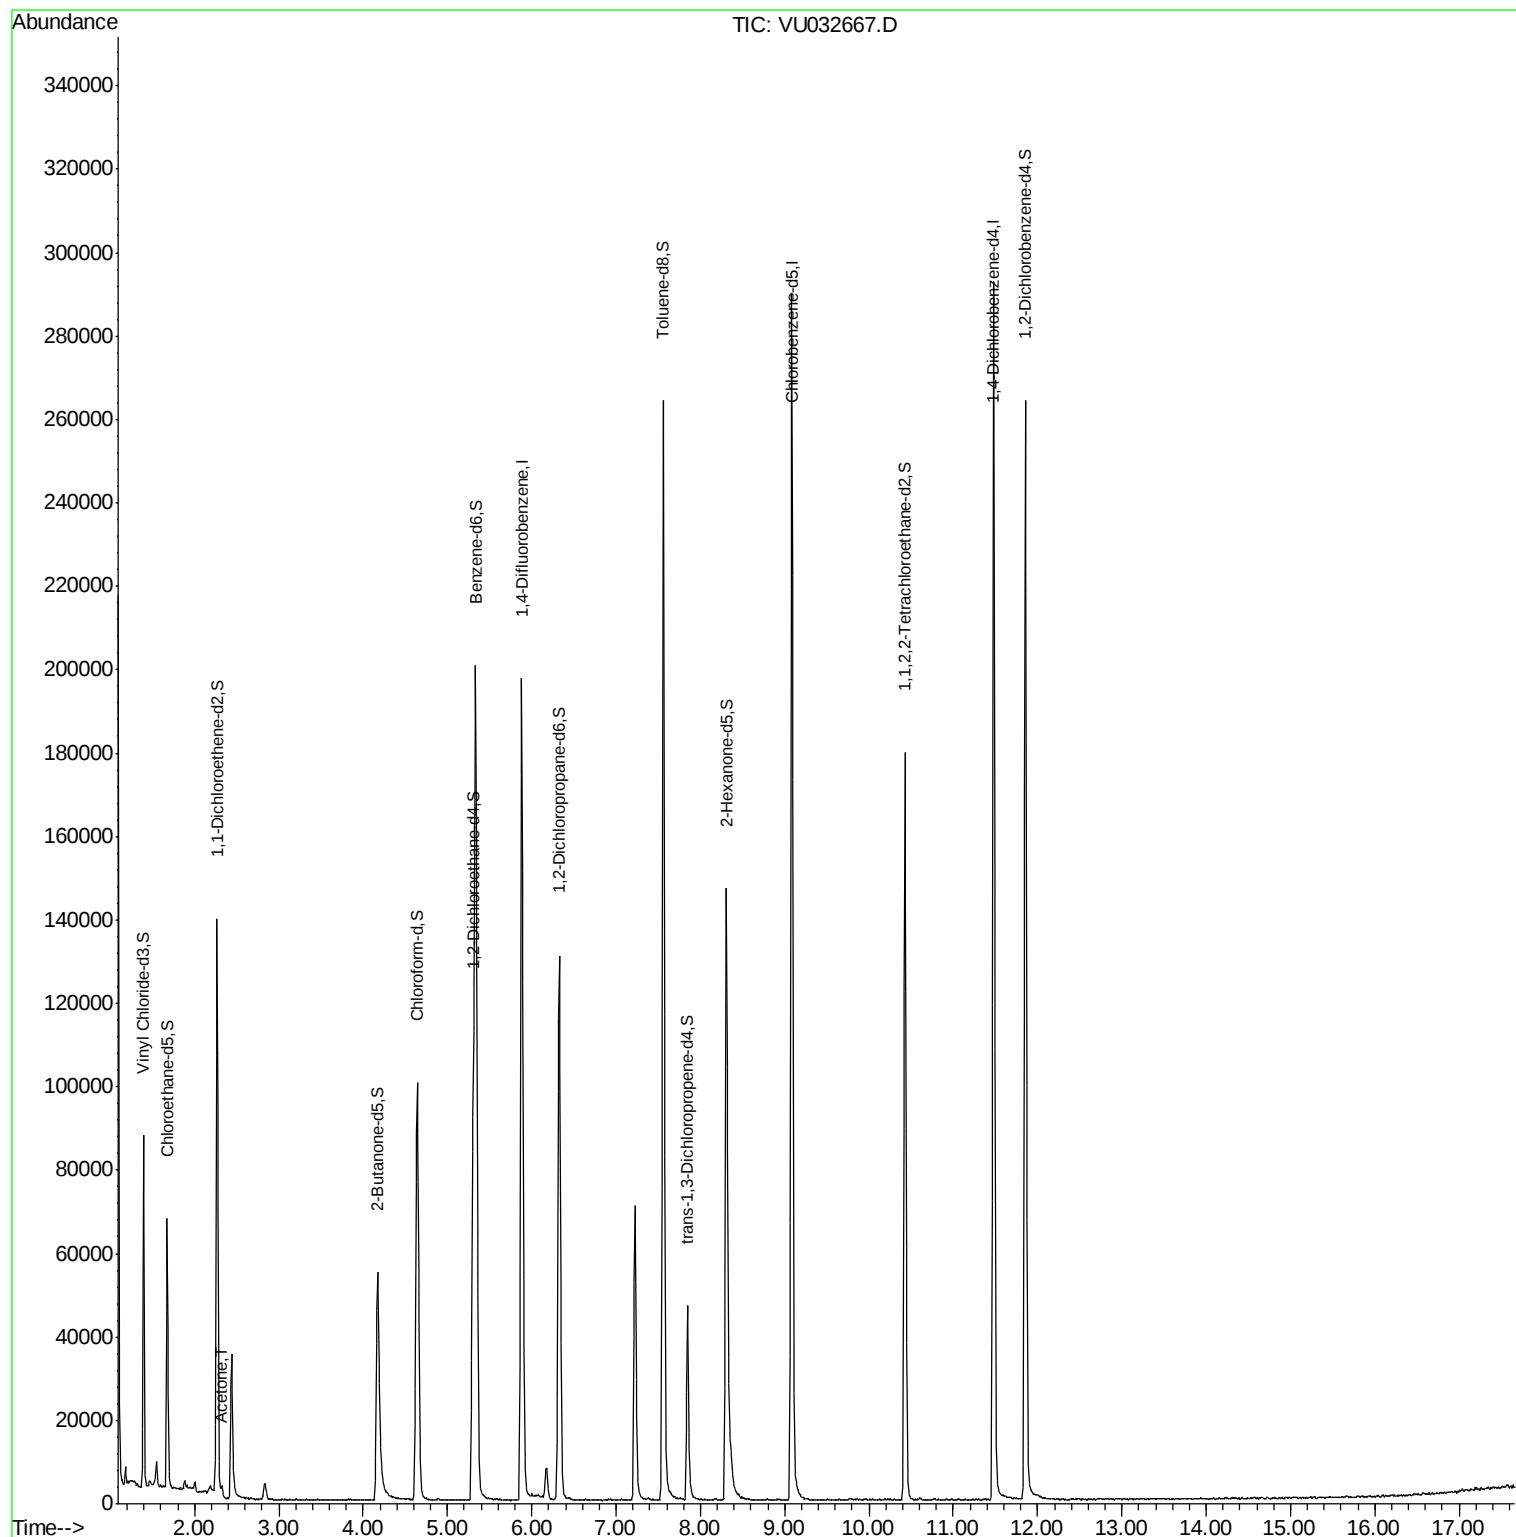

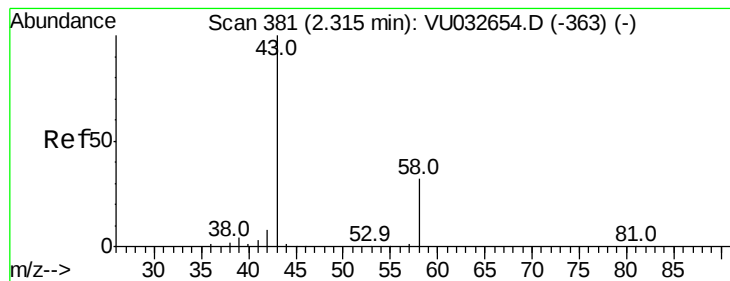

#13

Acetone

Concen: 2.755 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU032667.D

Acq: 12 Jun 2019 21:05

Instrument :
MSVOA_U
ClientSampleId :
COLY9

Tot Ion: 43 Resp: 2584

Ion Ratio Lower Upper

43 100

58 25.2 0.0 64.0

