

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061219\
 Data File : VU032652.D
 Acq On : 12 Jun 2019 15:19
 Operator : JC/SP
 Sample : K3292-08DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8P9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.280	56	59	69	rVB	21881	20525	3.30%	0.384%
2	1.396	89	95	107	rVB	92781	93980	15.11%	1.757%
3	1.672	174	181	197	rVB	67495	85729	13.78%	1.602%
4	2.267	356	366	379	rVB	151631	227393	36.56%	4.251%
5	2.672	490	492	493	rBV	277	125	0.02%	0.002%
6	2.830	530	541	555	rBV	7798	15925	2.56%	0.298%
7	3.232	662	666	668	rBV2	261	219	0.04%	0.004%
8	3.376	708	711	717	rVB2	254	243	0.04%	0.005%
9	3.418	721	724	729	rBV2	228	263	0.04%	0.005%
10	3.701	809	812	815	rBV2	182	108	0.02%	0.002%
11	3.929	880	883	889	rVB2	265	214	0.03%	0.004%
12	3.994	900	903	905	rBV2	165	114	0.02%	0.002%
13	4.171	946	958	994	rBV	58070	158104	25.42%	2.955%
14	4.640	1089	1104	1128	rBV	104750	242018	38.91%	4.524%
15	5.257	1291	1296	1297	rBV	163	137	0.02%	0.003%
16	5.334	1297	1320	1351	rVV2	214093	622043	100.00%	11.627%
17	5.585	1395	1398	1401	rBV2	243	213	0.03%	0.004%
18	5.659	1418	1421	1424	rBV2	197	127	0.02%	0.002%
19	5.730	1440	1443	1446	rBV2	136	73	0.01%	0.001%
20	5.752	1446	1450	1453	rBV2	203	200	0.03%	0.004%
21	5.881	1477	1490	1510	rBV	194497	383607	61.67%	7.171%
22	6.180	1571	1583	1601	rVB	212726	412904	66.38%	7.718%
23	6.325	1616	1628	1650	rVB	138519	276647	44.47%	5.171%
24	6.460	1667	1670	1671	rBV	493	252	0.04%	0.005%
25	6.646	1725	1728	1734	rVB2	514	602	0.10%	0.011%
26	6.672	1734	1736	1738	rBV	195	89	0.01%	0.002%
27	6.698	1742	1744	1745	rBV2	201	86	0.01%	0.002%
28	7.006	1837	1840	1842	rBV2	242	136	0.02%	0.003%
29	7.064	1854	1858	1861	rBV2	281	229	0.04%	0.004%
30	7.113	1869	1873	1877	rBV4	392	353	0.06%	0.007%
31	7.135	1878	1880	1884	rVV2	215	93	0.01%	0.002%
32	7.158	1884	1887	1890	rVV2	236	138	0.02%	0.003%
33	7.222	1896	1907	1928	rBV	78555	143286	23.03%	2.678%
34	7.379	1954	1956	1960	rVB2	359	188	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061219\
 Data File : VU032652.D
 Acq On : 12 Jun 2019 15:19
 Operator : JC/SP
 Sample : K3292-08DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8P9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

35	7.405	1960	1964	1967	rBV	203	199	0.03%	0.004%
36	7.424	1967	1970	1972	rVV	315	180	0.03%	0.003%
37	7.460	1976	1981	1983	rBV	481	357	0.06%	0.007%
38	7.473	1983	1985	1990	rVB2	409	268	0.04%	0.005%
39	7.559	2000	2012	2033	rBV	286263	498694	80.17%	9.322%
40	7.846	2088	2101	2125	rBV2	52710	93725	15.07%	1.752%
41	8.035	2157	2160	2166	rVB2	191	136	0.02%	0.003%
42	8.164	2193	2200	2203	rBV2	519	646	0.10%	0.012%
43	8.225	2215	2219	2225	rVB4	1242	1366	0.22%	0.026%
44	8.260	2225	2230	2234	rBV	267	265	0.04%	0.005%
45	8.305	2234	2244	2275	rBV	169324	316518	50.88%	5.916%
46	8.569	2321	2326	2331	rBV2	488	613	0.10%	0.011%
47	8.608	2336	2338	2340	rVV	113	47	0.01%	0.001%
48	8.717	2369	2372	2374	rVB	182	95	0.02%	0.002%
49	8.743	2377	2380	2382	rBV	350	216	0.03%	0.004%
50	8.830	2403	2407	2408	rBV	276	164	0.03%	0.003%
51	8.862	2415	2417	2420	rBV	210	143	0.02%	0.003%
52	8.891	2423	2426	2428	rBV2	189	115	0.02%	0.002%
53	8.903	2428	2430	2433	rBV2	242	136	0.02%	0.003%
54	8.945	2439	2443	2445	rVB	248	175	0.03%	0.003%
55	8.961	2445	2448	2451	rBV	206	157	0.03%	0.003%
56	9.029	2465	2469	2471	rBV	276	191	0.03%	0.004%
57	9.084	2475	2486	2527	rBV	278954	474055	76.21%	8.861%
58	9.248	2531	2537	2538	rBV	943	719	0.12%	0.013%
59	9.357	2568	2571	2573	rBV2	243	127	0.02%	0.002%
60	9.379	2573	2578	2584	rBV4	599	877	0.14%	0.016%
61	9.489	2610	2612	2615	rVB	175	98	0.02%	0.002%
62	9.508	2615	2618	2624	rBV2	236	253	0.04%	0.005%
63	9.543	2626	2629	2630	rBV	124	69	0.01%	0.001%
64	9.601	2640	2647	2653	rBV2	334	471	0.08%	0.009%
65	9.627	2653	2655	2657	rBV2	143	84	0.01%	0.002%
66	9.756	2690	2695	2697	rBV2	223	190	0.03%	0.004%
67	9.781	2701	2703	2706	rBV2	205	124	0.02%	0.002%
68	9.849	2722	2724	2726	rBV	151	90	0.01%	0.002%
69	9.894	2736	2738	2740	rBV	113	71	0.01%	0.001%
70	10.074	2790	2794	2795	rBV	188	119	0.02%	0.002%
71	10.167	2816	2823	2832	rBV2	834	1311	0.21%	0.025%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061219\
 Data File : VU032652.D
 Acq On : 12 Jun 2019 15:19
 Operator : JC/SP
 Sample : K3292-08DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8P9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

72	10.264	2848	2853	2856	rVB2	278	236	0.04%	0.004%
73	10.289	2858	2861	2865	rBV	196	164	0.03%	0.003%
74	10.428	2893	2904	2925	rBV	190201	308263	49.56%	5.762%
75	10.604	2954	2959	2964	rVB2	380	438	0.07%	0.008%
76	10.643	2968	2971	2973	rBV	205	133	0.02%	0.002%
77	10.701	2986	2989	2992	rBV	182	113	0.02%	0.002%
78	10.739	2999	3001	3004	rVB	172	80	0.01%	0.001%
79	10.755	3004	3006	3009	rBV	137	89	0.01%	0.002%
80	10.791	3014	3017	3022	rVB2	278	212	0.03%	0.004%
81	10.894	3043	3049	3051	rBV2	284	312	0.05%	0.006%
82	11.087	3106	3109	3113	rBV2	360	287	0.05%	0.005%
83	11.241	3153	3157	3161	rBV	319	300	0.05%	0.006%
84	11.292	3169	3173	3176	rBV2	303	277	0.04%	0.005%
85	11.357	3187	3193	3195	rBV	221	217	0.03%	0.004%
86	11.479	3220	3231	3262	rBV	297626	475548	76.45%	8.889%
87	11.794	3325	3329	3332	rBV	269	220	0.04%	0.004%
88	11.855	3336	3348	3378	rVV	287806	478641	76.95%	8.947%
89	12.276	3475	3479	3482	rBV	359	299	0.05%	0.006%
90	12.353	3501	3503	3505	rBV2	196	120	0.02%	0.002%
91	12.897	3665	3672	3682	rBV4	948	1777	0.29%	0.033%
92	13.347	3809	3812	3817	rBV2	249	290	0.05%	0.005%
93	13.553	3872	3876	3878	rBV	333	306	0.05%	0.006%
94	13.903	3983	3985	3986	rBV	289	134	0.02%	0.003%
95	13.961	4000	4003	4009	rVB2	330	319	0.05%	0.006%
96	14.019	4013	4021	4022	rBV2	1118	1306	0.21%	0.024%
97	14.225	4082	4085	4088	rBV2	353	271	0.04%	0.005%


Sum of corrected areas: 5349779

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061219\
Data File : VU032652.D
Acq On : 12 Jun 2019 15:19
Operator : JC/SP
Sample : K3292-08DL 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8P9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

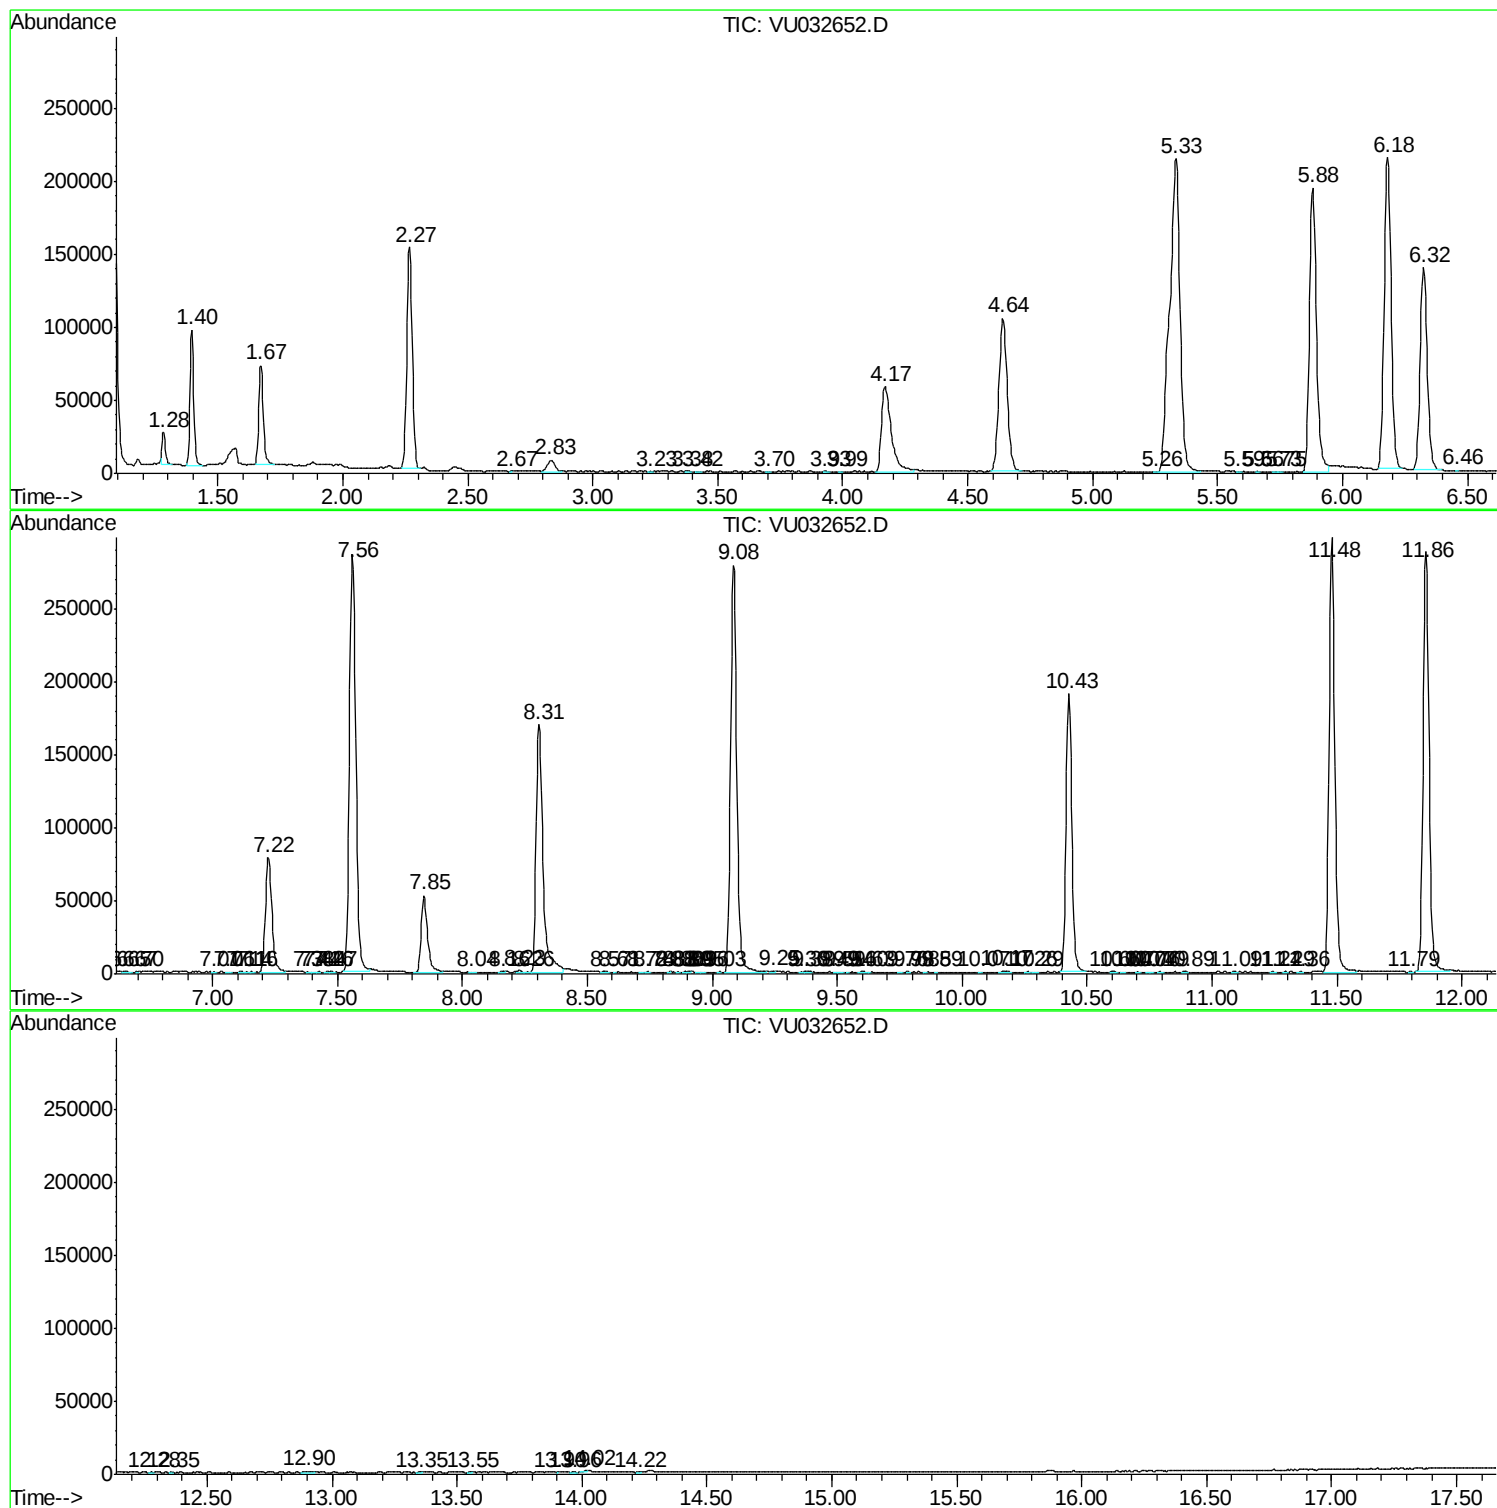

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061219\
Data File : VU032652.D
Acq On : 12 Jun 2019 15:19
Operator : JC/SP
Sample : K3292-08DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8P9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU061219\
Data File : VU032652.D
Acq On : 12 Jun 2019 15:19
Operator : JC/SP
Sample : K3292-08DL 10X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
DB8P9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc