


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061219\
 Data File : VU032636.D
 Acq On : 12 Jun 2019 09:03
 Operator : JC/SP
 Sample : BFB54
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB54

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis
 Last Update : Thu Jun 13 05:57:37 2019

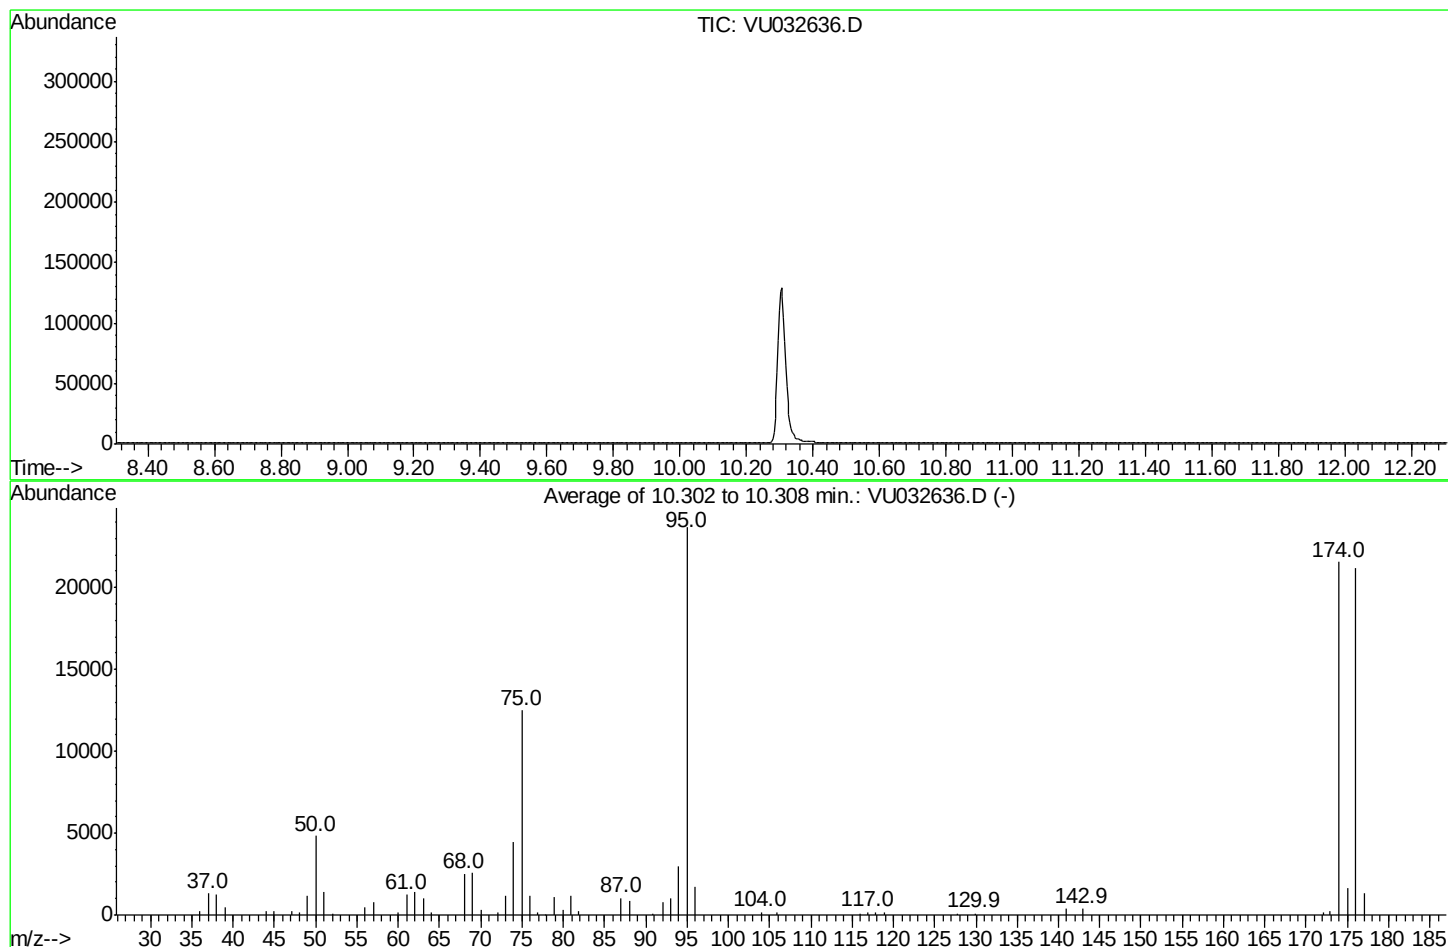

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	4843	PASS
75	95	30	80	52.7	12479	PASS
95	95	100	100	100.0	23682	PASS
96	95	5	9	7.4	1746	PASS
173	174	0.00	2	1.1	231	PASS
174	95	50	120	91.1	21573	PASS
175	174	5	9	7.6	1641	PASS
176	174	95	101	98.3	21210	PASS
177	176	5	9	6.3	1330	PASS

Scan 2854 (10.266 min): VU032636.D
BFB54

m/z	Abundance
39.90	567.0
43.90	304.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
35.90	248.0
37.00	1289.0
38.00	1317.0
39.00	498.0
39.90	537.0
44.00	563.0
44.90	269.0
47.00	267.0
48.00	167.0
49.00	1180.0
50.00	4944.0
51.00	1412.0
52.00	110.0
55.90	523.0
57.00	724.0
60.00	201.0
61.00	1240.0
62.00	1376.0
63.00	1052.0
63.90	121.0
68.00	2635.0
69.00	2779.0
70.00	313.0
72.00	153.0
73.00	1204.0
74.00	4285.0
75.00	12916.0
76.00	1116.0
76.90	159.0
78.90	1152.0
79.90	348.0
80.90	1261.0
81.80	295.0
87.00	1038.0
88.00	809.0
90.90	111.0
92.00	768.0
93.00	1008.0
94.00	3180.0
95.00	23816.0
96.00	1802.0
103.90	173.0
105.90	142.0
116.90	187.0
117.80	133.0
118.80	127.0
129.90	115.0
140.90	359.0
142.90	385.0
172.10	136.0
172.90	233.0
174.00	21360.0
175.00	1591.0
176.00	20432.0
177.00	1359.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
35.90	265.0
37.00	1372.0
38.00	1315.0
39.00	491.0
39.90	500.0
44.00	542.0
45.00	253.0
47.10	280.0
48.00	179.0
49.00	1291.0
50.00	4902.0
51.00	1437.0
52.00	127.0
55.90	488.0
57.10	811.0
60.00	195.0
61.00	1242.0
62.00	1475.0
63.00	1011.0
64.00	125.0
68.00	2597.0
69.00	2703.0
70.00	345.0
72.00	190.0
73.00	1188.0
74.00	4586.0
75.00	12868.0
76.00	1184.0
76.90	137.0
78.90	1139.0
79.90	318.0
80.90	1235.0
81.80	257.0
87.00	1062.0
88.00	850.0
90.90	114.0
92.00	846.0
93.00	1044.0
94.00	3094.0
95.00	24296.0
96.00	1801.0
103.90	170.0
105.90	150.0
115.90	107.0
116.90	183.0
117.80	149.0
118.80	125.0
127.80	116.0
129.90	126.0
140.90	383.0
143.00	397.0
172.10	133.0
173.00	236.0
174.00	22240.0
175.00	1704.0
176.00	21920.0
177.00	1357.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
35.90	228.0
37.00	1306.0
38.00	1215.0
39.00	443.0
39.90	506.0
44.00	456.0
45.00	218.0
47.10	265.0
48.00	149.0
49.00	1170.0
50.00	4683.0
51.00	1350.0
56.00	426.0
57.10	770.0
59.90	197.0
61.00	1164.0
62.00	1422.0
63.00	877.0
64.10	131.0
68.00	2322.0
69.00	2375.0
70.00	320.0
72.00	177.0
73.00	1100.0
74.00	4436.0
75.00	11654.0
76.00	1122.0
76.90	125.0
77.80	106.0
78.90	1046.0
79.90	265.0
80.90	1103.0
81.80	253.0
87.00	1037.0
88.00	843.0
90.90	102.0
92.00	787.0
93.00	996.0
94.00	2722.0
95.00	22936.0
96.00	1636.0
104.00	128.0
105.90	143.0
115.90	113.0
117.00	170.0
117.90	146.0
118.90	113.0
127.80	118.0
129.90	118.0
140.90	352.0
142.90	321.0
172.00	101.0
173.00	226.0
174.00	21120.0
175.00	1628.0
176.00	21280.0
177.00	1276.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54