

Data File : VU038835.D
Acq On : 11 Jun 2020 19:15
Operator : SY/MD
Sample : L2911-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Jun 12 03:48:27 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 12 01:02:05 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	285931	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	286694	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	133201	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	82358	4.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.00%
7) Chloroethane-d5	1.93	69	72617	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.20%
11) 1,1-Dichloroethene-d2	2.59	63	126625	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	4.68	46	333327	59.29	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.58%
24) Chloroform-d	5.10	84	181789	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.60%
26) 1,2-Dichloroethane-d4	5.74	65	110687	5.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.20%
32) Benzene-d6	5.76	84	351431	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
36) 1,2-Dichloropropane-d6	6.72	67	110534	5.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.40%
41) Toluene-d8	7.92	98	284865	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
43) trans-1,3-Dichloropropene-	8.20	79	43712	4.62	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.40%
46) 2-Hexanone-d5	8.65	63	273562	58.53	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	117.06%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	97855	5.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.80%
64) 1,2-Dichlorobenzene-d4	12.20	152	121493	5.29	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.80%


Target Compounds						Qvalue
16) Methylene chloride	3.07	84	3314	0.166	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU038835.D
Acq On : 11 Jun 2020 19:15
Operator : SY/MD
Sample : L2911-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Jun 12 03:48:27 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 12 01:02:05 2020
Response via : Initial Calibration

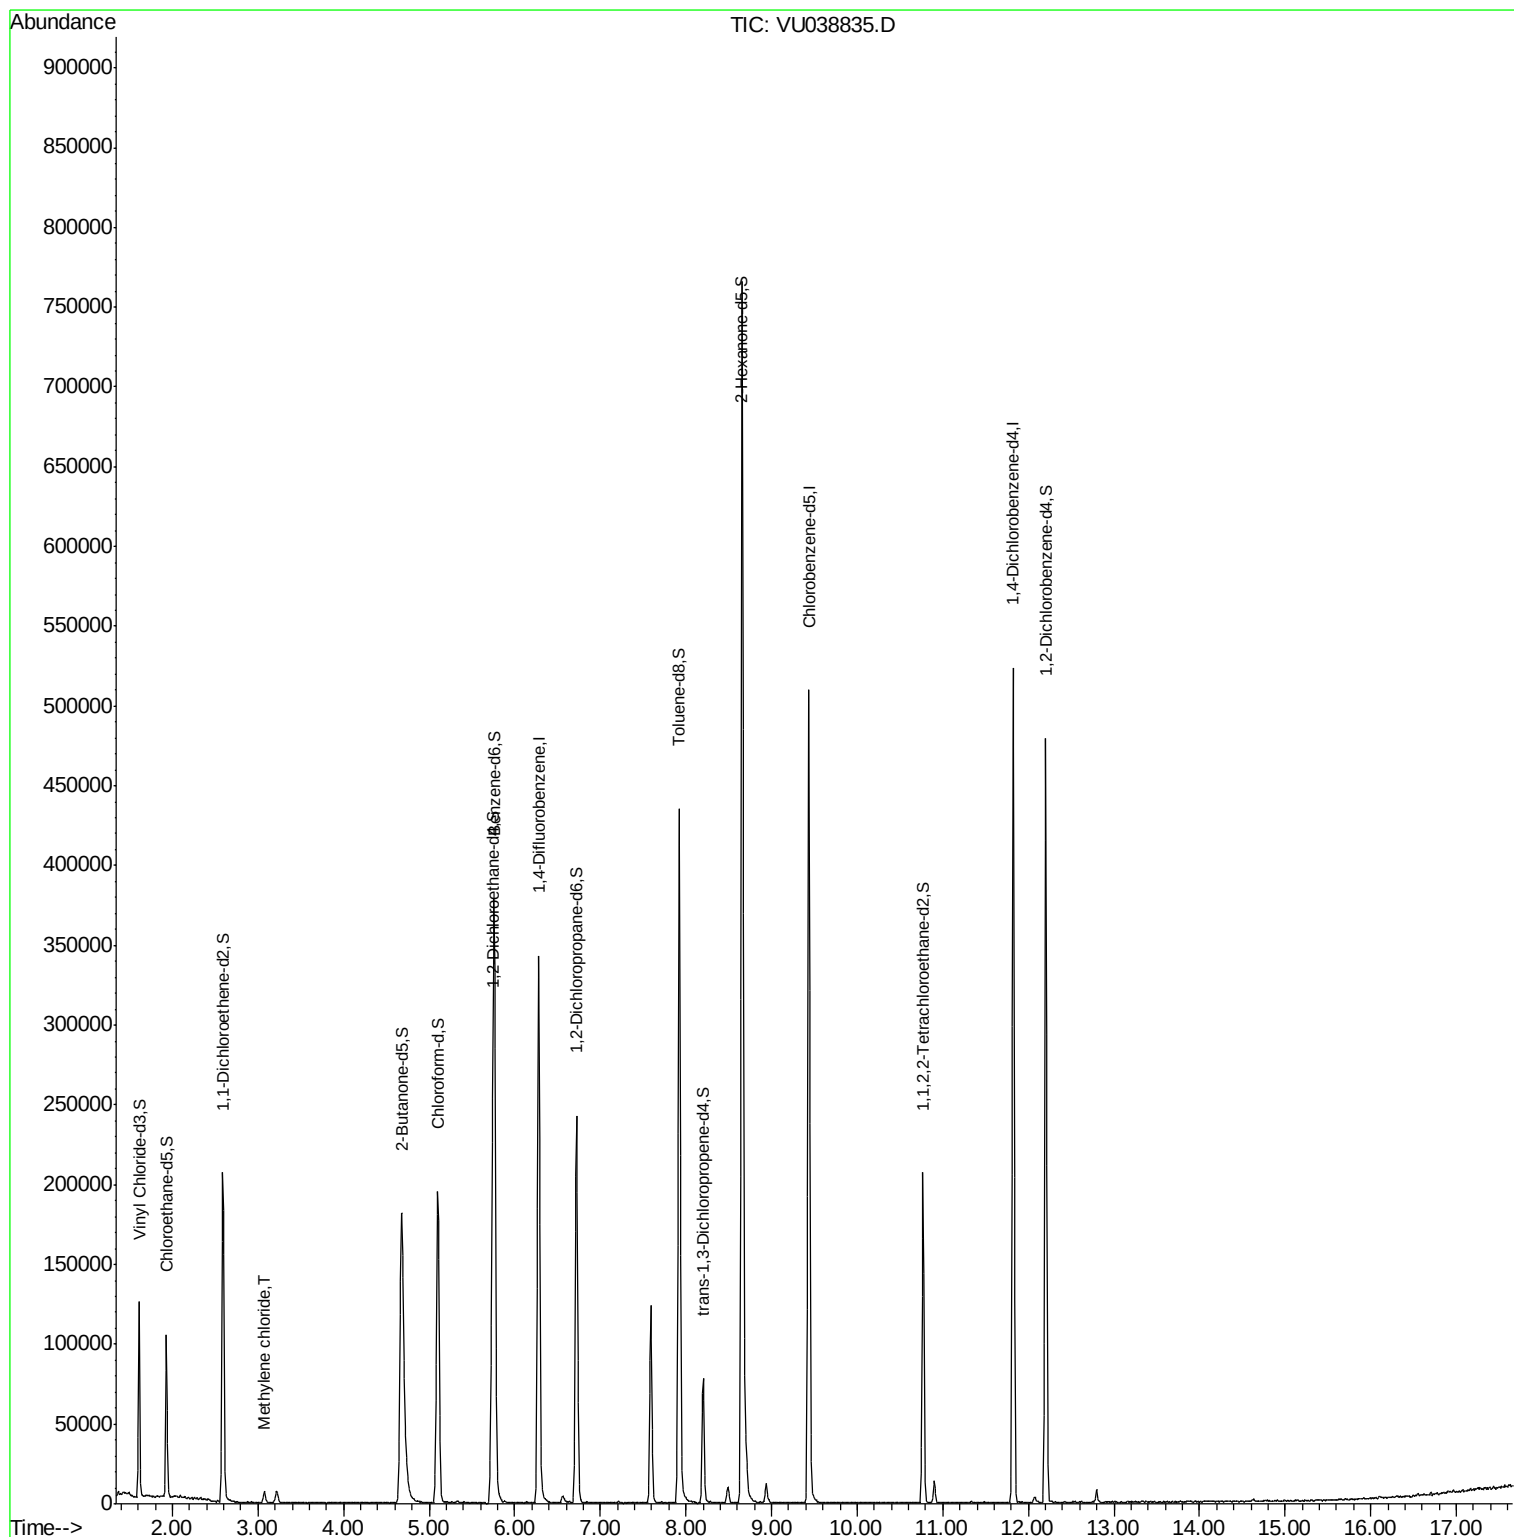

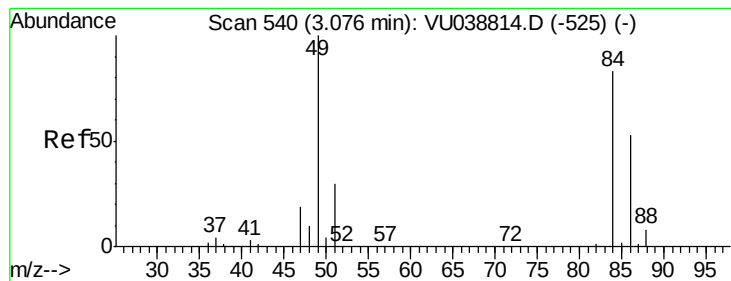

#16
Methylene chloride
Concen: 0.166 ug/L
RT: 3.07 min Scan# 539
Delta R.T. -0.00 min
Lab File: VU038835.D
Acq: 11 Jun 2020 19:15

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Tgt Ion: 84 Resp: 3314
Ion Ratio Lower Upper
84 100
86 61.9 45.0 83.6
49 115.2 85.5 158.9

