

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049082.D
 Acq On : 12 Jun 2022 11:41
 Operator : SY/MD
 Sample : N3255-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CODH8

Quant Time: Jun 13 05:02:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jun 13 05:01:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	236686	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	236634	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	100526	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	60416	41.435	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.860%
7) Chloroethane-d5	1.899	69	47860	44.704	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.400%
11) 1,1-Dichloroethene-d2	2.565	63	87727	31.885	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.760%
21) 2-Butanone-d5	4.623	46	153764	96.184	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.180%
24) Chloroform-d	5.063	84	154570	49.693	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.380%
26) 1,2-Dichloroethane-d4	5.700	65	108706	53.943	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.880%
32) Benzene-d6	5.726	84	282262	48.104	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.200%
36) 1,2-Dichloropropane-d6	6.690	67	97176	49.263	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.520%
41) Toluene-d8	7.899	98	235075	45.426	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.860%
43) trans-1,3-Dichloroprop...	8.179	79	39133	42.169	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.340%
47) 2-Hexanone-d5	8.636	63	86982	84.252	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.250%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	156537	47.513	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.020%
66) 1,2-Dichlorobenzene-d4	12.195	152	95267	54.466	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.940%
Target Compounds					Qvalue	
13) Acetone	2.629	43	70400	55.964	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049082.D
Acq On : 12 Jun 2022 11:41
Operator : SY/MD
Sample : N3255-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DH8

Quant Time: Jun 13 05:02:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jun 13 05:01:30 2022
Response via : Initial Calibration

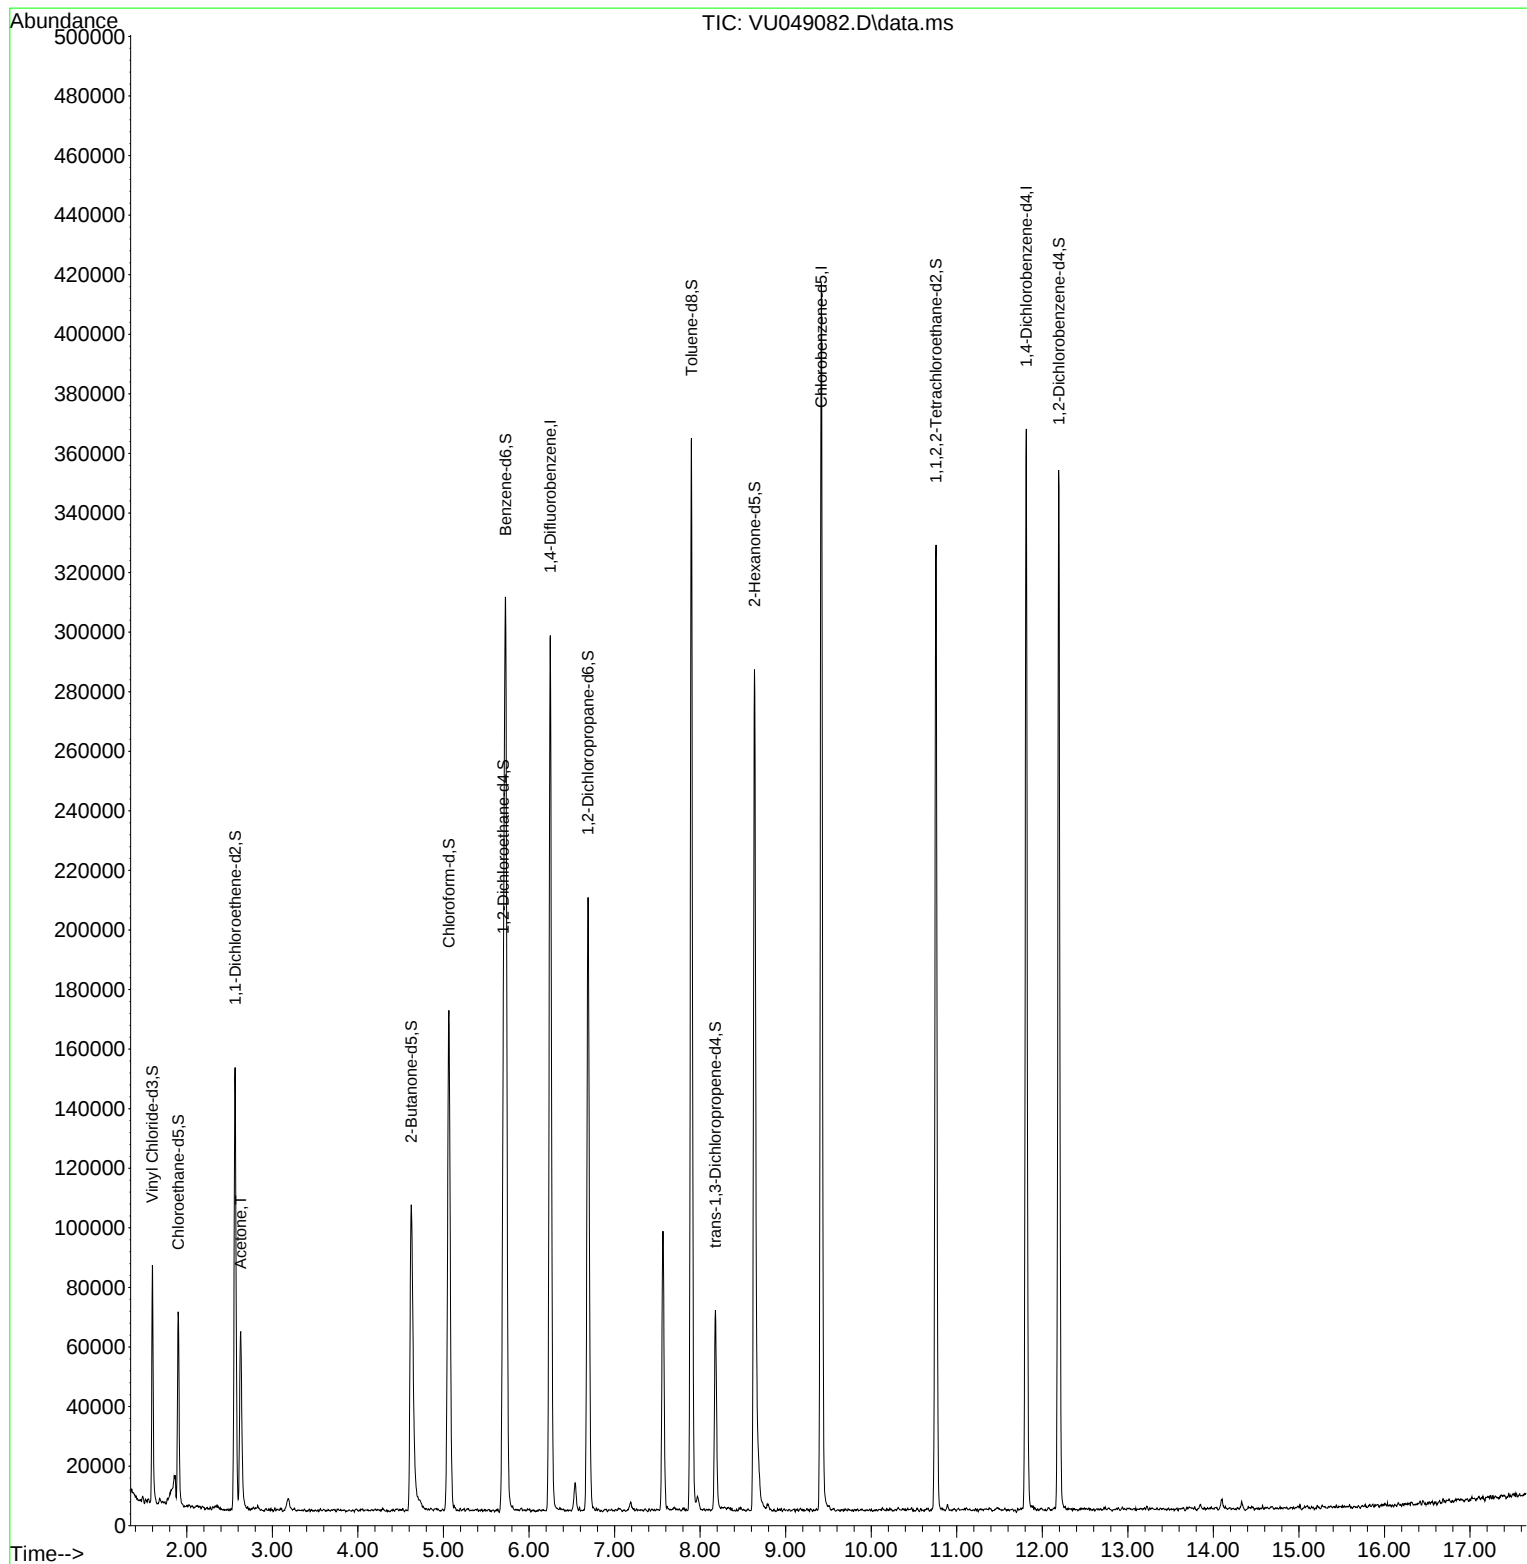

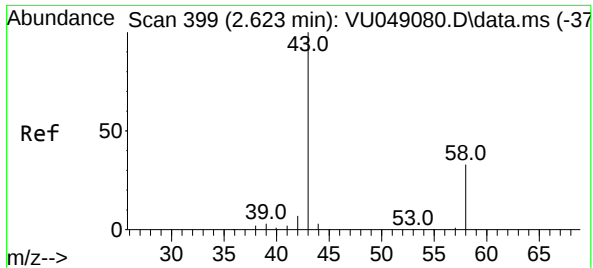

#13
 Acetone
 Concen: 55.964 ug/L
 RT: 2.629 min Scan# 401
 Delta R.T. 0.006 min
 Lab File: VU049082.D
 Acq: 12 Jun 2022 11:41

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DH8

Tgt Ion: 43 Resp: 70400
 Ion Ratio Lower Upper
 43 100
 58 33.9 0.0 66.4

