

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049083.D
 Acq On : 12 Jun 2022 12:04
 Operator : SY/MD
 Sample : N3255-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CODJ0

Quant Time: Jun 13 05:02:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jun 13 05:01:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	244942	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	241912	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	101961	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	63634	42.171	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	84.340%	
7) Chloroethane-d5	1.909	69	52783	47.641	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	95.280%	
11) 1,1-Dichloroethene-d2	2.565	63	93908	32.981	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	65.960%	
21) 2-Butanone-d5	4.626	46	162342	98.127	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	98.130%	
24) Chloroform-d	5.063	84	158519	49.245	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.480%	
26) 1,2-Dichloroethane-d4	5.703	65	109056	52.293	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	104.580%	
32) Benzene-d6	5.729	84	292052	48.686	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.380%	
36) 1,2-Dichloropropane-d6	6.690	67	98606	48.898	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	97.800%	
41) Toluene-d8	7.899	98	240693	45.497	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	91.000%	
43) trans-1,3-Dichloroprop...	8.179	79	39395	41.525	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	83.040%	
47) 2-Hexanone-d5	8.636	63	87483	82.889	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	82.890%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	154463	45.860	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	91.720%	
66) 1,2-Dichlorobenzene-d4	12.192	152	92355	52.058	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	104.120%	
Target Compounds						
13) Acetone	2.636	43	2931	2.251	ug/L	Qvalue 74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049083.D
Acq On : 12 Jun 2022 12:04
Operator : SY/MD
Sample : N3255-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ0

Quant Time: Jun 13 05:02:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jun 13 05:01:30 2022
Response via : Initial Calibration

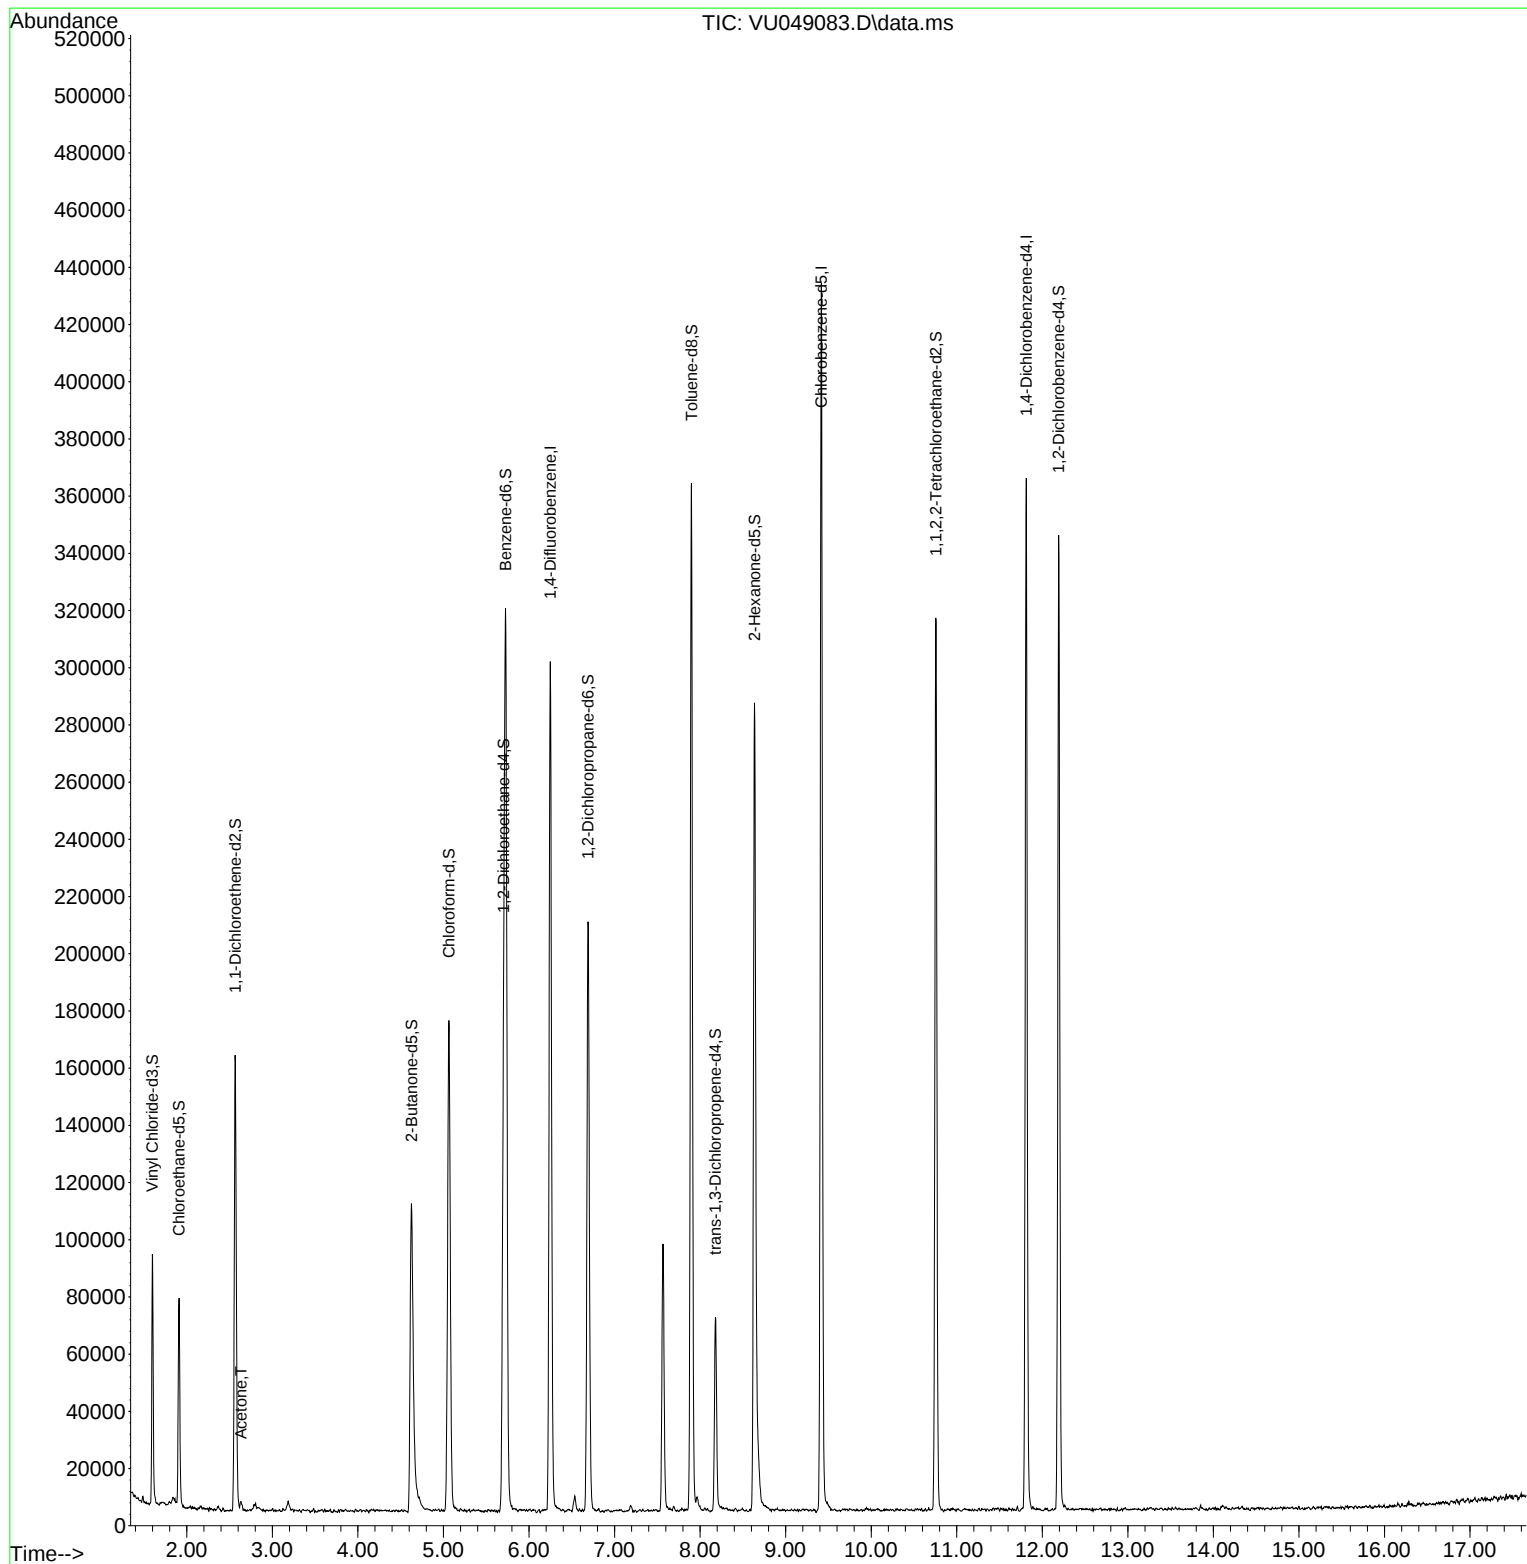

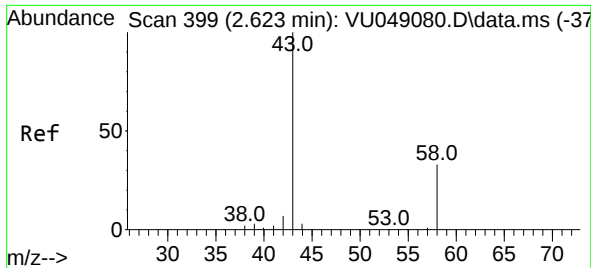

#13

Acetone

Concen: 2.251 ug/L

RT: 2.636 min Scan# 40

Delta R.T. 0.013 min

Lab File: VU049083.D


Acq: 12 Jun 2022 12:04

Instrument :

MSVOA_U

ClientSampleId :

C0DJ0

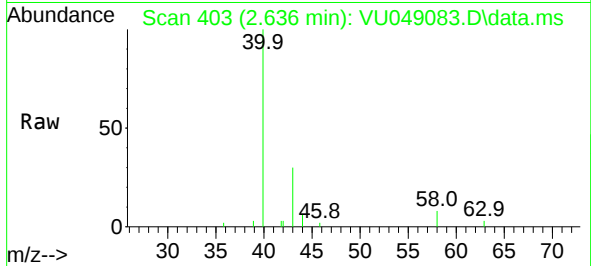

Tgt Ion: 43 Resp: 2931

Ion Ratio Lower Upper

43 100

58 18.3 0.0 66.4

