

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049092.D
 Acq On : 12 Jun 2022 15:36
 Operator : SY/MD
 Sample : N3255-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DL3

Quant Time: Jun 13 05:04:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jun 13 05:01:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	214000	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	197195	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	74684	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	57056	43.279	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.560%
7) Chloroethane-d5	1.896	69	46758	48.305	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.600%
11) 1,1-Dichloroethene-d2	2.562	63	77263	31.059	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.120%
21) 2-Butanone-d5	4.626	46	173888	120.303	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	120.300%
24) Chloroform-d	5.064	84	154002	54.759	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.520%
26) 1,2-Dichloroethane-d4	5.700	65	110930	60.883	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	121.760%
32) Benzene-d6	5.726	84	268687	54.949	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.900%
36) 1,2-Dichloropropane-d6	6.690	67	97203	59.132	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	118.260%
41) Toluene-d8	7.899	98	198132	45.945	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.880%
43) trans-1,3-Dichloroprop...	8.179	79	37418	48.385	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.760%
47) 2-Hexanone-d5	8.636	63	97914	113.810	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	113.810%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	164143	59.786	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	119.580%
66) 1,2-Dichlorobenzene-d4	12.192	152	77438	59.592	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	119.180%
Target Compounds						
13) Acetone	2.633	43	5011	4.406	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049092.D
Acq On : 12 Jun 2022 15:36
Operator : SY/MD
Sample : N3255-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DL3

Quant Time: Jun 13 05:04:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jun 13 05:01:30 2022
Response via : Initial Calibration

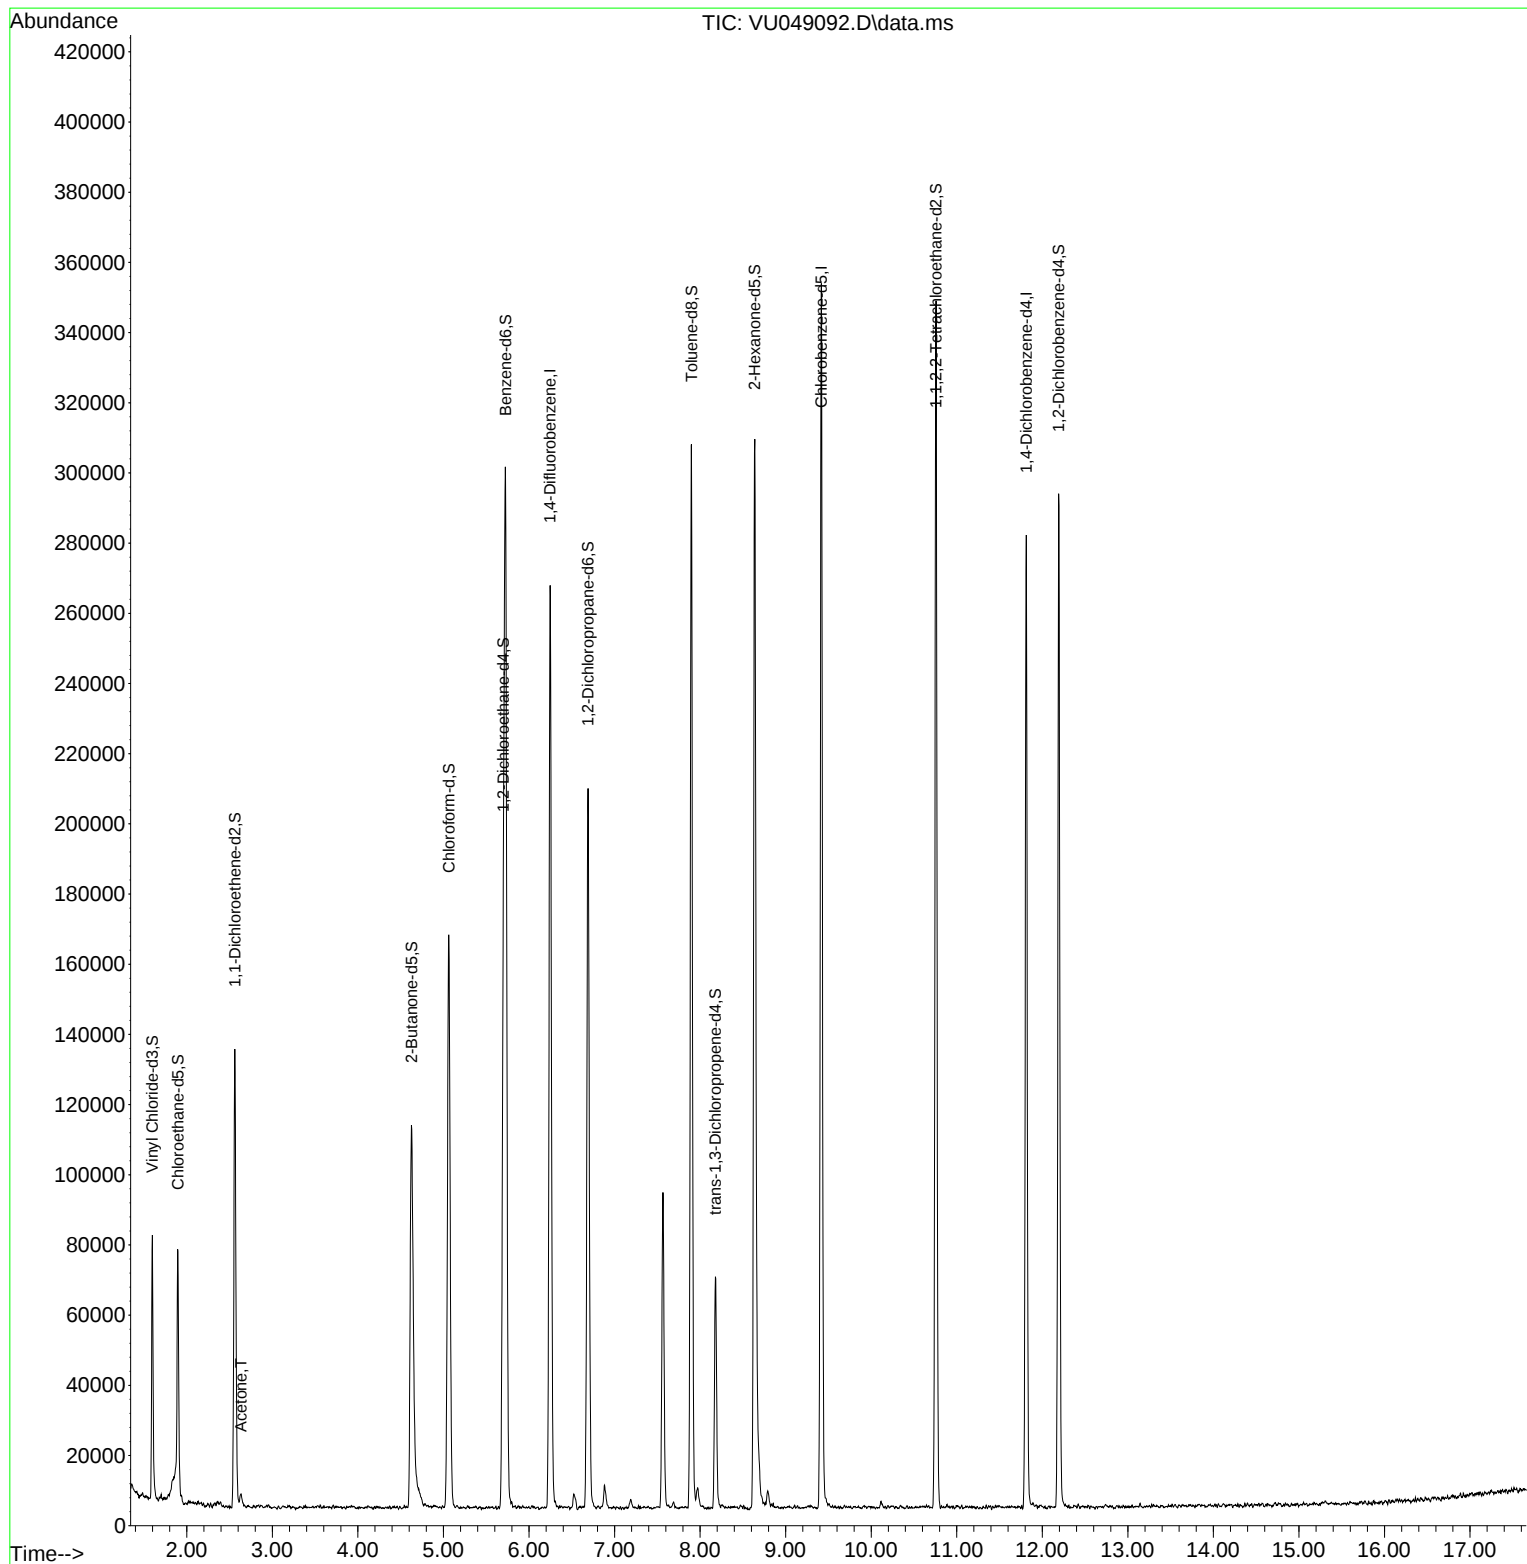

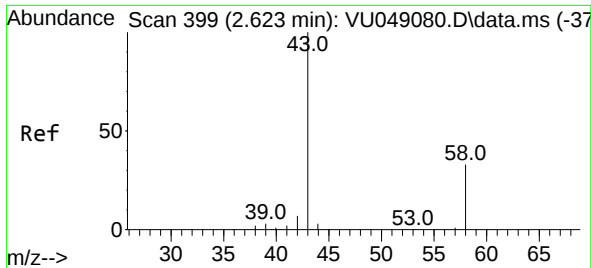

#13

Acetone

Concen: 4.406 ug/L

RT: 2.633 min Scan# 40

Delta R.T. 0.010 min

Lab File: VU049092.D


Acq: 12 Jun 2022 15:36

Instrument :

MSVOA_U

ClientSampleId :

C0DL3

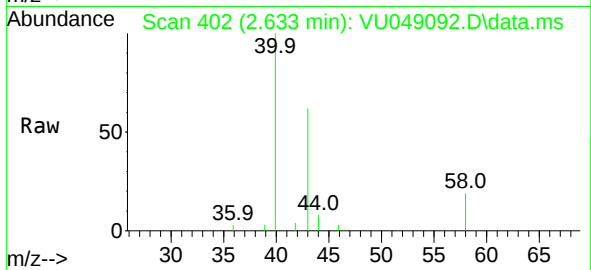

Tgt Ion: 43 Resp: 5011

Ion Ratio Lower Upper

43 100

58 35.0 0.0 66.4

