

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049097.D
 Acq On : 12 Jun 2022 17:33
 Operator : SY/MD
 Sample : N3255-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DR9

Quant Time: Jun 13 05:05:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jun 13 05:01:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	221858	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	213946	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	90492	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	58306	42.660	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	85.320%	
7) Chloroethane-d5	1.903	69	48778	48.607	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	97.220%	
11) 1,1-Dichloroethene-d2	2.565	63	88114	34.166	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	68.340%	
21) 2-Butanone-d5	4.620	46	150355	100.338	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	100.340%	
24) Chloroform-d	5.063	84	153386	52.608	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	105.220%	
26) 1,2-Dichloroethane-d4	5.700	65	106058	56.147	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	112.300%	
32) Benzene-d6	5.726	84	281280	53.020	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	106.040%	
36) 1,2-Dichloropropane-d6	6.690	67	95823	53.729	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	107.460%	
41) Toluene-d8	7.896	98	230825	49.335	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	98.680%	
43) trans-1,3-Dichloroprop...	8.179	79	35629	42.464	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	84.920%	
47) 2-Hexanone-d5	8.632	63	85644	91.754	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	91.750%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	152346	51.144	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	102.280%	
66) 1,2-Dichlorobenzene-d4	12.192	152	91605	58.180	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	116.360%	
Target Compounds						
13) Acetone	2.633	43	2600	2.205	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049097.D
Acq On : 12 Jun 2022 17:33
Operator : SY/MD
Sample : N3255-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DR9

Quant Time: Jun 13 05:05:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jun 13 05:01:30 2022
Response via : Initial Calibration

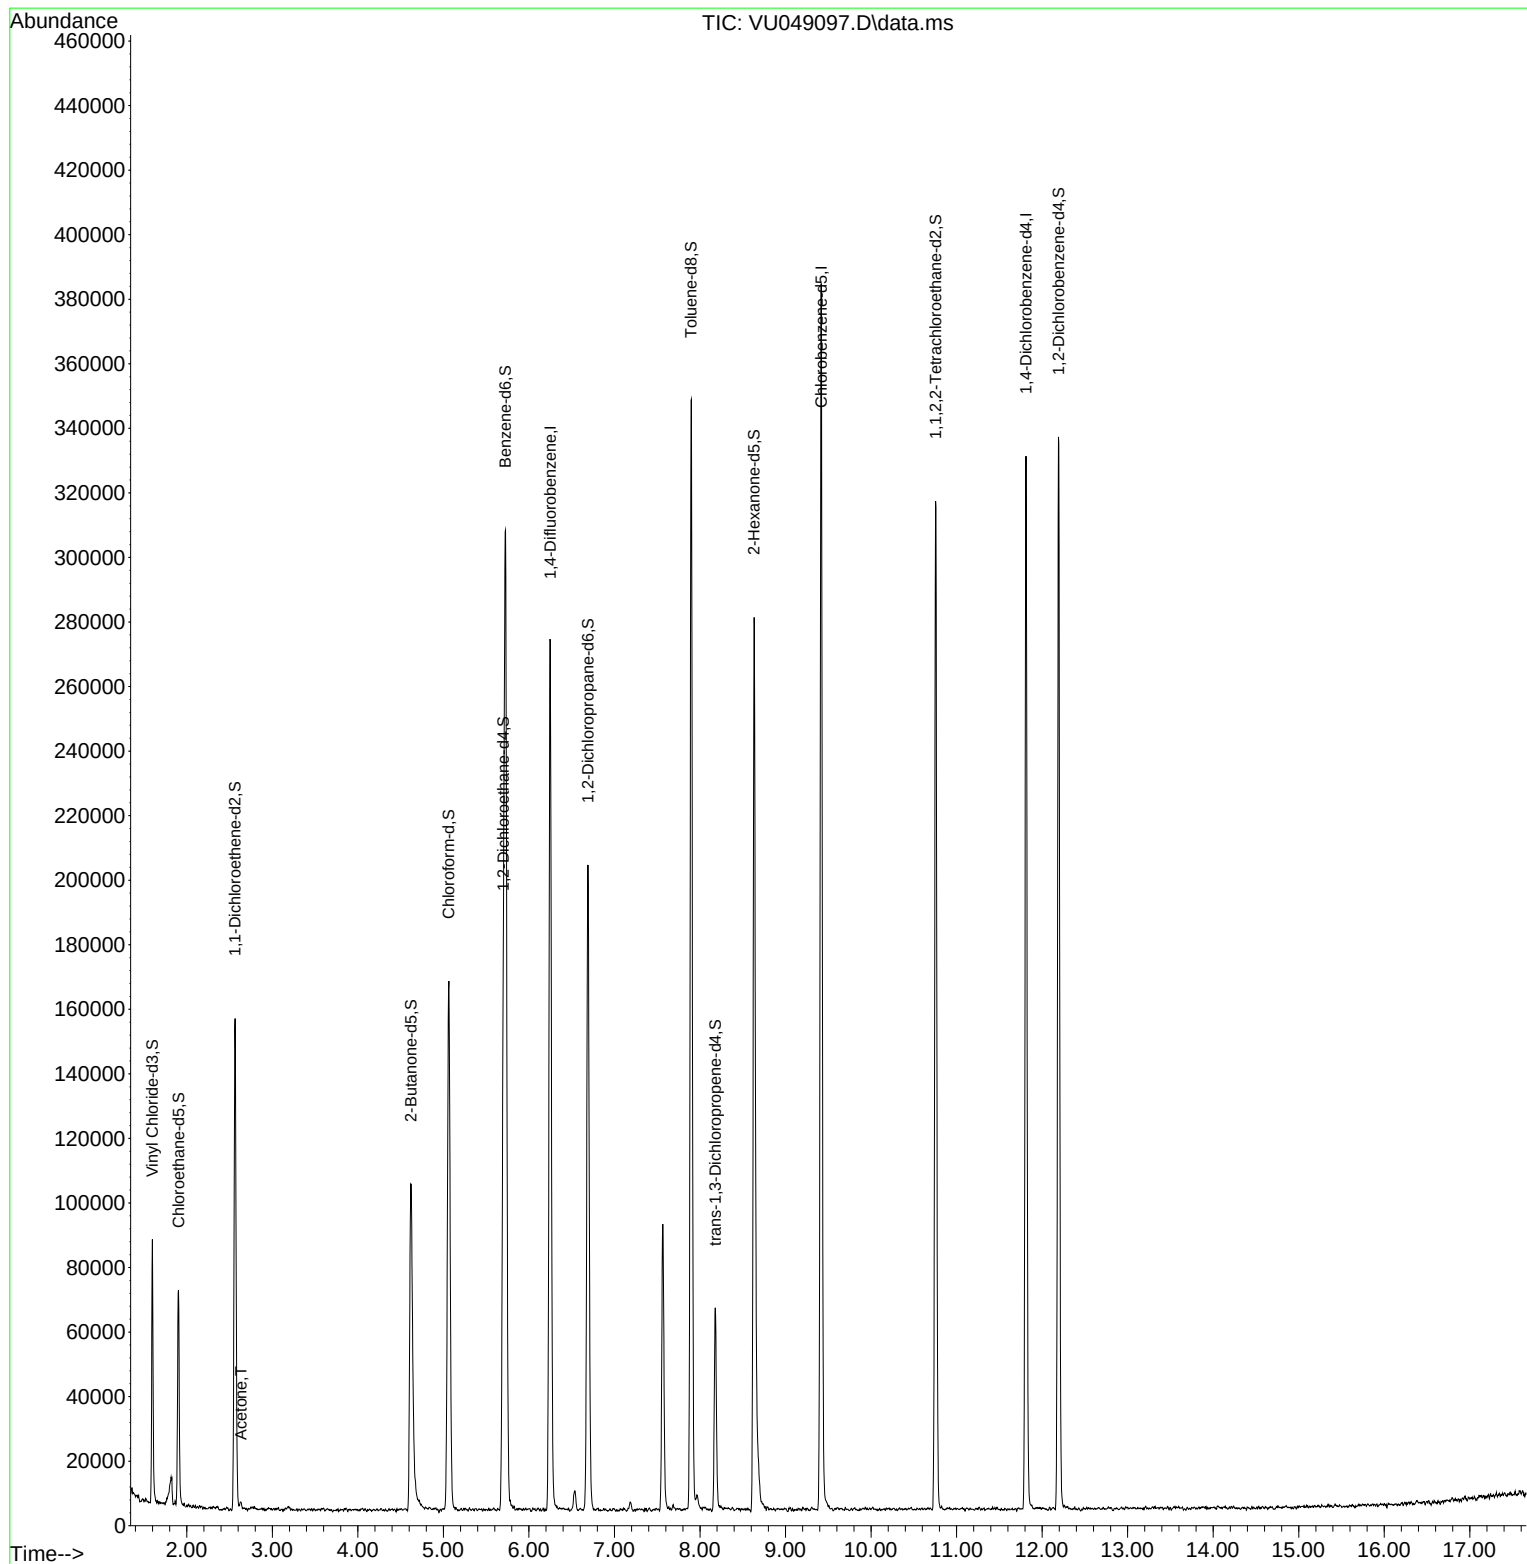

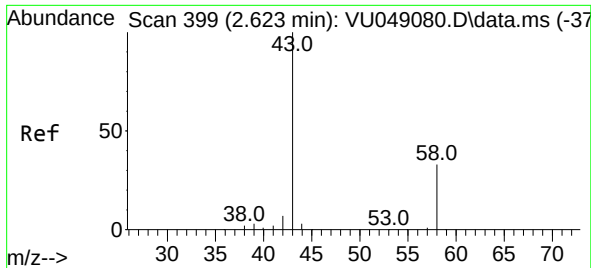

#13
 Acetone
 Concen: 2.205 ug/L
 RT: 2.633 min Scan# 40
 Delta R.T. 0.010 min
 Lab File: VU049097.D
 Acq: 12 Jun 2022 17:33

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DR9

Tgt Ion: 43 Resp: 2600
 Ion Ratio Lower Upper
 43 100
 58 28.7 0.0 66.4

