

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049082.D
 Acq On : 12 Jun 2022 11:41
 Operator : SY/MD
 Sample : N3255-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049082.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	97	rVB	80220	94679	11.10%	1.386%
2	1.899	167	174	195	rVB	65639	90203	10.57%	1.320%
3	2.565	369	381	392	rBV	148549	243283	28.52%	3.560%
4	2.629	393	401	424	rVB	59576	109418	12.83%	1.601%
5	2.928	488	494	500	rBV3	861	1265	0.15%	0.019%
6	2.983	508	511	514	rBV	864	535	0.06%	0.008%
7	3.028	519	525	528	rBV2	1292	1061	0.12%	0.016%
8	3.186	561	574	583	rBV3	4029	9520	1.12%	0.139%
9	3.407	640	643	645	rBV	322	166	0.02%	0.002%
10	3.452	654	657	659	rBV	774	524	0.06%	0.008%
11	3.562	685	691	695	rBV	1119	1248	0.15%	0.018%
12	3.629	710	712	714	rBV	406	193	0.02%	0.003%
13	3.758	748	752	754	rBV	973	721	0.08%	0.011%
14	3.867	783	786	788	rBV2	370	267	0.03%	0.004%
15	4.034	835	838	843	rBV2	661	672	0.08%	0.010%
16	4.279	911	914	916	rBV2	704	481	0.06%	0.007%
17	4.350	934	936	938	rBV2	407	193	0.02%	0.003%
18	4.391	944	949	952	rBV2	650	625	0.07%	0.009%
19	4.446	961	966	968	rBV2	742	790	0.09%	0.012%
20	4.562	997	1002	1005	rBV	730	767	0.09%	0.011%
21	4.623	1009	1021	1049	rBV	102708	268926	31.53%	3.936%
22	5.063	1142	1158	1175	rBV	167779	367198	43.05%	5.374%
23	5.195	1196	1199	1204	rBV	966	772	0.09%	0.011%
24	5.417	1266	1268	1272	rBV2	503	403	0.05%	0.006%
25	5.465	1281	1283	1285	rBV	433	243	0.03%	0.004%
26	5.571	1313	1316	1317	rBV	423	265	0.03%	0.004%
27	5.604	1324	1326	1328	rBV2	463	295	0.03%	0.004%
28	5.636	1333	1336	1341	rVB2	1176	999	0.12%	0.015%
29	5.722	1341	1363	1387	rBV2	307395	852986	100.00%	12.483%
30	6.031	1456	1459	1462	rBV2	570	459	0.05%	0.007%
31	6.047	1462	1464	1468	rVB	598	427	0.05%	0.006%
32	6.086	1473	1476	1478	rBV	383	208	0.02%	0.003%
33	6.105	1478	1482	1484	rBV2	590	407	0.05%	0.006%
34	6.250	1512	1527	1557	rBV	293882	558019	65.42%	8.167%
35	6.465	1592	1594	1597	rBV	364	260	0.03%	0.004%
36	6.539	1603	1617	1630	rBV5	9559	18687	2.19%	0.273%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049082.D
 Acq On : 12 Jun 2022 11:41
 Operator : SY/MD
 Sample : N3255-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CODH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.591	1630	1633	1637	rVB2	1304	864	0.10%	0.013%
38	6.690	1650	1664	1681	rBV	205688	396232	46.45%	5.799%
39	6.841	1709	1711	1717	rVB2	518	375	0.04%	0.005%
40	6.870	1717	1720	1721	rBV	405	243	0.03%	0.004%
41	6.931	1735	1739	1745	rBV	695	1028	0.12%	0.015%
42	7.012	1761	1764	1765	rBV	548	334	0.04%	0.005%
43	7.102	1789	1792	1794	rBV	467	334	0.04%	0.005%
44	7.404	1881	1886	1890	rBV	1053	1155	0.14%	0.017%
45	7.565	1925	1936	1949	rBV	93550	163488	19.17%	2.393%
46	7.899	2027	2040	2055	rBV	359965	613625	71.94%	8.980%
47	8.179	2117	2127	2147	rVB	66657	110954	13.01%	1.624%
48	8.427	2201	2204	2206	rBV2	739	432	0.05%	0.006%
49	8.546	2239	2241	2243	rBV	460	297	0.03%	0.004%
50	8.636	2257	2269	2297	rBV3	282365	549334	64.40%	8.039%
51	8.864	2337	2340	2343	rBV2	655	304	0.04%	0.004%
52	8.893	2347	2349	2350	rBV	214	116	0.01%	0.002%
53	8.906	2350	2353	2355	rBV	839	457	0.05%	0.007%
54	8.947	2363	2366	2370	rVB	1041	758	0.09%	0.011%
55	8.983	2370	2377	2381	rBV	958	1200	0.14%	0.018%
56	9.121	2417	2420	2423	rBV	877	725	0.08%	0.011%
57	9.214	2446	2449	2451	rBV	644	370	0.04%	0.005%
58	9.291	2469	2473	2480	rVB	997	1121	0.13%	0.016%
59	9.417	2500	2512	2534	rBV	411662	685264	80.34%	10.029%
60	9.642	2580	2582	2584	rBV	479	253	0.03%	0.004%
61	9.684	2592	2595	2597	rBV2	773	479	0.06%	0.007%
62	9.729	2607	2609	2613	rBV2	670	489	0.06%	0.007%
63	9.783	2622	2626	2629	rVB	564	401	0.05%	0.006%
64	9.803	2629	2632	2637	rBV2	680	698	0.08%	0.010%
65	10.002	2691	2694	2698	rVB	867	534	0.06%	0.008%
66	10.182	2747	2750	2752	rBV	775	455	0.05%	0.007%
67	10.217	2758	2761	2765	rBV	905	690	0.08%	0.010%
68	10.504	2848	2850	2854	rBV2	275	177	0.02%	0.003%
69	10.581	2869	2874	2877	rBV	1086	1052	0.12%	0.015%
70	10.629	2886	2889	2891	rBV	657	511	0.06%	0.007%
71	10.713	2912	2915	2916	rBV2	729	450	0.05%	0.007%
72	10.758	2917	2929	2947	rVB	324002	518120	60.74%	7.583%
73	11.240	3075	3079	3082	rVB	906	740	0.09%	0.011%
74	11.259	3082	3085	3086	rBV	625	372	0.04%	0.005%
75	11.590	3185	3188	3190	rBV	521	326	0.04%	0.005%
76	11.713	3221	3226	3230	rBV	1409	1485	0.17%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049082.D
 Acq On : 12 Jun 2022 11:41
 Operator : SY/MD
 Sample : N3255-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

77	11.812	3245	3257	3274	rBV	362396	579982	67.99%	8.488%
78	12.037	3325	3327	3330	rVB2	514	199	0.02%	0.003%
79	12.192	3363	3375	3394	rBV	348682	567250	66.50%	8.302%
80	12.359	3425	3427	3430	rBV2	858	536	0.06%	0.008%
81	12.828	3570	3573	3576	rBV2	546	528	0.06%	0.008%
82	13.092	3653	3655	3657	rVB	719	220	0.03%	0.003%
83	13.597	3809	3812	3816	rBV2	813	873	0.10%	0.013%




Sum of corrected areas: 6832995

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049082.D
Acq On : 12 Jun 2022 11:41
Operator : SY/MD
Sample : N3255-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

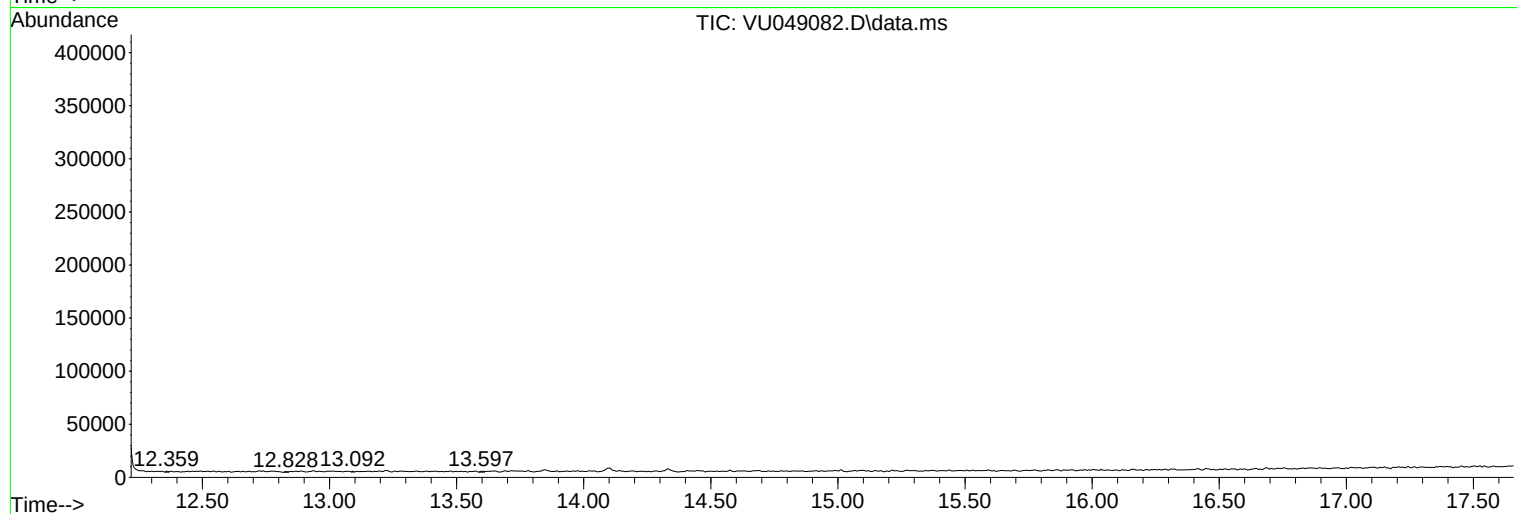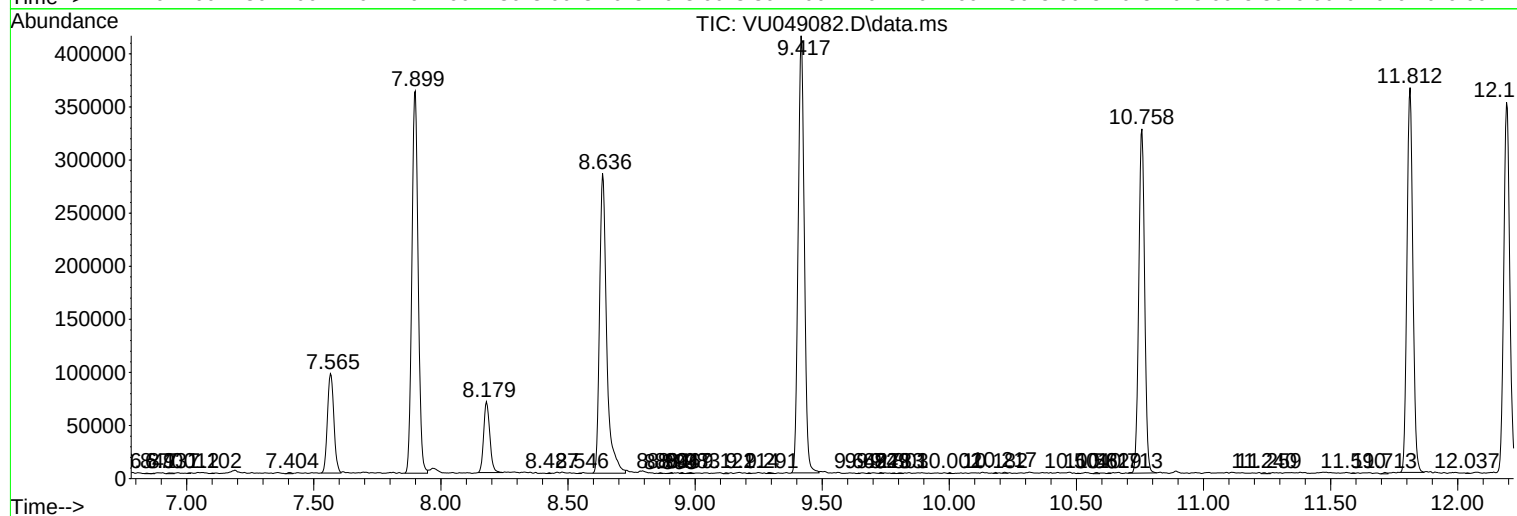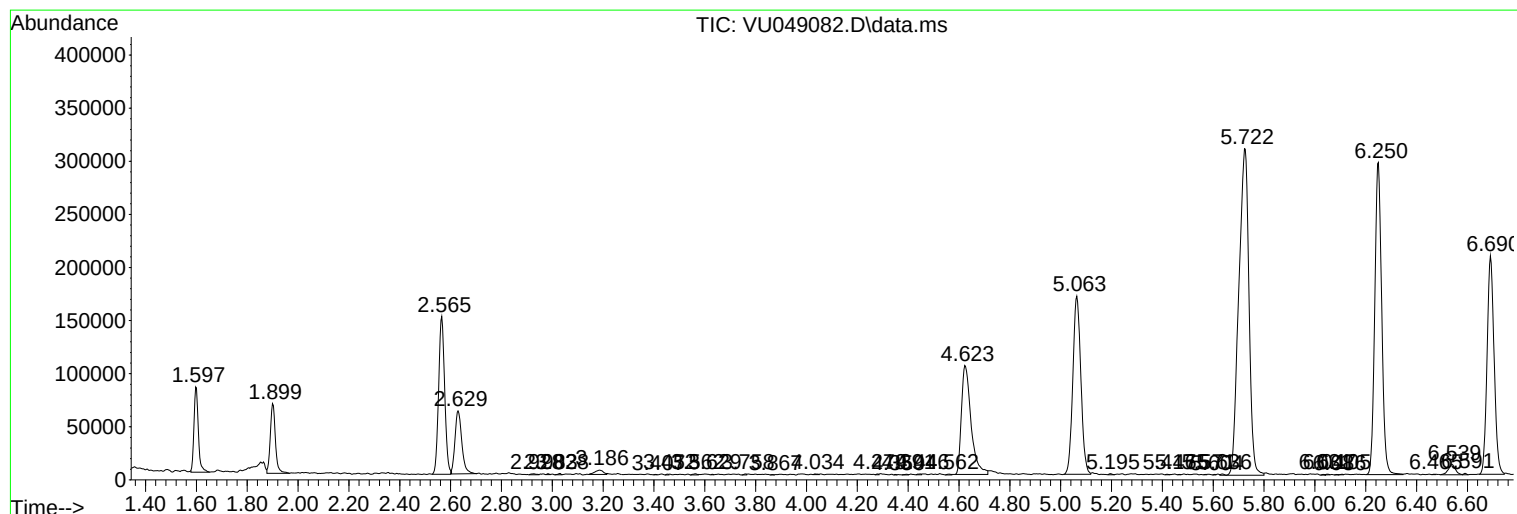

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049082.D
Acq On : 12 Jun 2022 11:41
Operator : SY/MD
Sample : N3255-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049082.D
Acq On : 12 Jun 2022 11:41
Operator : SY/MD
Sample : N3255-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------