

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049083.D
 Acq On : 12 Jun 2022 12:04
 Operator : SY/MD
 Sample : N3255-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049083.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	95	rVB	87092	99389	11.44%	1.455%
2	1.909	170	177	191	rVB	73020	95395	10.98%	1.396%
3	2.266	285	288	292	rBV4	1360	1128	0.13%	0.017%
4	2.324	303	306	307	rBV	748	429	0.05%	0.006%
5	2.424	330	337	343	rBV4	1298	1457	0.17%	0.021%
6	2.565	370	381	397	rBV	159395	263636	30.35%	3.859%
7	2.928	491	494	496	rBV2	659	448	0.05%	0.007%
8	3.051	529	532	536	rBV2	504	409	0.05%	0.006%
9	3.125	551	555	558	rBV	1047	851	0.10%	0.012%
10	3.260	594	597	599	rBV	732	511	0.06%	0.007%
11	3.359	621	628	631	rBV2	1060	1518	0.17%	0.022%
12	3.453	654	657	659	rBV	553	427	0.05%	0.006%
13	3.501	670	672	676	rBV	524	356	0.04%	0.005%
14	3.539	679	684	686	rBV	679	568	0.07%	0.008%
15	3.613	702	707	710	rBV	1062	893	0.10%	0.013%
16	3.633	710	713	715	rBV2	398	226	0.03%	0.003%
17	3.694	730	732	734	rVB	281	114	0.01%	0.002%
18	3.707	734	736	737	rBV	131	52	0.01%	0.001%
19	3.719	737	740	745	rBV2	896	729	0.08%	0.011%
20	3.774	752	757	760	rBV	986	684	0.08%	0.010%
21	3.800	760	765	769	rBV	975	1226	0.14%	0.018%
22	3.970	815	818	824	rBV2	1035	1132	0.13%	0.017%
23	4.063	841	847	855	rBV	568	947	0.11%	0.014%
24	4.099	855	858	863	rBV2	763	716	0.08%	0.010%
25	4.137	867	870	872	rBV	865	615	0.07%	0.009%
26	4.411	952	955	956	rBV	364	202	0.02%	0.003%
27	4.478	974	976	980	rVB	352	180	0.02%	0.003%
28	4.626	1009	1022	1049	rBV	107970	287968	33.15%	4.215%
29	5.063	1143	1158	1175	rBV	171311	374884	43.15%	5.487%
30	5.198	1196	1200	1202	rBV3	914	765	0.09%	0.011%
31	5.247	1213	1215	1218	rBV2	637	317	0.04%	0.005%
32	5.288	1223	1228	1230	rBV3	679	696	0.08%	0.010%
33	5.330	1236	1241	1244	rBV2	715	707	0.08%	0.010%
34	5.456	1278	1280	1284	rVB2	356	209	0.02%	0.003%
35	5.475	1284	1286	1288	rBV	400	171	0.02%	0.003%
36	5.491	1288	1291	1297	rBV	547	557	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049083.D
 Acq On : 12 Jun 2022 12:04
 Operator : SY/MD
 Sample : N3255-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.520	1297	1300	1301	rBV	709	476	0.05%	0.007%
38	5.623	1329	1332	1335	rVB	781	478	0.06%	0.007%
39	5.645	1335	1339	1342	rBV	896	840	0.10%	0.012%
40	5.726	1342	1364	1385	rBV2	315966	868766	100.00%	12.717%
41	5.970	1437	1440	1445	rVB	703	486	0.06%	0.007%
42	6.118	1476	1486	1490	rBV	1103	1504	0.17%	0.022%
43	6.157	1490	1498	1500	rBV	1042	1284	0.15%	0.019%
44	6.250	1514	1527	1546	rBV2	296485	570503	65.67%	8.351%
45	6.536	1605	1616	1624	rBV8	5555	10232	1.18%	0.150%
46	6.591	1630	1633	1636	rVB	811	505	0.06%	0.007%
47	6.690	1651	1664	1682	rBV2	205745	402848	46.37%	5.897%
48	6.854	1712	1715	1717	rBV	384	230	0.03%	0.003%
49	6.886	1722	1725	1727	rBV	618	472	0.05%	0.007%
50	6.960	1745	1748	1752	rVB2	379	240	0.03%	0.004%
51	7.121	1795	1798	1801	rBV2	369	297	0.03%	0.004%
52	7.221	1827	1829	1831	rBV	475	184	0.02%	0.003%
53	7.243	1831	1836	1841	rVB2	754	763	0.09%	0.011%
54	7.272	1841	1845	1846	rBV	416	289	0.03%	0.004%
55	7.507	1916	1918	1921	rBV	331	179	0.02%	0.003%
56	7.565	1925	1936	1951	rBV	93325	165996	19.11%	2.430%
57	7.899	2027	2040	2055	rBV	358771	623731	71.80%	9.130%
58	8.128	2108	2111	2113	rBV	505	309	0.04%	0.005%
59	8.179	2116	2127	2145	rVV	67637	117489	13.52%	1.720%
60	8.636	2256	2269	2297	rBV2	282509	561371	64.62%	8.217%
61	8.841	2330	2333	2337	rBV	798	768	0.09%	0.011%
62	9.160	2429	2432	2438	rBV	727	732	0.08%	0.011%
63	9.417	2493	2512	2532	rBV	429771	713306	82.11%	10.441%
64	10.517	2851	2854	2858	rBV2	745	728	0.08%	0.011%
65	10.754	2917	2928	2948	rVB	311915	508521	58.53%	7.444%
66	10.861	2957	2961	2964	rBV2	788	686	0.08%	0.010%
67	11.002	3002	3005	3007	rBV	852	663	0.08%	0.010%
68	11.513	3161	3164	3166	rBV2	1011	725	0.08%	0.011%
69	11.652	3204	3207	3211	rBV	842	651	0.07%	0.010%
70	11.812	3245	3257	3277	rVB	360378	580072	66.77%	8.491%
71	12.192	3363	3375	3394	rBV	340520	553283	63.69%	8.099%
72	12.603	3500	3503	3508	rBV	828	885	0.10%	0.013%
73	12.877	3585	3588	3594	rBV	1132	734	0.08%	0.011%




Sum of corrected areas: 6831738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049083.D
Acq On : 12 Jun 2022 12:04
Operator : SY/MD
Sample : N3255-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

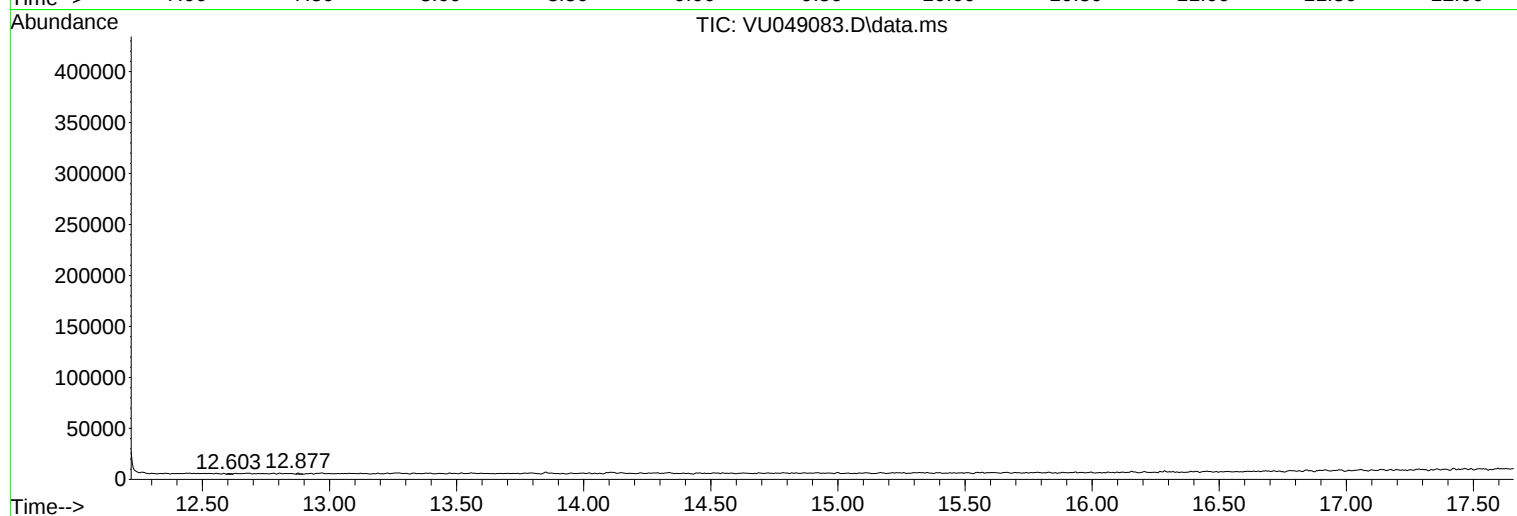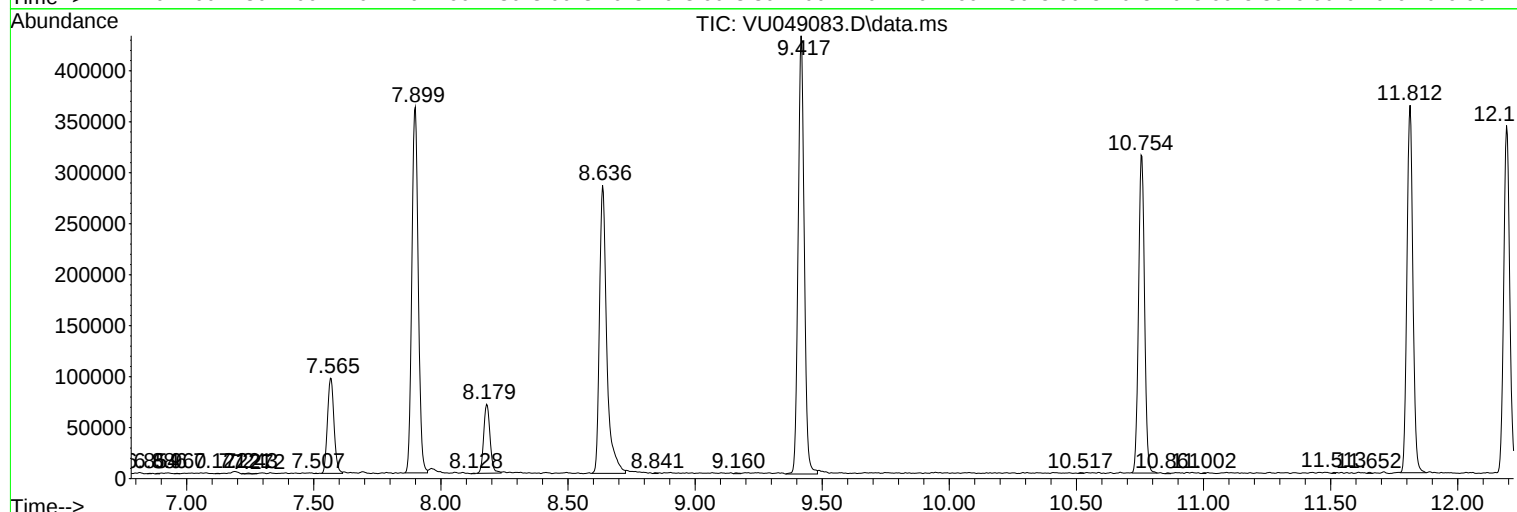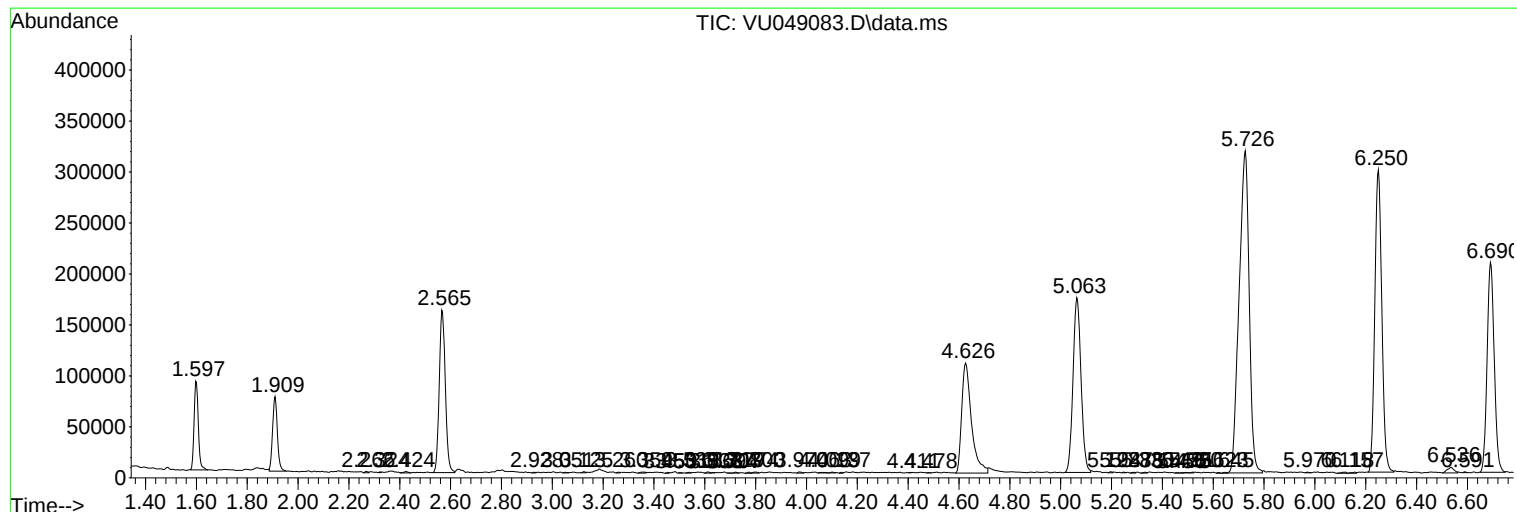

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049083.D
Acq On : 12 Jun 2022 12:04
Operator : SY/MD
Sample : N3255-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049083.D
Acq On : 12 Jun 2022 12:04
Operator : SY/MD
Sample : N3255-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc