

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049084.D
 Acq On : 12 Jun 2022 12:28
 Operator : SY/MD
 Sample : N3255-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	95	rVB	82149	91978	11.25%	1.413%
2	1.899	167	174	185	rVB	64643	85977	10.52%	1.321%
3	2.565	369	381	394	rBV	149450	245435	30.02%	3.771%
4	2.764	434	443	446	rBV2	2887	3831	0.47%	0.059%
5	3.009	516	519	522	rBV	669	402	0.05%	0.006%
6	3.102	545	548	554	rBV	781	691	0.08%	0.011%
7	3.395	636	639	641	rBV2	580	412	0.05%	0.006%
8	3.520	675	678	680	rBV	504	404	0.05%	0.006%
9	3.565	689	692	695	rBV	623	475	0.06%	0.007%
10	3.690	728	731	732	rBV	403	213	0.03%	0.003%
11	3.742	743	747	749	rBV	866	617	0.08%	0.009%
12	3.816	766	770	775	rBV	869	708	0.09%	0.011%
13	3.932	803	806	807	rBV	438	266	0.03%	0.004%
14	4.031	834	837	840	rBV	480	416	0.05%	0.006%
15	4.144	870	872	875	rVB	695	337	0.04%	0.005%
16	4.192	884	887	890	rVB	701	456	0.06%	0.007%
17	4.214	890	894	897	rBV2	640	637	0.08%	0.010%
18	4.369	940	942	944	rBV	486	314	0.04%	0.005%
19	4.427	957	960	962	rBV	723	533	0.07%	0.008%
20	4.510	983	986	988	rBV	871	555	0.07%	0.009%
21	4.620	1007	1020	1039	rBV	107429	263269	32.20%	4.045%
22	4.877	1097	1100	1102	rBV	887	636	0.08%	0.010%
23	5.063	1143	1158	1177	rVB	169859	377886	46.22%	5.806%
24	5.182	1192	1195	1200	rBV	910	754	0.09%	0.012%
25	5.349	1242	1247	1253	rVB2	983	1139	0.14%	0.017%
26	5.375	1253	1255	1258	rBV	681	436	0.05%	0.007%
27	5.407	1262	1265	1268	rVB	538	333	0.04%	0.005%
28	5.427	1268	1271	1273	rBV	609	412	0.05%	0.006%
29	5.501	1288	1294	1296	rBV	1004	837	0.10%	0.013%
30	5.562	1310	1313	1316	rBV	381	262	0.03%	0.004%
31	5.603	1323	1326	1330	rBV2	429	286	0.03%	0.004%
32	5.722	1343	1363	1382	rBV2	297598	817574	100.00%	12.561%
33	5.938	1426	1430	1434	rBV3	789	929	0.11%	0.014%
34	6.012	1449	1453	1456	rBV2	1068	835	0.10%	0.013%
35	6.028	1456	1458	1460	rBV2	405	255	0.03%	0.004%
36	6.076	1469	1473	1475	rBV2	909	715	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049084.D
 Acq On : 12 Jun 2022 12:28
 Operator : SY/MD
 Sample : N3255-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CODJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.250	1509	1527	1545	rBV	289829	556725	68.09%	8.553%
38	6.578	1626	1629	1631	rBV	636	443	0.05%	0.007%
39	6.690	1651	1664	1682	rBV	196659	380980	46.60%	5.853%
40	6.787	1691	1694	1695	rBV	516	277	0.03%	0.004%
41	6.803	1696	1699	1703	rVV4	1299	988	0.12%	0.015%
42	6.857	1713	1716	1720	rBV	756	559	0.07%	0.009%
43	6.877	1720	1722	1725	rVB	359	175	0.02%	0.003%
44	6.896	1725	1728	1729	rBV	511	301	0.04%	0.005%
45	7.005	1758	1762	1764	rBV	934	651	0.08%	0.010%
46	7.131	1795	1801	1803	rBV	515	617	0.08%	0.009%
47	7.179	1810	1816	1825	rBV7	2019	3731	0.46%	0.057%
48	7.234	1828	1833	1837	rBV	692	698	0.09%	0.011%
49	7.288	1847	1850	1852	rBV	464	228	0.03%	0.004%
50	7.372	1871	1876	1879	rBV	837	818	0.10%	0.013%
51	7.565	1924	1936	1949	rBV2	90928	160119	19.58%	2.460%
52	7.735	1985	1989	1992	rBV	597	607	0.07%	0.009%
53	7.896	2025	2039	2055	rBV	335689	581986	71.18%	8.941%
54	8.179	2116	2127	2143	rBV	65126	107193	13.11%	1.647%
55	8.574	2247	2250	2252	rBV	550	327	0.04%	0.005%
56	8.587	2252	2254	2256	rBV	317	157	0.02%	0.002%
57	8.636	2256	2269	2295	rBV3	266629	526923	64.45%	8.095%
58	9.012	2383	2386	2387	rBV	688	409	0.05%	0.006%
59	9.301	2473	2476	2477	rBV	591	378	0.05%	0.006%
60	9.333	2483	2486	2489	rBV	1204	846	0.10%	0.013%
61	9.417	2500	2512	2528	rBV	405760	670696	82.03%	10.304%
62	9.562	2553	2557	2560	rBV2	1338	1109	0.14%	0.017%
63	9.844	2642	2645	2647	rBV	700	459	0.06%	0.007%
64	10.005	2693	2695	2697	rBV	371	229	0.03%	0.004%
65	10.259	2771	2774	2777	rBV	683	545	0.07%	0.008%
66	10.754	2917	2928	2951	rVB	301848	501351	61.32%	7.702%
67	11.047	3016	3019	3021	rBV	552	396	0.05%	0.006%
68	11.160	3052	3054	3056	rBV	643	348	0.04%	0.005%
69	11.211	3067	3070	3072	rBV	695	496	0.06%	0.008%
70	11.253	3078	3083	3086	rBV	1036	979	0.12%	0.015%
71	11.507	3156	3162	3164	rBV	1063	1016	0.12%	0.016%
72	11.812	3244	3257	3276	rBV	351624	565624	69.18%	8.690%
73	11.944	3296	3298	3300	rBV2	719	436	0.05%	0.007%
74	12.192	3363	3375	3394	rBV	329908	537394	65.73%	8.256%
75	13.204	3688	3690	3694	rBV	880	515	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049084.D
Acq On : 12 Jun 2022 12:28
Operator : SY/MD
Sample : N3255-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Title : VOC Analysis




Sum of corrected areas: 6508944

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049084.D
Acq On : 12 Jun 2022 12:28
Operator : SY/MD
Sample : N3255-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

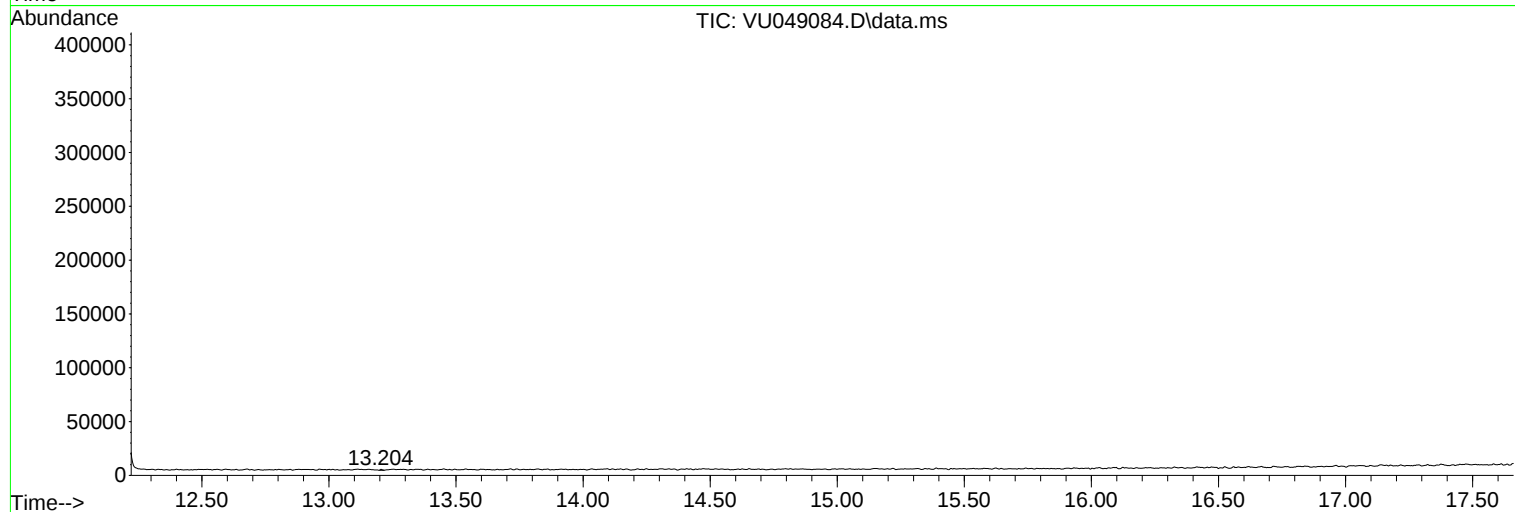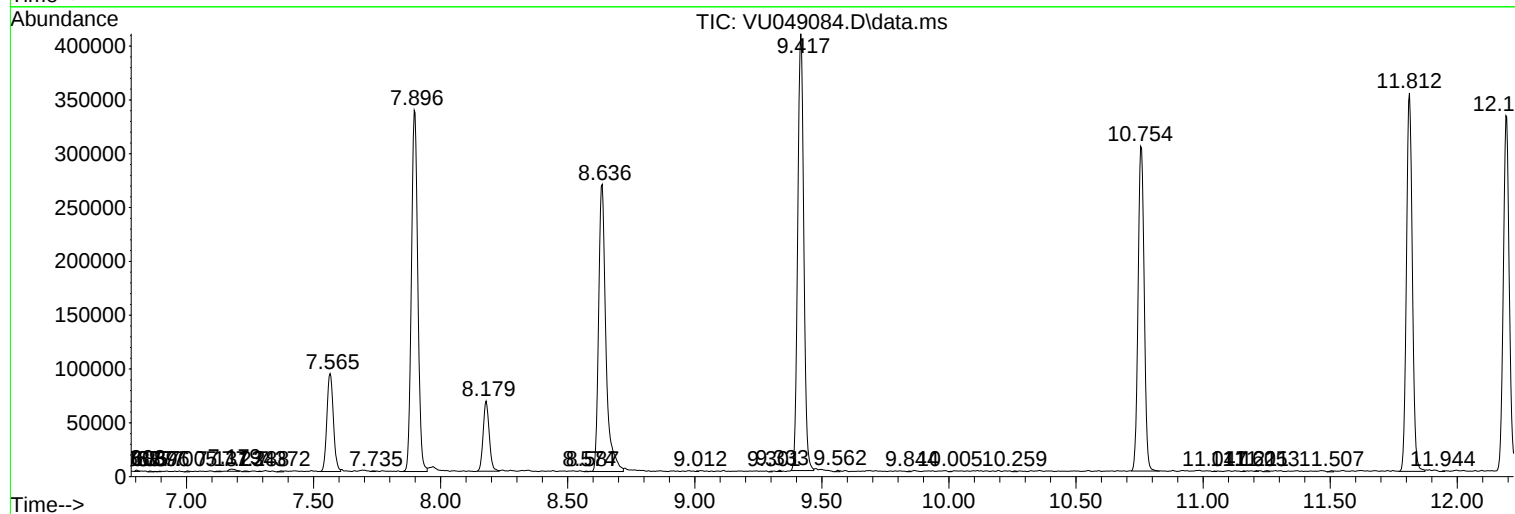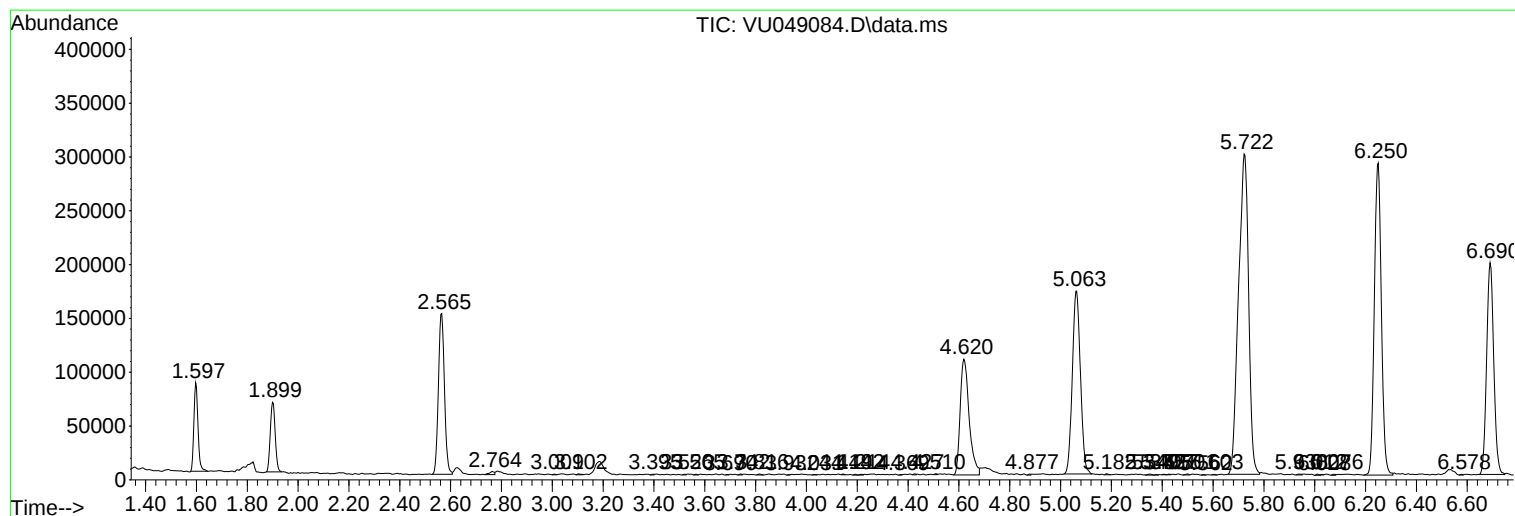

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049084.D
Acq On : 12 Jun 2022 12:28
Operator : SY/MD
Sample : N3255-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049084.D
Acq On : 12 Jun 2022 12:28
Operator : SY/MD
Sample : N3255-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------