

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049085.D
 Acq On : 12 Jun 2022 12:51
 Operator : SY/MD
 Sample : N3255-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	96	rVB	82265	95056	11.69%	1.499%
2	1.912	171	178	188	rVB	66252	81932	10.07%	1.292%
3	2.391	324	327	329	rBV	1095	700	0.09%	0.011%
4	2.507	360	363	365	rBV	705	452	0.06%	0.007%
5	2.565	370	381	397	rBV	140925	233318	28.69%	3.680%
6	2.784	446	449	451	rBV2	605	438	0.05%	0.007%
7	2.954	500	502	504	rBV2	669	312	0.04%	0.005%
8	3.031	523	526	527	rBV	528	276	0.03%	0.004%
9	3.112	549	551	554	rBV	937	524	0.06%	0.008%
10	3.131	554	557	559	rBV	654	493	0.06%	0.008%
11	3.301	607	610	612	rBV	373	238	0.03%	0.004%
12	3.327	612	618	621	rVV	645	875	0.11%	0.014%
13	3.382	630	635	639	rBV2	990	1029	0.13%	0.016%
14	3.430	647	650	651	rBV2	393	207	0.03%	0.003%
15	3.523	673	679	683	rBV2	757	782	0.10%	0.012%
16	3.546	683	686	687	rBV	420	252	0.03%	0.004%
17	3.604	701	704	710	rVB	411	307	0.04%	0.005%
18	3.716	735	739	741	rBV	609	442	0.05%	0.007%
19	3.771	752	756	761	rVB2	580	620	0.08%	0.010%
20	3.829	771	774	780	rBV2	453	438	0.05%	0.007%
21	3.906	793	798	804	rVB	733	948	0.12%	0.015%
22	4.121	860	865	869	rBV2	691	769	0.09%	0.012%
23	4.324	925	928	932	rBV2	980	878	0.11%	0.014%
24	4.449	964	967	970	rVB	721	428	0.05%	0.007%
25	4.578	1001	1007	1010	rBV	822	910	0.11%	0.014%
26	4.632	1012	1024	1049	rBV	97985	279333	34.35%	4.406%
27	4.957	1123	1125	1129	rVB	985	552	0.07%	0.009%
28	4.983	1129	1133	1134	rBB	137	201	0.02%	0.003%
29	5.063	1144	1158	1180	rVB2	164350	359737	44.23%	5.675%
30	5.221	1205	1207	1210	rBV	583	308	0.04%	0.005%
31	5.295	1227	1230	1236	rVB2	1584	1394	0.17%	0.022%
32	5.327	1236	1240	1242	rBV	978	754	0.09%	0.012%
33	5.343	1242	1245	1247	rBV2	647	440	0.05%	0.007%
34	5.398	1259	1262	1266	rBV2	690	640	0.08%	0.010%
35	5.449	1275	1278	1279	rBV2	461	255	0.03%	0.004%
36	5.526	1298	1302	1305	rBV	304	278	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049085.D
 Acq On : 12 Jun 2022 12:51
 Operator : SY/MD
 Sample : N3255-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.546	1305	1308	1312	rVB	858	621	0.08%	0.010%
38	5.568	1312	1315	1321	rBV	855	872	0.11%	0.014%
39	5.726	1344	1364	1391	rBV3	289175	813278	100.00%	12.829%
40	6.144	1492	1494	1496	rBV	251	138	0.02%	0.002%
41	6.185	1504	1507	1512	rBV	753	583	0.07%	0.009%
42	6.250	1513	1527	1549	rBV	277932	528260	64.95%	8.333%
43	6.443	1584	1587	1590	rBV3	774	610	0.08%	0.010%
44	6.497	1600	1604	1606	rBV	1063	756	0.09%	0.012%
45	6.530	1606	1614	1623	rVV6	3718	6158	0.76%	0.097%
46	6.690	1650	1664	1688	rBV	195341	383082	47.10%	6.043%
47	6.912	1730	1733	1736	rBV2	945	729	0.09%	0.011%
48	6.993	1755	1758	1760	rBV	488	290	0.04%	0.005%
49	7.050	1773	1776	1779	rBV2	702	423	0.05%	0.007%
50	7.079	1783	1785	1787	rBV	402	210	0.03%	0.003%
51	7.128	1796	1800	1803	rBV2	705	524	0.06%	0.008%
52	7.144	1803	1805	1807	rBV	417	262	0.03%	0.004%
53	7.256	1836	1840	1842	rBV	1021	840	0.10%	0.013%
54	7.423	1890	1892	1897	rBV2	440	397	0.05%	0.006%
55	7.481	1908	1910	1916	rVB	731	542	0.07%	0.009%
56	7.513	1916	1920	1924	rBV	890	901	0.11%	0.014%
57	7.565	1924	1936	1960	rVV2	88528	162138	19.94%	2.558%
58	7.777	1999	2002	2004	rBV2	711	429	0.05%	0.007%
59	7.838	2018	2021	2022	rBV	678	364	0.04%	0.006%
60	7.899	2028	2040	2057	rBV	316603	547666	67.34%	8.639%
61	8.179	2117	2127	2148	rBV	61905	110010	13.53%	1.735%
62	8.587	2251	2254	2256	rBV2	553	436	0.05%	0.007%
63	8.639	2257	2270	2297	rVV4	268931	559617	68.81%	8.828%
64	8.925	2356	2359	2361	rBV	687	487	0.06%	0.008%
65	9.060	2398	2401	2405	rVB	668	430	0.05%	0.007%
66	9.082	2405	2408	2413	rBV	740	711	0.09%	0.011%
67	9.285	2468	2471	2474	rBV2	584	413	0.05%	0.007%
68	9.417	2500	2512	2534	rBV	383837	638707	78.53%	10.075%
69	9.571	2558	2560	2561	rBV	520	255	0.03%	0.004%
70	10.066	2710	2714	2716	rBV	838	596	0.07%	0.009%
71	10.163	2742	2744	2746	rVB	388	154	0.02%	0.002%
72	10.182	2746	2750	2754	rBV	789	729	0.09%	0.011%
73	10.221	2759	2762	2764	rBV2	566	405	0.05%	0.006%
74	10.314	2787	2791	2796	rBV	1168	1487	0.18%	0.023%
75	10.401	2812	2818	2819	rBV	605	678	0.08%	0.011%
76	10.510	2846	2852	2855	rBV	968	1274	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049085.D
 Acq On : 12 Jun 2022 12:51
 Operator : SY/MD
 Sample : N3255-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

77	10.558	2863	2867	2871	rBV	473	611	0.08%	0.010%
78	10.758	2917	2929	2943	rBV	312527	503641	61.93%	7.945%
79	10.983	2993	2999	3002	rBV	983	1047	0.13%	0.017%
80	11.423	3132	3136	3138	rBV	1002	692	0.09%	0.011%
81	11.812	3246	3257	3273	rBV	315093	501114	61.62%	7.905%
82	12.002	3313	3316	3318	rBV2	620	467	0.06%	0.007%
83	12.192	3364	3375	3391	rBV	309251	497371	61.16%	7.846%
84	12.346	3417	3423	3426	rBV2	1317	1394	0.17%	0.022%




Sum of corrected areas: 6339315

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049085.D
Acq On : 12 Jun 2022 12:51
Operator : SY/MD
Sample : N3255-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

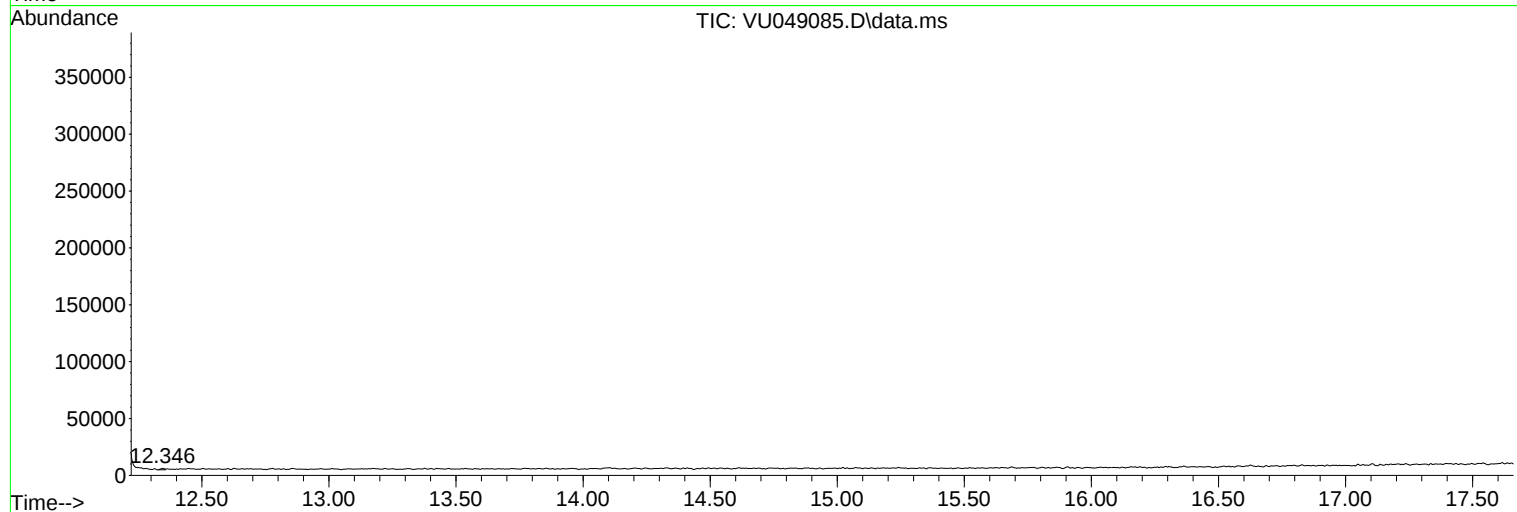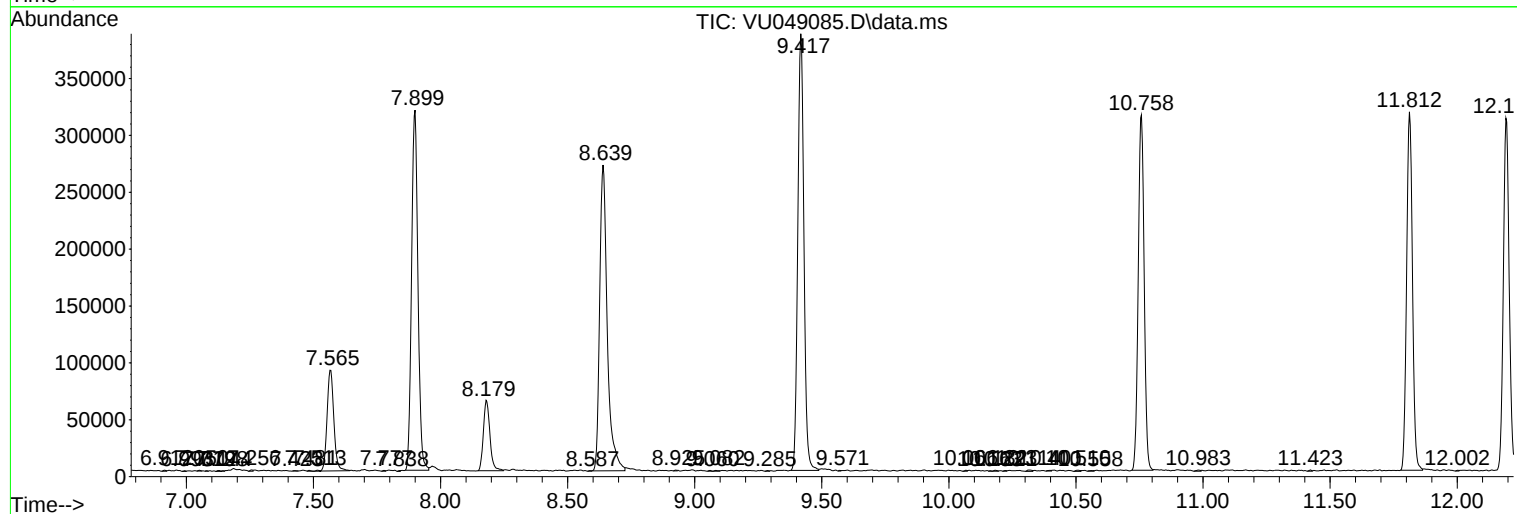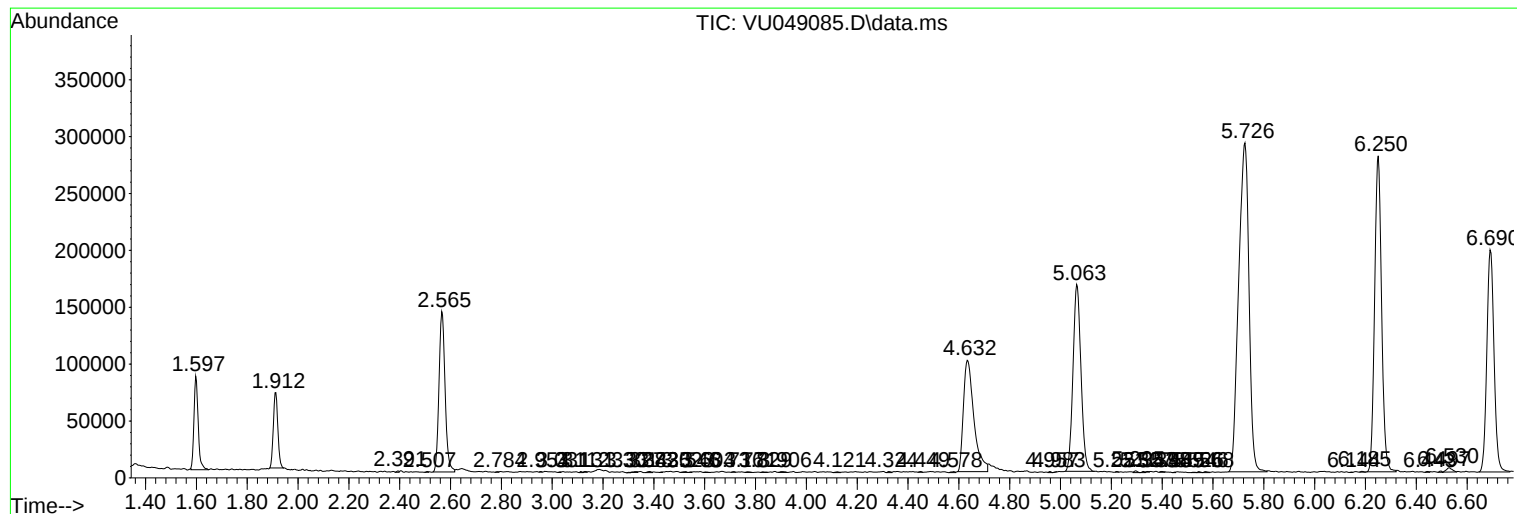

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049085.D
Acq On : 12 Jun 2022 12:51
Operator : SY/MD
Sample : N3255-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049085.D
Acq On : 12 Jun 2022 12:51
Operator : SY/MD
Sample : N3255-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
