

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049086.D
 Acq On : 12 Jun 2022 13:15
 Operator : SY/MD
 Sample : N3255-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	80078	94244	11.08%	1.429%
2	1.909	170	177	191	rVB	69553	88656	10.43%	1.344%
3	2.243	278	281	282	rBV2	866	534	0.06%	0.008%
4	2.498	353	360	366	rBV3	1278	1443	0.17%	0.022%
5	2.565	369	381	399	rBV	144745	240276	28.26%	3.643%
6	2.780	446	448	450	rBV	684	382	0.04%	0.006%
7	3.051	530	532	535	rBV2	307	217	0.03%	0.003%
8	3.102	545	548	550	rBV2	420	287	0.03%	0.004%
9	3.388	635	637	640	rVB	609	320	0.04%	0.005%
10	3.414	640	645	650	rBV2	676	781	0.09%	0.012%
11	3.497	662	671	674	rBV2	595	849	0.10%	0.013%
12	3.517	674	677	678	rBV	484	284	0.03%	0.004%
13	3.578	693	696	702	rBV	591	582	0.07%	0.009%
14	3.607	702	705	708	rBV	953	623	0.07%	0.009%
15	3.819	768	771	773	rBV	511	301	0.04%	0.005%
16	3.851	778	781	782	rBV2	672	355	0.04%	0.005%
17	3.887	789	792	796	rBV2	416	396	0.05%	0.006%
18	3.986	821	823	829	rVB	1030	667	0.08%	0.010%
19	4.018	829	833	835	rBV	663	547	0.06%	0.008%
20	4.086	850	854	857	rBV	590	529	0.06%	0.008%
21	4.279	912	914	917	rBV2	364	280	0.03%	0.004%
22	4.404	950	953	954	rBV2	193	119	0.01%	0.002%
23	4.446	963	966	968	rBV2	599	408	0.05%	0.006%
24	4.629	1012	1023	1062	rBV	100941	273480	32.17%	4.146%
25	4.980	1127	1132	1136	rBV2	788	882	0.10%	0.013%
26	5.063	1142	1158	1176	rBV2	163809	359095	42.24%	5.444%
27	5.227	1205	1209	1210	rBV2	419	279	0.03%	0.004%
28	5.240	1210	1213	1216	rVV2	598	425	0.05%	0.006%
29	5.481	1285	1288	1290	rBV2	702	541	0.06%	0.008%
30	5.517	1297	1299	1301	rBV	342	173	0.02%	0.003%
31	5.533	1301	1304	1307	rVV	550	334	0.04%	0.005%
32	5.568	1313	1315	1318	rBV	325	188	0.02%	0.003%
33	5.587	1318	1321	1323	rBV	513	394	0.05%	0.006%
34	5.629	1330	1334	1337	rBV	712	587	0.07%	0.009%
35	5.726	1342	1364	1393	rVV2	309748	850214	100.00%	12.890%
36	5.941	1426	1431	1432	rBV	886	636	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049086.D
 Acq On : 12 Jun 2022 13:15
 Operator : SY/MD
 Sample : N3255-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.076	1471	1473	1478	rVB	560	403	0.05%	0.006%
38	6.102	1478	1481	1483	rBV	661	465	0.05%	0.007%
39	6.250	1514	1527	1552	rBV	285544	546545	64.28%	8.286%
40	6.484	1598	1600	1603	rBV2	416	253	0.03%	0.004%
41	6.539	1606	1617	1630	rVV7	13656	26916	3.17%	0.408%
42	6.607	1635	1638	1640	rBV2	292	172	0.02%	0.003%
43	6.690	1650	1664	1686	rBV	202637	399194	46.95%	6.052%
44	6.796	1692	1697	1700	rBV2	790	830	0.10%	0.013%
45	6.841	1707	1711	1713	rBV	693	491	0.06%	0.007%
46	6.854	1713	1715	1717	rBV	372	225	0.03%	0.003%
47	6.931	1736	1739	1741	rBV2	798	592	0.07%	0.009%
48	7.047	1769	1775	1776	rBV	856	701	0.08%	0.011%
49	7.298	1851	1853	1856	rVB	716	356	0.04%	0.005%
50	7.320	1856	1860	1865	rBV	969	1001	0.12%	0.015%
51	7.369	1871	1875	1880	rBV	823	719	0.08%	0.011%
52	7.481	1907	1910	1912	rBV	582	337	0.04%	0.005%
53	7.565	1925	1936	1954	rBV2	91315	161133	18.95%	2.443%
54	7.681	1965	1972	1975	rBV2	1728	2283	0.27%	0.035%
55	7.755	1991	1995	1997	rBV	539	397	0.05%	0.006%
56	7.899	2027	2040	2056	rBV	343722	598598	70.41%	9.075%
57	8.179	2117	2127	2141	rBV	65568	110471	12.99%	1.675%
58	8.340	2174	2177	2180	rBV2	690	546	0.06%	0.008%
59	8.436	2199	2207	2211	rBV	866	1224	0.14%	0.019%
60	8.462	2211	2215	2218	rBV2	774	710	0.08%	0.011%
61	8.639	2258	2270	2296	rBV3	282576	564600	66.41%	8.560%
62	8.896	2347	2350	2353	rVB	988	633	0.07%	0.010%
63	8.912	2353	2355	2357	rBV2	446	271	0.03%	0.004%
64	9.047	2393	2397	2401	rBV	1017	994	0.12%	0.015%
65	9.272	2465	2467	2470	rBV	451	213	0.03%	0.003%
66	9.288	2470	2472	2473	rBV	494	222	0.03%	0.003%
67	9.317	2479	2481	2483	rBV	465	255	0.03%	0.004%
68	9.417	2499	2512	2533	rBV	404065	675653	79.47%	10.243%
69	9.597	2563	2568	2571	rBV2	831	778	0.09%	0.012%
70	9.687	2594	2596	2600	rVV2	721	413	0.05%	0.006%
71	9.722	2604	2607	2611	rBV	727	551	0.06%	0.008%
72	9.745	2611	2614	2618	rVB2	558	387	0.05%	0.006%
73	9.828	2638	2640	2642	rBV2	486	283	0.03%	0.004%
74	10.131	2730	2734	2736	rBV	674	518	0.06%	0.008%
75	10.192	2751	2753	2758	rBV	521	503	0.06%	0.008%
76	10.430	2824	2827	2831	rVB	908	552	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049086.D
 Acq On : 12 Jun 2022 13:15
 Operator : SY/MD
 Sample : N3255-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	10.452	2831	2834	2836	rBV	394	261	0.03%	0.004%
78	10.465	2836	2838	2842	rBV	695	406	0.05%	0.006%
79	10.494	2842	2847	2849	rBV2	679	638	0.08%	0.010%
80	10.758	2917	2929	2943	rBV	314603	506612	59.59%	7.680%
81	10.928	2979	2982	2987	rBV2	705	832	0.10%	0.013%
82	11.070	3022	3026	3030	rBV	1153	1148	0.14%	0.017%
83	11.192	3059	3064	3069	rBV2	691	962	0.11%	0.015%
84	11.812	3245	3257	3273	rBV	333753	531739	62.54%	8.061%
85	12.147	3358	3361	3363	rBV	571	373	0.04%	0.006%
86	12.192	3363	3375	3392	rVV	319896	529076	62.23%	8.021%
87	12.651	3515	3518	3520	rBV	760	547	0.06%	0.008%
88	12.925	3600	3603	3605	rBV2	944	620	0.07%	0.009%
89	12.976	3616	3619	3622	rBV2	1171	886	0.10%	0.013%
90	13.465	3768	3771	3772	rBV2	525	293	0.03%	0.004%


Sum of corrected areas: 6596089

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049086.D
Acq On : 12 Jun 2022 13:15
Operator : SY/MD
Sample : N3255-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

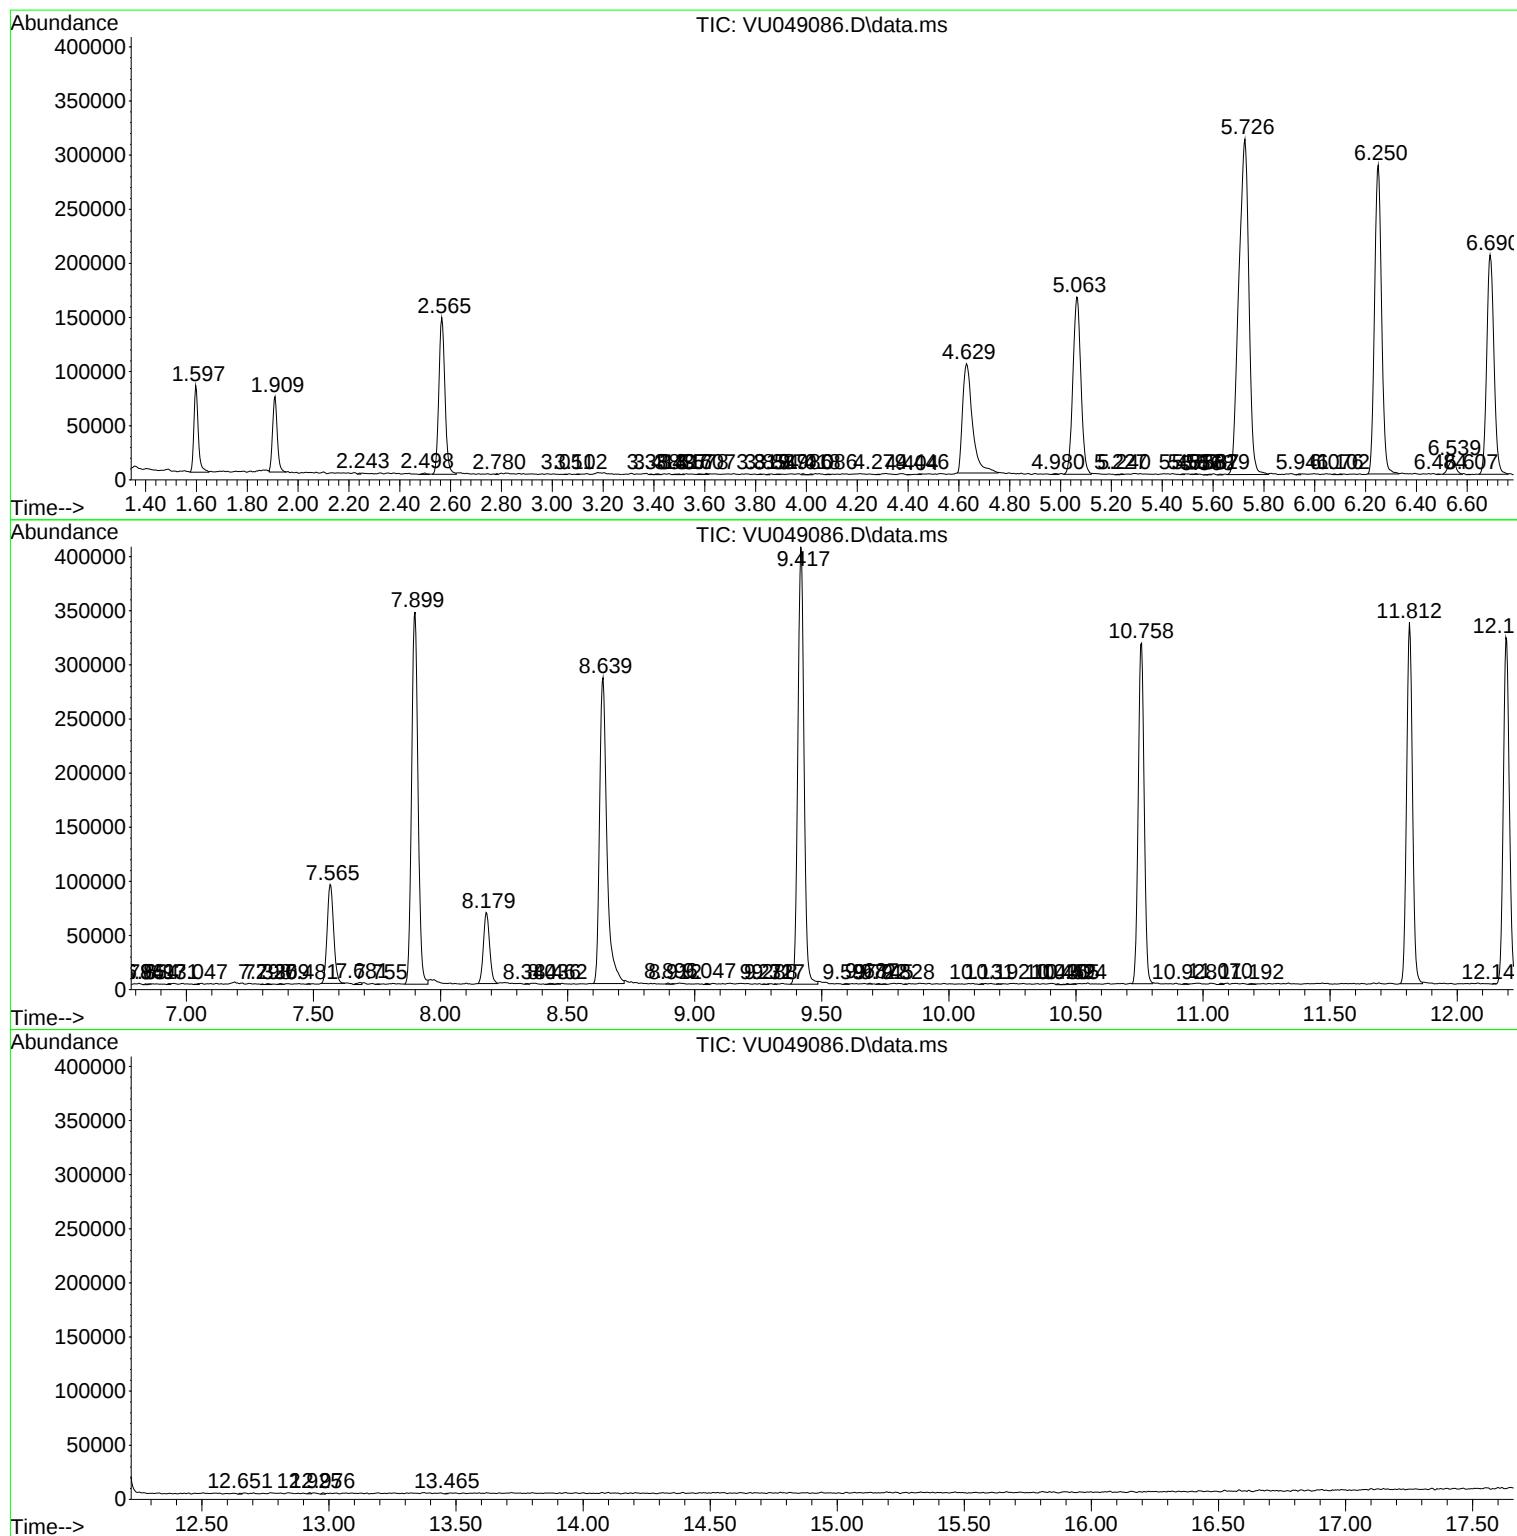

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049086.D
Acq On : 12 Jun 2022 13:15
Operator : SY/MD
Sample : N3255-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049086.D
Acq On : 12 Jun 2022 13:15
Operator : SY/MD
Sample : N3255-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------