

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049087.D
 Acq On : 12 Jun 2022 13:38
 Operator : SY/MD
 Sample : N3255-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

Signal : TIC: VU049087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	92050	101258	11.56%	1.459%
2	1.906	170	176	186	rVB	67503	79689	9.10%	1.149%
3	2.478	352	354	356	rBV	427	236	0.03%	0.003%
4	2.565	369	381	398	rBV2	194148	372204	42.49%	5.365%
5	2.761	439	442	446	rVB2	802	567	0.06%	0.008%
6	2.784	446	449	454	rBV2	929	919	0.10%	0.013%
7	2.954	499	502	505	rBV3	869	608	0.07%	0.009%
8	2.973	505	508	510	rVB2	729	393	0.04%	0.006%
9	3.115	549	552	555	rBV	802	618	0.07%	0.009%
10	3.153	560	564	566	rBV	829	684	0.08%	0.010%
11	3.298	606	609	612	rBV	543	389	0.04%	0.006%
12	3.549	684	687	690	rBV	840	728	0.08%	0.010%
13	3.719	738	740	742	rBV	338	181	0.02%	0.003%
14	3.800	763	765	768	rBV2	359	204	0.02%	0.003%
15	3.867	773	786	788	rBV2	3508	4703	0.54%	0.068%
16	3.986	818	823	824	rBV	770	547	0.06%	0.008%
17	4.031	834	837	840	rBV	734	505	0.06%	0.007%
18	4.276	909	913	916	rBV	807	740	0.08%	0.011%
19	4.340	927	933	938	rBV2	651	1019	0.12%	0.015%
20	4.449	963	967	970	rBV	947	747	0.09%	0.011%
21	4.491	978	980	984	rVB	693	358	0.04%	0.005%
22	4.513	984	987	990	rBV	776	629	0.07%	0.009%
23	4.578	1004	1007	1010	rBV	734	608	0.07%	0.009%
24	4.632	1011	1024	1029	rBV	105794	226012	25.80%	3.258%
25	4.973	1126	1130	1132	rBV2	837	656	0.07%	0.009%
26	5.063	1144	1158	1183	rVB	179905	399985	45.66%	5.765%
27	5.195	1197	1199	1203	rBV	435	229	0.03%	0.003%
28	5.417	1265	1268	1271	rVB2	537	324	0.04%	0.005%
29	5.436	1271	1274	1276	rBV	238	168	0.02%	0.002%
30	5.459	1278	1281	1284	rVB2	1153	700	0.08%	0.010%
31	5.504	1292	1295	1298	rBV	798	535	0.06%	0.008%
32	5.726	1342	1364	1386	rBV2	321802	876033	100.00%	12.626%
33	5.912	1418	1422	1425	rBV	1118	640	0.07%	0.009%
34	5.928	1425	1427	1429	rBV2	490	233	0.03%	0.003%
35	5.983	1441	1444	1447	rVB	861	525	0.06%	0.008%
36	6.005	1447	1451	1454	rBV2	981	764	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049087.D
 Acq On : 12 Jun 2022 13:38
 Operator : SY/MD
 Sample : N3255-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.115	1483	1485	1487	rBV2	270	142	0.02%	0.002%
38	6.250	1513	1527	1547	rBV	308592	582312	66.47%	8.393%
39	6.382	1565	1568	1570	rBV	596	445	0.05%	0.006%
40	6.539	1605	1617	1630	rBV6	15043	30946	3.53%	0.446%
41	6.690	1650	1664	1688	rBV	210045	410570	46.87%	5.918%
42	6.777	1688	1691	1693	rBV	720	439	0.05%	0.006%
43	6.912	1729	1733	1739	rBV2	1040	857	0.10%	0.012%
44	7.018	1764	1766	1768	rBV	451	237	0.03%	0.003%
45	7.185	1813	1818	1831	rBV6	1954	3775	0.43%	0.054%
46	7.259	1839	1841	1844	rBV	487	345	0.04%	0.005%
47	7.298	1851	1853	1855	rBV	414	246	0.03%	0.004%
48	7.427	1890	1893	1896	rBV	452	408	0.05%	0.006%
49	7.484	1908	1911	1915	rBV	827	708	0.08%	0.010%
50	7.565	1925	1936	1953	rBV2	94529	168376	19.22%	2.427%
51	7.732	1985	1988	1991	rBV	694	568	0.06%	0.008%
52	7.771	1997	2000	2004	rVB2	897	702	0.08%	0.010%
53	7.793	2004	2007	2010	rBV	552	471	0.05%	0.007%
54	7.841	2019	2022	2024	rBV	326	200	0.02%	0.003%
55	7.899	2024	2040	2056	rBV	361385	628866	71.79%	9.064%
56	8.179	2116	2127	2143	rBV	68529	115745	13.21%	1.668%
57	8.256	2148	2151	2154	rBV	997	763	0.09%	0.011%
58	8.336	2173	2176	2180	rBV	1166	820	0.09%	0.012%
59	8.385	2188	2191	2193	rBV2	701	506	0.06%	0.007%
60	8.462	2209	2215	2219	rBV2	1178	1541	0.18%	0.022%
61	8.639	2255	2270	2299	rBV2	278423	563426	64.32%	8.121%
62	8.806	2319	2322	2324	rBV2	641	395	0.05%	0.006%
63	9.208	2444	2447	2449	rBV	611	404	0.05%	0.006%
64	9.230	2451	2454	2458	rVB	630	467	0.05%	0.007%
65	9.314	2473	2480	2483	rBV2	558	747	0.09%	0.011%
66	9.417	2499	2512	2528	rBV	419132	696983	79.56%	10.046%
67	9.558	2554	2556	2559	rBV2	600	376	0.04%	0.005%
68	9.664	2587	2589	2592	rBV2	643	451	0.05%	0.007%
69	9.886	2655	2658	2661	rBV	819	658	0.08%	0.009%
70	9.947	2674	2677	2681	rVB2	565	387	0.04%	0.006%
71	9.967	2681	2683	2685	rBV	363	221	0.03%	0.003%
72	10.208	2755	2758	2761	rBV	432	277	0.03%	0.004%
73	10.288	2780	2783	2784	rBV2	666	342	0.04%	0.005%
74	10.545	2860	2863	2867	rBV	583	539	0.06%	0.008%
75	10.713	2911	2915	2916	rBV	632	460	0.05%	0.007%
76	10.758	2917	2929	2949	rVB2	316508	518014	59.13%	7.466%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049087.D
 Acq On : 12 Jun 2022 13:38
 Operator : SY/MD
 Sample : N3255-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

77	11.012	3001	3008	3010	rBV2	822	1084	0.12%	0.016%
78	11.192	3062	3064	3066	rBV2	625	337	0.04%	0.005%
79	11.230	3072	3076	3078	rBV	846	647	0.07%	0.009%
80	11.298	3090	3097	3099	rBV	806	945	0.11%	0.014%
81	11.356	3113	3115	3121	rBV	649	695	0.08%	0.010%
82	11.459	3142	3147	3149	rBV2	836	856	0.10%	0.012%
83	11.735	3230	3233	3236	rBV	718	655	0.07%	0.009%
84	11.812	3245	3257	3278	rBV	362699	568809	64.93%	8.198%
85	12.195	3364	3376	3394	rBV	339424	550455	62.83%	7.934%
86	12.500	3469	3471	3473	rBV	635	386	0.04%	0.006%
87	12.581	3493	3496	3499	rVB2	888	507	0.06%	0.007%
88	12.661	3518	3521	3524	rVB	1353	815	0.09%	0.012%
89	12.716	3535	3538	3540	rBV	691	448	0.05%	0.006%
90	12.931	3600	3605	3607	rBV2	673	676	0.08%	0.010%
91	13.259	3704	3707	3712	rBV2	795	782	0.09%	0.011%
92	14.491	4087	4090	4092	rBV	608	504	0.06%	0.007%




Sum of corrected areas: 6938074

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049087.D
Acq On : 12 Jun 2022 13:38
Operator : SY/MD
Sample : N3255-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

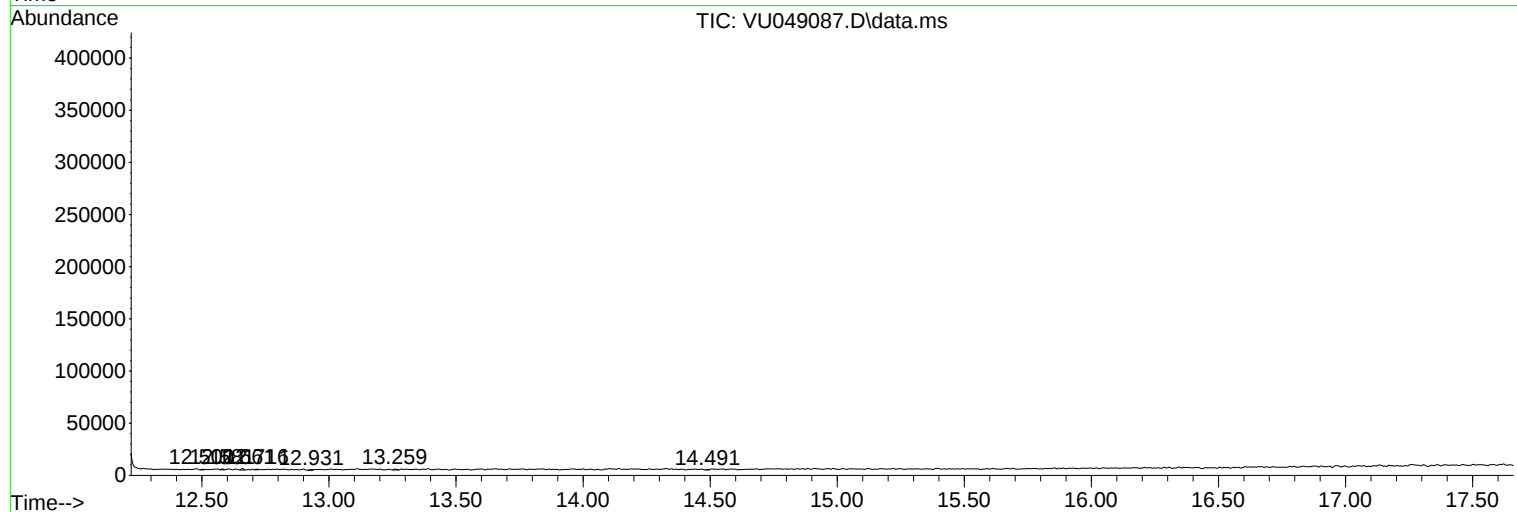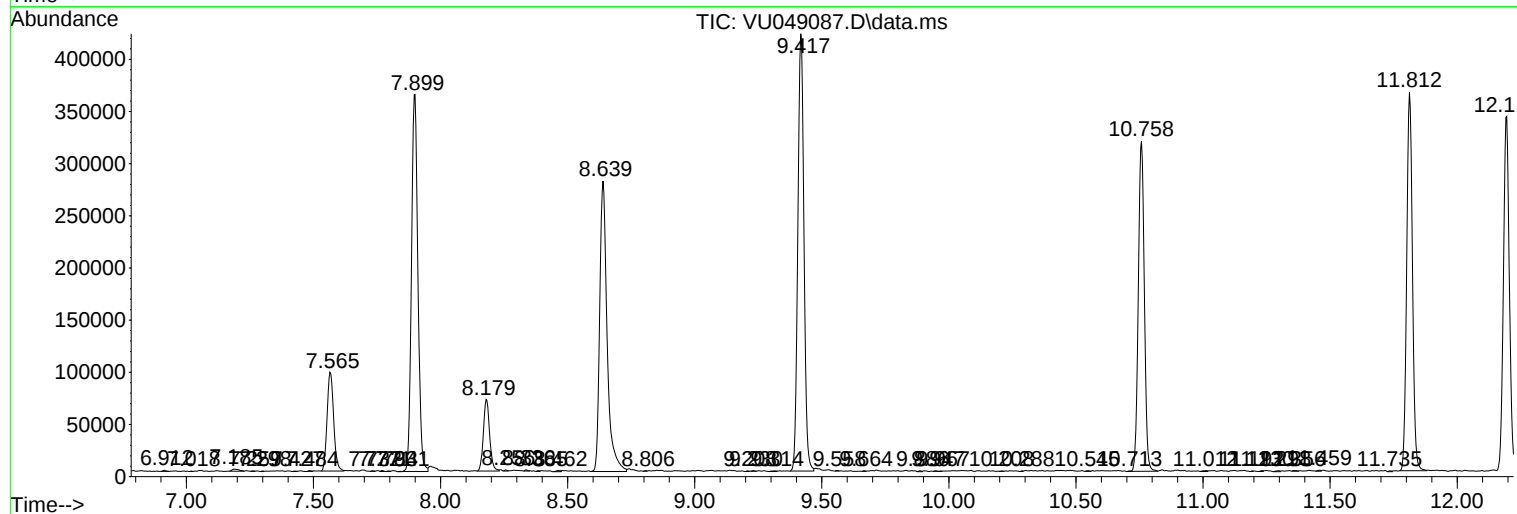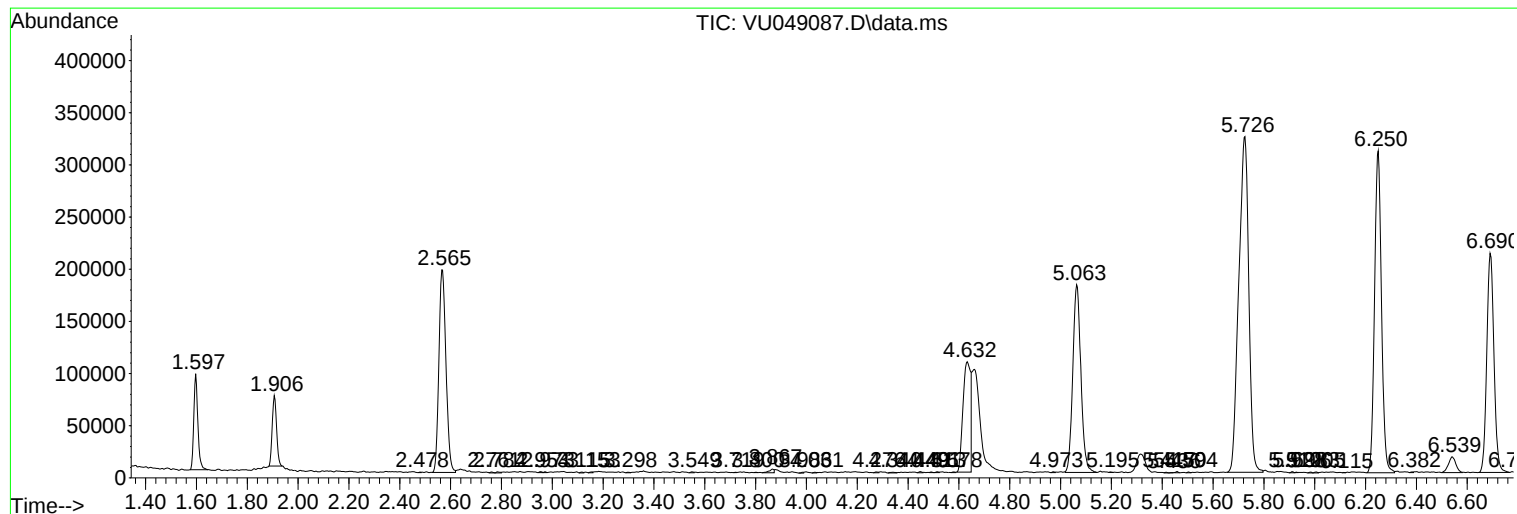

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049087.D
Acq On : 12 Jun 2022 13:38
Operator : SY/MD
Sample : N3255-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049087.D
Acq On : 12 Jun 2022 13:38
Operator : SY/MD
Sample : N3255-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------