

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049090.D
 Acq On : 12 Jun 2022 14:49
 Operator : SY/MD
 Sample : N3255-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	95	rVB	97435	107221	12.28%	1.583%
2	1.899	166	174	190	rVB	71712	95522	10.94%	1.410%
3	2.420	333	336	337	rBV	1096	568	0.07%	0.008%
4	2.562	368	380	398	rBV	162990	270613	30.99%	3.996%
5	2.713	423	427	434	rBV2	746	1049	0.12%	0.015%
6	2.755	437	440	443	rBV2	1209	939	0.11%	0.014%
7	3.282	601	604	608	rBV	915	798	0.09%	0.012%
8	3.639	713	715	718	rBV	532	308	0.04%	0.005%
9	3.658	718	721	723	rBV	821	541	0.06%	0.008%
10	3.732	739	744	750	rVB2	780	1123	0.13%	0.017%
11	3.764	750	754	757	rBV2	582	543	0.06%	0.008%
12	3.851	778	781	784	rBV2	560	347	0.04%	0.005%
13	3.877	784	789	790	rBV2	751	655	0.08%	0.010%
14	4.044	838	841	843	rBV	630	422	0.05%	0.006%
15	4.099	855	858	862	rBV2	747	643	0.07%	0.009%
16	4.259	904	908	909	rBV	847	563	0.06%	0.008%
17	4.362	937	940	944	rBV2	805	690	0.08%	0.010%
18	4.417	949	957	960	rBV	1108	1450	0.17%	0.021%
19	4.504	979	984	989	rBV2	934	1091	0.12%	0.016%
20	4.620	1008	1020	1043	rBV2	106098	256259	29.35%	3.784%
21	4.980	1130	1132	1135	rBV2	449	249	0.03%	0.004%
22	5.063	1143	1158	1175	rBV2	166990	368955	42.26%	5.448%
23	5.205	1199	1202	1205	rBV	1014	598	0.07%	0.009%
24	5.337	1241	1243	1247	rBV	608	476	0.05%	0.007%
25	5.722	1341	1363	1386	rBV2	316113	873107	100.00%	12.892%
26	5.893	1413	1416	1419	rBV	872	489	0.06%	0.007%
27	6.247	1514	1526	1548	rBV	296777	559050	64.03%	8.255%
28	6.452	1587	1590	1592	rBV	757	558	0.06%	0.008%
29	6.539	1606	1617	1630	rBV5	14934	29578	3.39%	0.437%
30	6.623	1638	1643	1646	rVB	641	651	0.07%	0.010%
31	6.690	1650	1664	1681	rVV	206714	399454	45.75%	5.898%
32	6.957	1744	1747	1751	rBV2	452	339	0.04%	0.005%
33	6.980	1751	1754	1756	rBV	775	542	0.06%	0.008%
34	7.427	1890	1893	1896	rBV	1002	631	0.07%	0.009%
35	7.484	1909	1911	1912	rBV	496	236	0.03%	0.003%
36	7.565	1924	1936	1952	rBV	94234	165765	18.99%	2.448%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049090.D
 Acq On : 12 Jun 2022 14:49
 Operator : SY/MD
 Sample : N3255-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	7.896	2026	2039	2057	rBV	358522	624054	71.48%	9.214%
38	8.179	2116	2127	2145	rBV	66799	114131	13.07%	1.685%
39	8.404	2193	2197	2202	rBV2	865	966	0.11%	0.014%
40	8.533	2234	2237	2239	rBV	840	450	0.05%	0.007%
41	8.632	2253	2268	2298	rBV3	271603	538681	61.70%	7.954%
42	8.883	2343	2346	2348	rBV	553	424	0.05%	0.006%
43	8.951	2365	2367	2372	rBV	861	708	0.08%	0.010%
44	9.015	2383	2387	2390	rBV2	811	869	0.10%	0.013%
45	9.176	2433	2437	2440	rBV	1108	871	0.10%	0.013%
46	9.240	2452	2457	2459	rBV2	626	632	0.07%	0.009%
47	9.372	2493	2498	2499	rBV	950	773	0.09%	0.011%
48	9.417	2500	2512	2529	rVV	414592	681998	78.11%	10.070%
49	9.587	2562	2565	2568	rBV2	970	751	0.09%	0.011%
50	9.989	2685	2690	2696	rVB	1192	1567	0.18%	0.023%
51	10.025	2696	2701	2706	rBV2	1226	1719	0.20%	0.025%
52	10.147	2736	2739	2742	rBV2	566	335	0.04%	0.005%
53	10.574	2869	2872	2875	rBV	872	572	0.07%	0.008%
54	10.754	2917	2928	2945	rVB	319308	516615	59.17%	7.628%
55	11.098	3030	3035	3040	rVB2	867	1067	0.12%	0.016%
56	11.176	3056	3059	3061	rBV	585	417	0.05%	0.006%
57	11.539	3169	3172	3175	rBV	775	575	0.07%	0.008%
58	11.664	3208	3211	3214	rBV	744	588	0.07%	0.009%
59	11.812	3245	3257	3277	rBV	352078	568027	65.06%	8.387%
60	12.063	3332	3335	3337	rBV	668	439	0.05%	0.006%
61	12.192	3360	3375	3398	rBV	346211	569201	65.19%	8.404%
62	12.446	3450	3454	3458	rBV2	858	863	0.10%	0.013%
63	12.864	3582	3584	3586	rBV	580	329	0.04%	0.005%
64	12.928	3602	3604	3607	rBV	685	462	0.05%	0.007%
65	13.266	3706	3709	3712	rBV	947	822	0.09%	0.012%
66	13.388	3745	3747	3753	rBV	912	770	0.09%	0.011%
67	14.108	3968	3971	3974	rBV3	1379	964	0.11%	0.014%




Sum of corrected areas: 6772663

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049090.D
Acq On : 12 Jun 2022 14:49
Operator : SY/MD
Sample : N3255-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

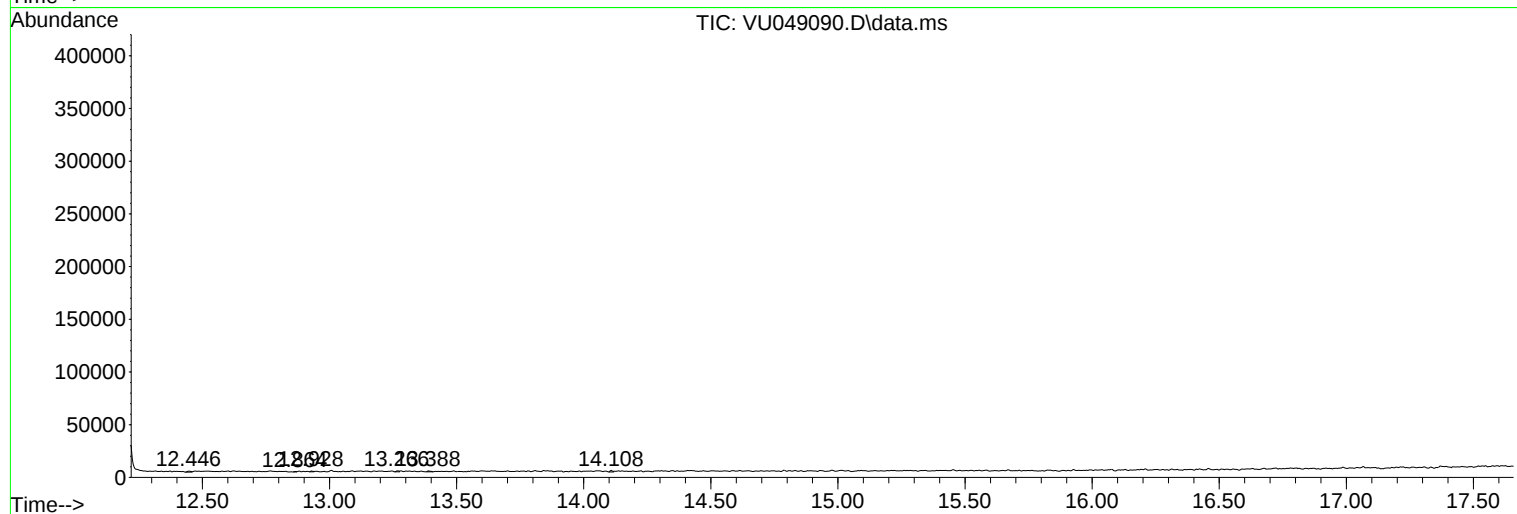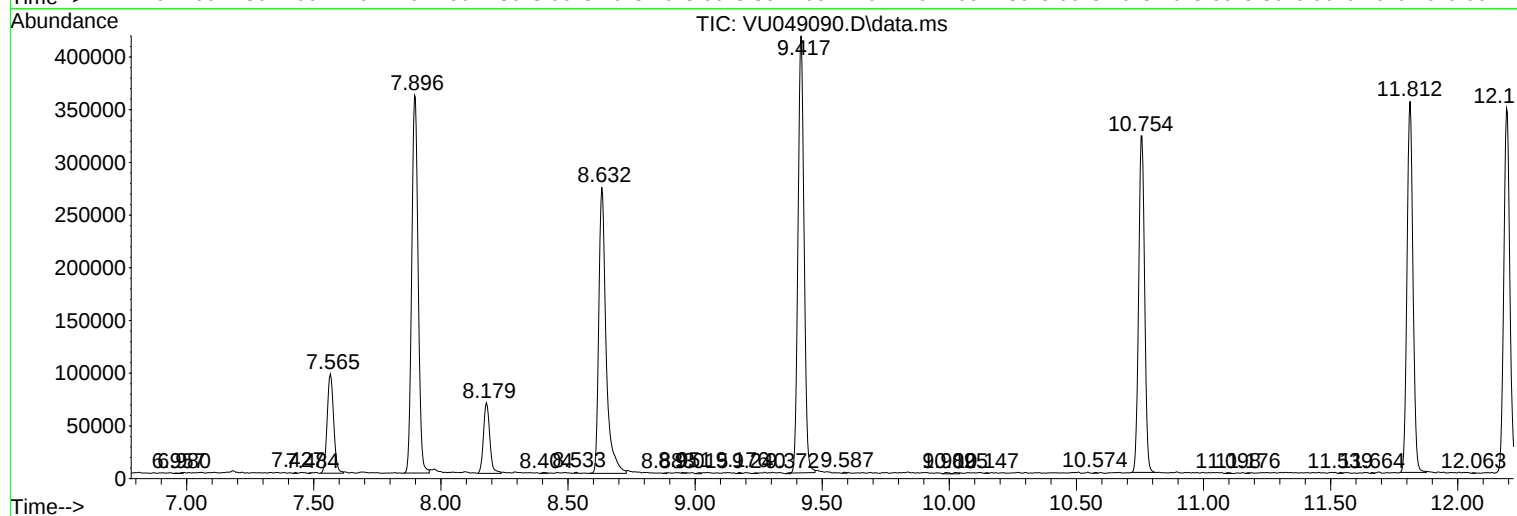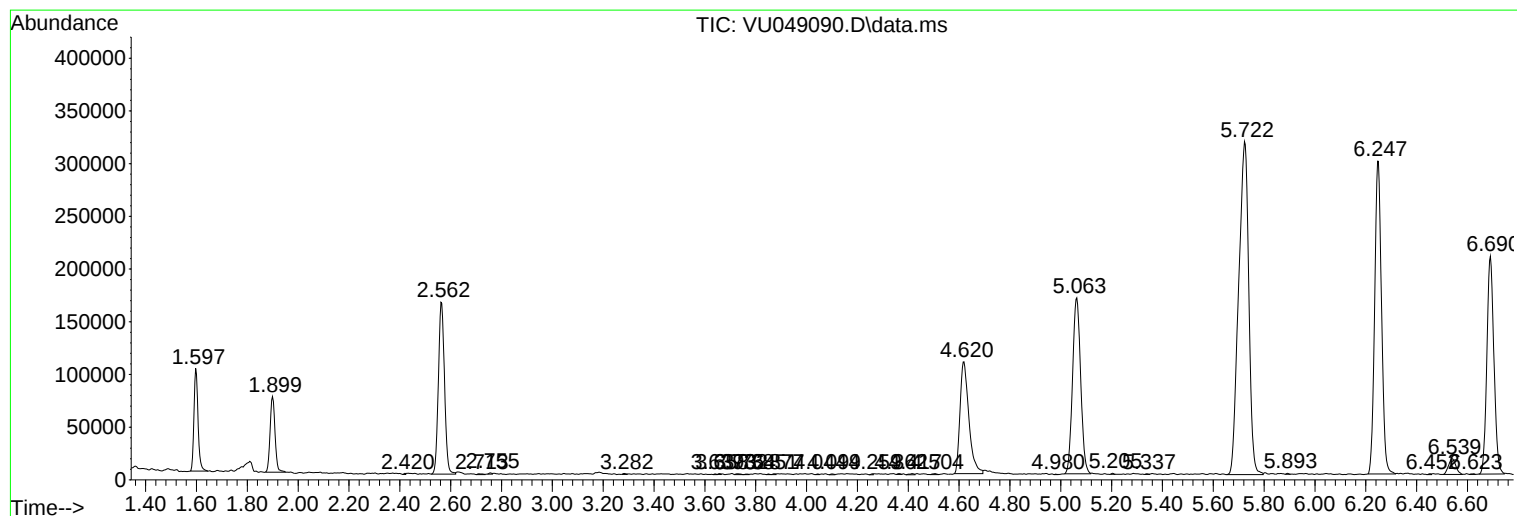

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049090.D
Acq On : 12 Jun 2022 14:49
Operator : SY/MD
Sample : N3255-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049090.D
Acq On : 12 Jun 2022 14:49
Operator : SY/MD
Sample : N3255-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc