

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049091.D
 Acq On : 12 Jun 2022 15:12
 Operator : SY/MD
 Sample : N3255-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	95172	106959	12.52%	1.566%
2	1.899	164	174	190	rBV	70418	98518	11.53%	1.443%
3	2.562	369	380	393	rVV	160773	265565	31.09%	3.889%
4	2.854	465	471	473	rBV	762	867	0.10%	0.013%
5	2.948	496	500	508	rVB2	991	1013	0.12%	0.015%
6	2.989	509	513	516	rBV2	902	791	0.09%	0.012%
7	3.092	541	545	550	rBV2	852	836	0.10%	0.012%
8	3.182	565	573	585	rVB4	2178	5027	0.59%	0.074%
9	3.308	609	612	616	rBV	812	671	0.08%	0.010%
10	3.359	623	628	631	rBV	758	742	0.09%	0.011%
11	3.452	654	657	660	rBV2	803	584	0.07%	0.009%
12	3.488	665	668	675	rVB2	656	691	0.08%	0.010%
13	3.520	675	678	682	rBV	681	589	0.07%	0.009%
14	3.552	685	688	693	rBV	597	606	0.07%	0.009%
15	3.626	708	711	715	rBV	717	573	0.07%	0.008%
16	3.665	720	723	726	rBV	839	668	0.08%	0.010%
17	4.006	821	829	832	rBV2	763	957	0.11%	0.014%
18	4.057	840	845	852	rBV	993	1454	0.17%	0.021%
19	4.205	884	891	894	rBV	765	974	0.11%	0.014%
20	4.459	967	970	978	rVB2	659	671	0.08%	0.010%
21	4.620	1007	1020	1045	rBV	106210	262128	30.68%	3.839%
22	4.944	1118	1121	1125	rVB	1197	987	0.12%	0.014%
23	4.973	1125	1130	1136	rBV3	816	1087	0.13%	0.016%
24	5.063	1140	1158	1178	rBV	167363	366892	42.95%	5.373%
25	5.443	1271	1276	1278	rBV	811	814	0.10%	0.012%
26	5.530	1299	1303	1306	rVV2	652	561	0.07%	0.008%
27	5.578	1314	1318	1323	rVB	1338	1255	0.15%	0.018%
28	5.607	1323	1327	1330	rBV2	667	616	0.07%	0.009%
29	5.629	1330	1334	1342	rVV2	539	848	0.10%	0.012%
30	5.726	1342	1364	1385	rBV2	310873	854312	100.00%	12.511%
31	5.803	1385	1388	1392	rVB3	1219	874	0.10%	0.013%
32	5.883	1407	1413	1416	rVB	949	963	0.11%	0.014%
33	6.028	1454	1458	1461	rBV	782	644	0.08%	0.009%
34	6.247	1511	1526	1547	rBV	301529	575292	67.34%	8.425%
35	6.340	1552	1555	1560	rBV2	946	723	0.08%	0.011%
36	6.436	1581	1585	1588	rVV2	679	581	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049091.D
 Acq On : 12 Jun 2022 15:12
 Operator : SY/MD
 Sample : N3255-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.456	1588	1591	1594	rVB2	907	601	0.07%	0.009%
38	6.488	1594	1601	1604	rBV2	955	1026	0.12%	0.015%
39	6.533	1604	1615	1624	rBV8	3232	6529	0.76%	0.096%
40	6.607	1634	1638	1642	rBV	842	724	0.08%	0.011%
41	6.690	1650	1664	1683	rBV	210534	402014	47.06%	5.887%
42	6.803	1694	1699	1701	rBV3	1444	1189	0.14%	0.017%
43	7.079	1782	1785	1790	rVB	863	772	0.09%	0.011%
44	7.115	1790	1796	1800	rBV	801	970	0.11%	0.014%
45	7.189	1806	1819	1826	rBV7	2277	4820	0.56%	0.071%
46	7.459	1897	1903	1906	rBV	666	797	0.09%	0.012%
47	7.565	1924	1936	1958	rVB	92820	160634	18.80%	2.352%
48	7.687	1966	1974	1980	rBV3	1686	1976	0.23%	0.029%
49	7.751	1991	1994	1999	rVB	916	804	0.09%	0.012%
50	7.796	1999	2008	2011	rBV	685	1124	0.13%	0.016%
51	7.822	2012	2016	2021	rBV	557	665	0.08%	0.010%
52	7.896	2025	2039	2056	rBV	354963	615543	72.05%	9.014%
53	8.179	2116	2127	2143	rBV	65412	110938	12.99%	1.625%
54	8.398	2192	2195	2197	rBV	828	588	0.07%	0.009%
55	8.632	2256	2268	2296	rBV2	272706	544492	63.73%	7.974%
56	8.809	2319	2323	2327	rBV2	760	719	0.08%	0.011%
57	9.047	2393	2397	2400	rBV	833	660	0.08%	0.010%
58	9.176	2435	2437	2441	rVB	947	696	0.08%	0.010%
59	9.201	2441	2445	2451	rVB2	705	897	0.10%	0.013%
60	9.301	2473	2476	2481	rBV2	795	657	0.08%	0.010%
61	9.417	2499	2512	2530	rBV	429321	706945	82.75%	10.353%
62	9.603	2567	2570	2579	rVB	1015	1173	0.14%	0.017%
63	9.655	2579	2586	2591	rVB	855	958	0.11%	0.014%
64	9.690	2591	2597	2602	rBV2	1115	1304	0.15%	0.019%
65	9.992	2688	2691	2694	rVB2	874	611	0.07%	0.009%
66	10.028	2699	2702	2707	rVB2	711	765	0.09%	0.011%
67	10.089	2718	2721	2730	rVB2	630	851	0.10%	0.012%
68	10.127	2730	2733	2737	rVB	1008	811	0.09%	0.012%
69	10.153	2737	2741	2746	rBV2	569	568	0.07%	0.008%
70	10.349	2798	2802	2805	rBV	826	604	0.07%	0.009%
71	10.388	2811	2814	2819	rBV	805	894	0.10%	0.013%
72	10.475	2838	2841	2846	rVB2	789	683	0.08%	0.010%
73	10.607	2878	2882	2884	rBV	688	577	0.07%	0.008%
74	10.655	2894	2897	2899	rBV2	909	643	0.08%	0.009%
75	10.684	2904	2906	2912	rVB	859	810	0.09%	0.012%
76	10.758	2917	2929	2948	rVB	324406	525443	61.50%	7.695%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049091.D
 Acq On : 12 Jun 2022 15:12
 Operator : SY/MD
 Sample : N3255-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	10.954	2985	2990	2993	rBV	811	754	0.09%	0.011%
78	11.002	3001	3005	3012	rBV2	1008	1415	0.17%	0.021%
79	11.137	3043	3047	3050	rVB	1011	747	0.09%	0.011%
80	11.516	3163	3165	3171	rVB	839	555	0.06%	0.008%
81	11.697	3217	3221	3224	rBV2	485	550	0.06%	0.008%
82	11.812	3244	3257	3273	rBV	370610	585758	68.56%	8.578%
83	11.970	3301	3306	3312	rVB2	989	995	0.12%	0.015%
84	12.192	3363	3375	3395	rBV	338255	563107	65.91%	8.246%
85	12.417	3442	3445	3455	rBV3	1213	1611	0.19%	0.024%
86	12.536	3477	3482	3485	rBV2	935	824	0.10%	0.012%
87	12.674	3522	3525	3530	rBV2	989	1023	0.12%	0.015%
88	12.832	3571	3574	3581	rVB	759	925	0.11%	0.014%
89	13.066	3644	3647	3653	rVB2	702	649	0.08%	0.010%
90	13.098	3653	3657	3661	rBV	940	889	0.10%	0.013%
91	13.237	3694	3700	3708	rBV2	973	1510	0.18%	0.022%
92	13.703	3843	3845	3850	rVB2	1041	660	0.08%	0.010%
93	13.751	3855	3860	3862	rBV	720	797	0.09%	0.012%
94	14.111	3969	3972	3976	rVB2	922	760	0.09%	0.011%
95	14.134	3976	3979	3982	rBV2	773	622	0.07%	0.009%
96	14.359	4045	4049	4050	rBV	897	649	0.08%	0.010%
97	14.815	4188	4191	4193	rBV2	728	556	0.07%	0.008%
98	15.092	4273	4277	4281	rBV2	1006	919	0.11%	0.013%
99	15.561	4419	4423	4424	rBV	977	723	0.08%	0.011%
100	15.613	4436	4439	4443	rBV3	984	869	0.10%	0.013%




Sum of corrected areas: 6828675

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049091.D
Acq On : 12 Jun 2022 15:12
Operator : SY/MD
Sample : N3255-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

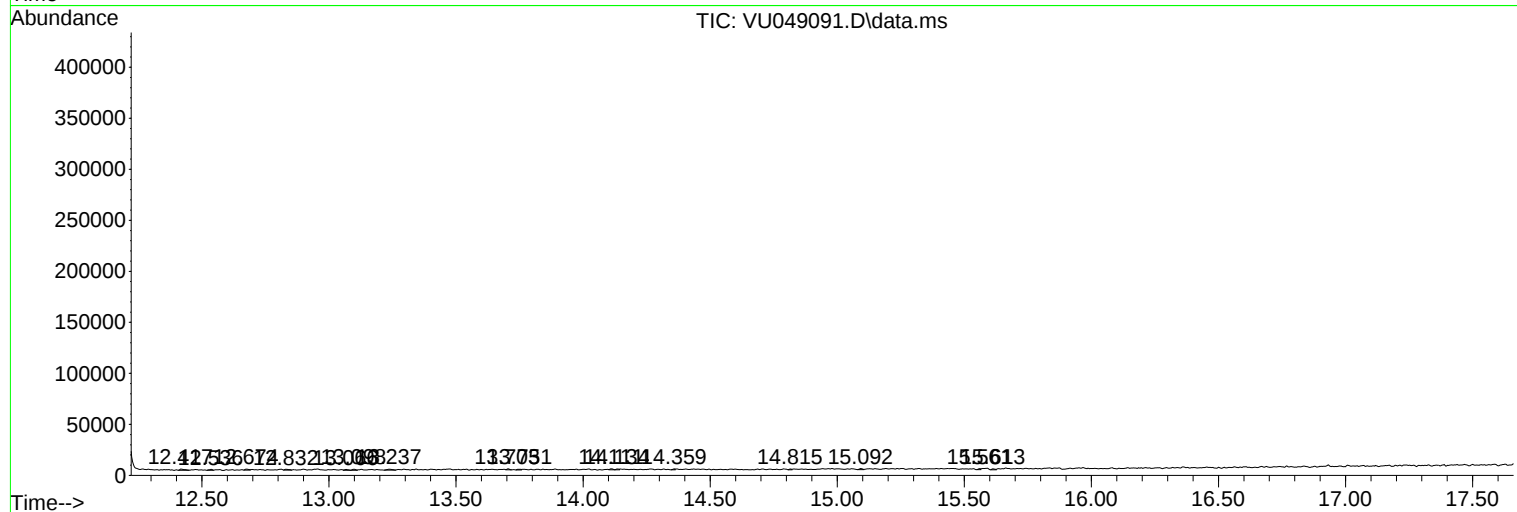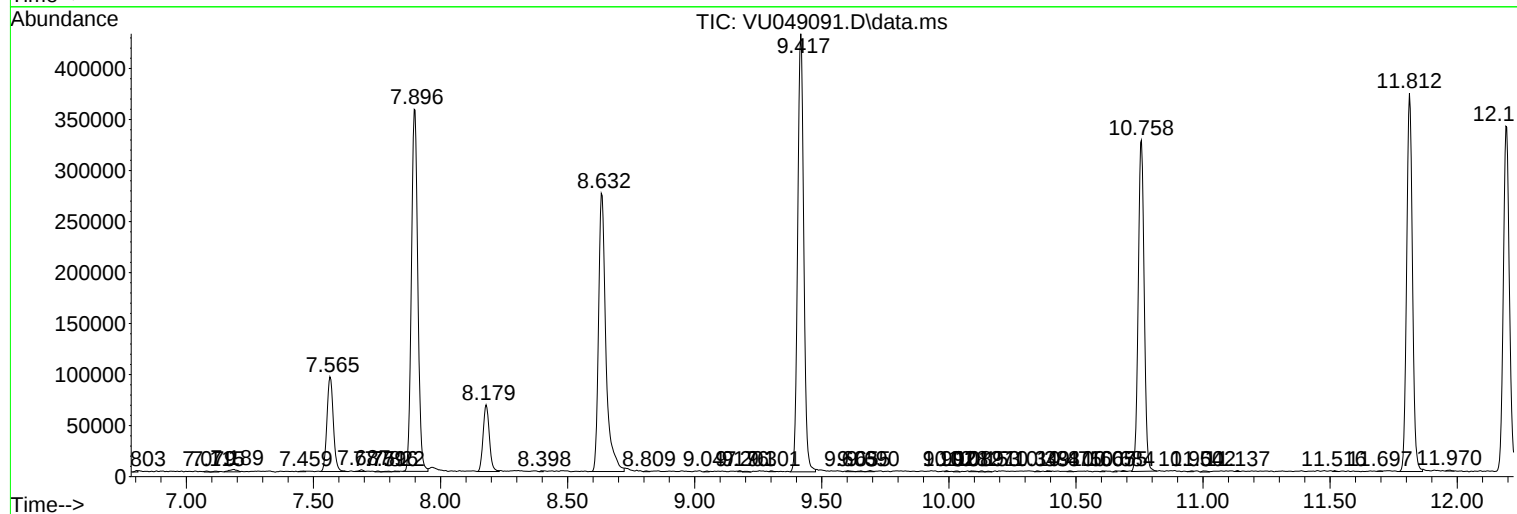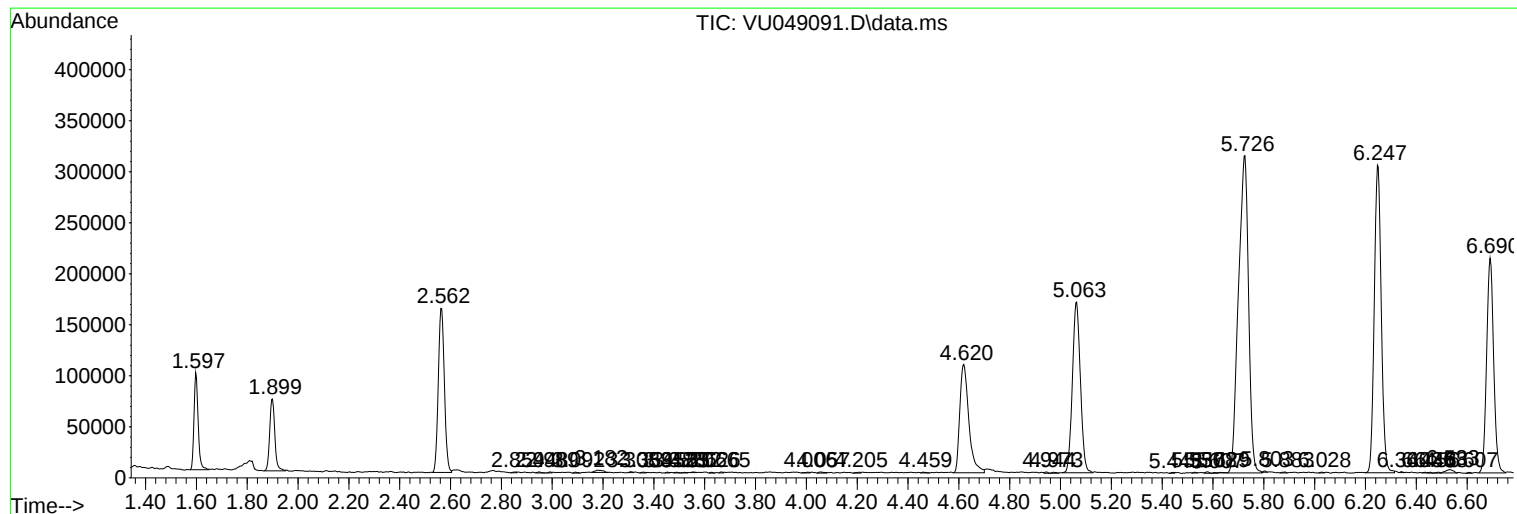

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049091.D
Acq On : 12 Jun 2022 15:12
Operator : SY/MD
Sample : N3255-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049091.D
Acq On : 12 Jun 2022 15:12
Operator : SY/MD
Sample : N3255-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------