

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049092.D
 Acq On : 12 Jun 2022 15:36
 Operator : SY/MD
 Sample : N3255-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049092.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	75160	89244	10.78%	1.433%
2	1.893	168	172	184	rVB	70303	87405	10.55%	1.404%
3	2.308	298	301	303	rBV2	890	615	0.07%	0.010%
4	2.511	361	364	368	rBV2	603	447	0.05%	0.007%
5	2.562	368	380	395	rBV	130803	218646	26.40%	3.511%
6	2.777	444	447	450	rBV	687	489	0.06%	0.008%
7	3.070	533	538	545	rBV2	934	1094	0.13%	0.018%
8	3.276	600	602	604	rBV	484	263	0.03%	0.004%
9	3.369	628	631	634	rBV	774	533	0.06%	0.009%
10	3.559	687	690	695	rVB	949	776	0.09%	0.012%
11	3.601	700	703	706	rBV2	685	444	0.05%	0.007%
12	3.736	742	745	748	rBV	628	427	0.05%	0.007%
13	3.871	783	787	790	rBV2	793	638	0.08%	0.010%
14	4.015	829	832	835	rBV	630	442	0.05%	0.007%
15	4.115	860	863	865	rBV	599	460	0.06%	0.007%
16	4.195	884	888	891	rBV2	778	621	0.07%	0.010%
17	4.215	891	894	897	rBV2	647	465	0.06%	0.007%
18	4.256	905	907	910	rBV	474	265	0.03%	0.004%
19	4.372	940	943	947	rVB2	827	664	0.08%	0.011%
20	4.491	975	980	987	rBV2	822	992	0.12%	0.016%
21	4.626	1010	1022	1047	rBV	108539	286692	34.62%	4.604%
22	4.867	1095	1097	1099	rBV	456	243	0.03%	0.004%
23	4.990	1131	1135	1139	rBV2	873	858	0.10%	0.014%
24	5.064	1143	1158	1175	rVV	162867	356649	43.06%	5.728%
25	5.282	1219	1226	1229	rBV2	879	962	0.12%	0.015%
26	5.453	1276	1279	1281	rBV2	541	354	0.04%	0.006%
27	5.501	1292	1294	1300	rBV2	489	337	0.04%	0.005%
28	5.642	1332	1338	1341	rBV2	800	703	0.08%	0.011%
29	5.723	1341	1363	1384	rBV2	296884	828216	100.00%	13.301%
30	5.900	1415	1418	1420	rBV	431	246	0.03%	0.004%
31	6.247	1514	1526	1543	rBV	262438	490598	59.24%	7.879%
32	6.359	1557	1561	1563	rBV2	839	527	0.06%	0.008%
33	6.488	1598	1601	1603	rBV2	638	452	0.05%	0.007%
34	6.523	1607	1612	1626	rVB5	4433	9130	1.10%	0.147%
35	6.581	1626	1630	1631	rBV	704	428	0.05%	0.007%
36	6.690	1651	1664	1693	rVB	205201	400390	48.34%	6.430%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049092.D
 Acq On : 12 Jun 2022 15:36
 Operator : SY/MD
 Sample : N3255-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CODL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.845	1708	1712	1714	rBV	630	569	0.07%	0.009%
38	7.022	1764	1767	1771	rBV	648	676	0.08%	0.011%
39	7.067	1778	1781	1785	rVB2	799	614	0.07%	0.010%
40	7.096	1785	1790	1794	rBV2	619	643	0.08%	0.010%
41	7.125	1794	1799	1802	rBV2	641	583	0.07%	0.009%
42	7.189	1811	1819	1829	rBV3	2431	4203	0.51%	0.068%
43	7.279	1844	1847	1850	rBV	909	517	0.06%	0.008%
44	7.298	1850	1853	1856	rBV	738	415	0.05%	0.007%
45	7.565	1925	1936	1955	rBV	89833	158656	19.16%	2.548%
46	7.899	2027	2040	2055	rBV	303082	517992	62.54%	8.319%
47	8.086	2095	2098	2100	rBV2	519	272	0.03%	0.004%
48	8.102	2100	2103	2107	rVB2	603	453	0.05%	0.007%
49	8.128	2107	2111	2116	rBV	583	601	0.07%	0.010%
50	8.179	2116	2127	2141	rBV	65974	112102	13.54%	1.800%
51	8.256	2146	2151	2153	rBV3	787	892	0.11%	0.014%
52	8.330	2172	2174	2177	rBV	446	284	0.03%	0.005%
53	8.359	2181	2183	2187	rBV	524	387	0.05%	0.006%
54	8.469	2212	2217	2227	rBV3	940	1601	0.19%	0.026%
55	8.510	2227	2230	2234	rVB2	893	645	0.08%	0.010%
56	8.530	2234	2236	2239	rBV	398	251	0.03%	0.004%
57	8.555	2242	2244	2247	rVB	541	262	0.03%	0.004%
58	8.587	2251	2254	2256	rBV	635	432	0.05%	0.007%
59	8.639	2258	2270	2300	rBV2	304111	596675	72.04%	9.583%
60	8.951	2365	2367	2369	rBV2	427	242	0.03%	0.004%
61	8.986	2373	2378	2382	rBV2	633	734	0.09%	0.012%
62	9.089	2408	2410	2412	rBV	416	271	0.03%	0.004%
63	9.417	2499	2512	2527	rBV	348874	576068	69.56%	9.252%
64	9.639	2578	2581	2584	rBV	672	477	0.06%	0.008%
65	9.793	2624	2629	2631	rBV2	646	574	0.07%	0.009%
66	9.909	2659	2665	2666	rBV	738	680	0.08%	0.011%
67	10.063	2709	2713	2716	rBV	525	516	0.06%	0.008%
68	10.115	2723	2729	2733	rBV4	1866	2182	0.26%	0.035%
69	10.198	2750	2755	2759	rBV2	786	853	0.10%	0.014%
70	10.285	2779	2782	2784	rBV	612	418	0.05%	0.007%
71	10.340	2794	2799	2801	rBV2	859	796	0.10%	0.013%
72	10.420	2819	2824	2829	rVB2	757	749	0.09%	0.012%
73	10.446	2830	2832	2838	rBV	483	337	0.04%	0.005%
74	10.472	2838	2840	2844	rVB	526	324	0.04%	0.005%
75	10.758	2916	2929	2945	rVB	344154	546168	65.95%	8.771%
76	10.822	2945	2949	2954	rBV2	756	676	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049092.D
 Acq On : 12 Jun 2022 15:36
 Operator : SY/MD
 Sample : N3255-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	10.960	2989	2992	2996	rVB2	855	599	0.07%	0.010%
78	10.996	3000	3003	3005	rBV2	594	439	0.05%	0.007%
79	11.185	3060	3062	3064	rBV2	470	251	0.03%	0.004%
80	11.240	3074	3079	3085	rVB2	712	737	0.09%	0.012%
81	11.272	3085	3089	3094	rBV	468	464	0.06%	0.007%
82	11.308	3097	3100	3105	rBV2	717	614	0.07%	0.010%
83	11.343	3108	3111	3116	rVB	930	678	0.08%	0.011%
84	11.372	3116	3120	3123	rBV	813	708	0.09%	0.011%
85	11.420	3131	3135	3139	rBV	977	965	0.12%	0.015%
86	11.761	3238	3241	3244	rVB	995	581	0.07%	0.009%
87	11.812	3244	3257	3275	rBV	277567	437134	52.78%	7.020%
88	11.951	3298	3300	3303	rBV	672	429	0.05%	0.007%
89	12.079	3333	3340	3344	rBV2	881	1155	0.14%	0.019%
90	12.102	3344	3347	3353	rBV2	573	668	0.08%	0.011%
91	12.192	3363	3375	3397	rBV	288710	462793	55.88%	7.432%
92	12.311	3409	3412	3416	rVB2	933	609	0.07%	0.010%
93	12.333	3416	3419	3422	rBV	452	339	0.04%	0.005%
94	12.456	3453	3457	3460	rBV2	571	586	0.07%	0.009%
95	12.533	3478	3481	3483	rBV	762	478	0.06%	0.008%
96	12.568	3488	3492	3498	rBV	808	1057	0.13%	0.017%
97	12.629	3507	3511	3512	rBV	679	458	0.06%	0.007%
98	12.944	3607	3609	3611	rBV	636	371	0.04%	0.006%
99	12.973	3615	3618	3621	rBV	578	324	0.04%	0.005%
100	13.279	3710	3713	3717	rBV3	978	701	0.08%	0.011%




Sum of corrected areas: 6226643

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049092.D
Acq On : 12 Jun 2022 15:36
Operator : SY/MD
Sample : N3255-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

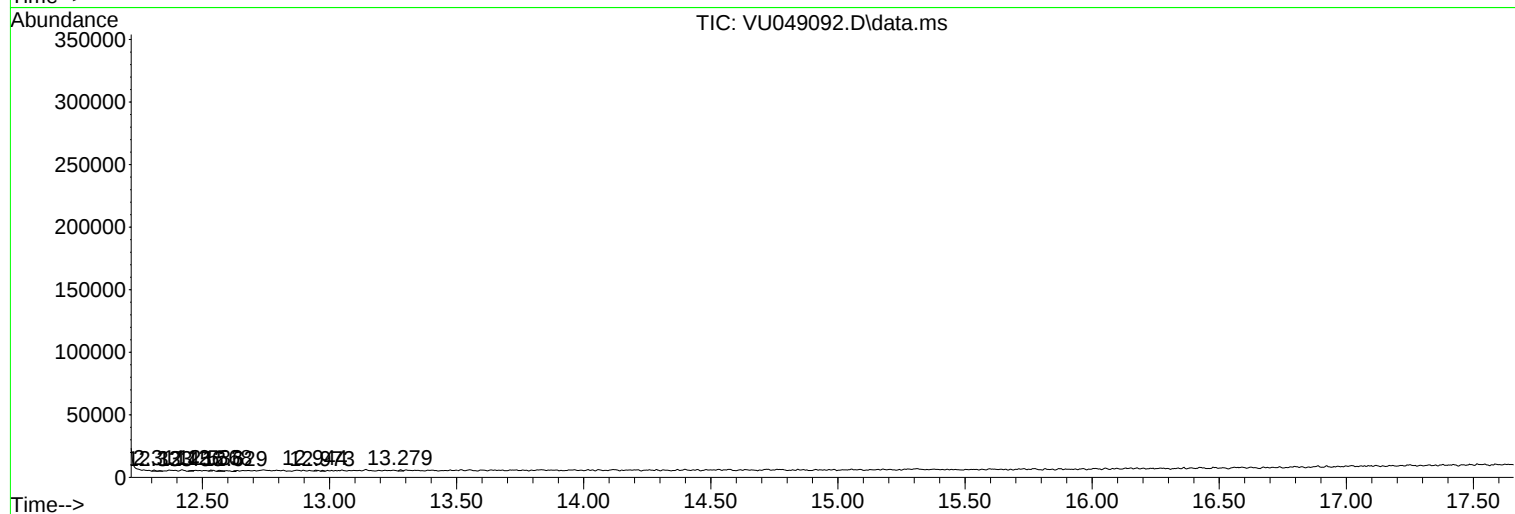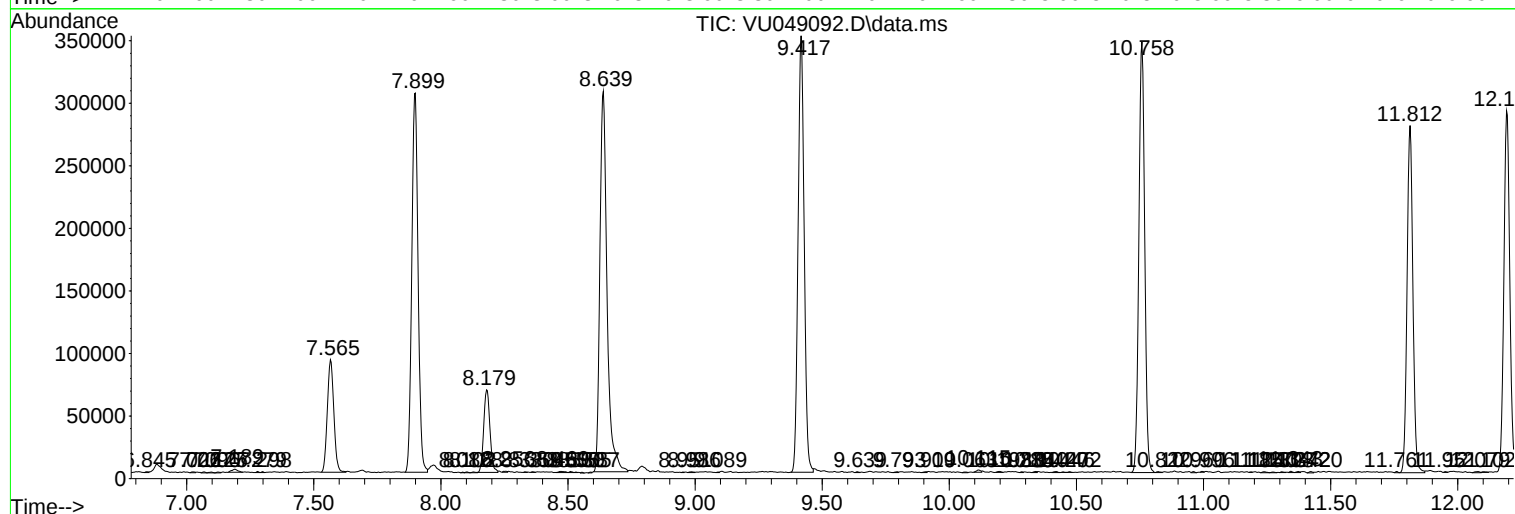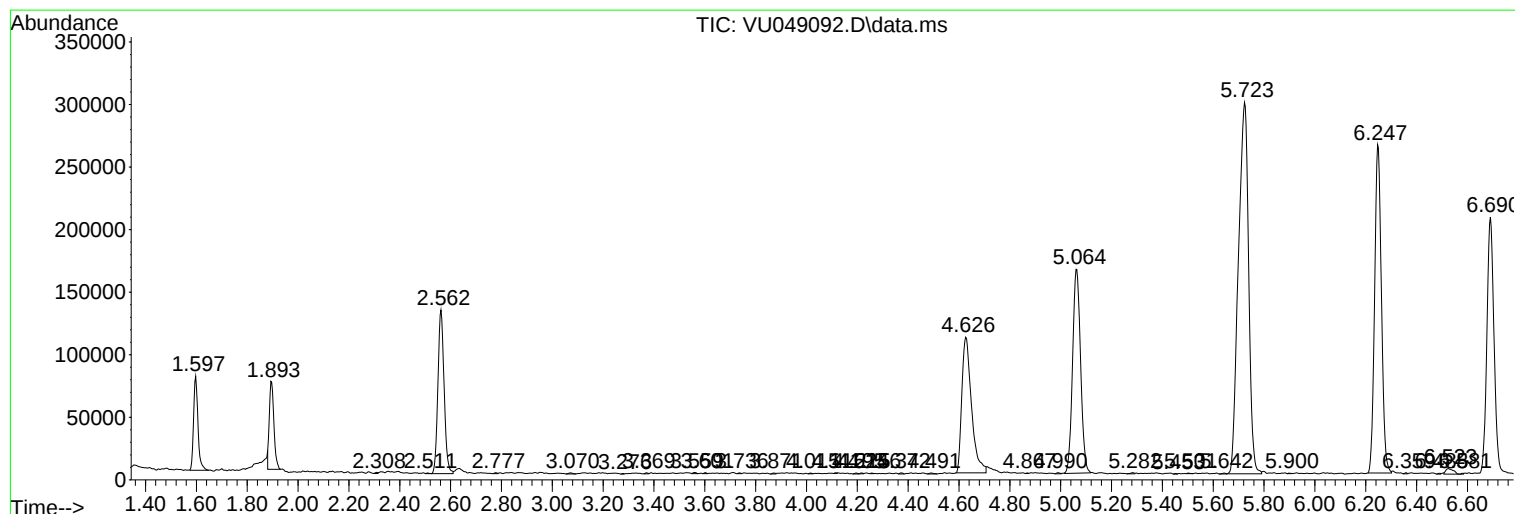

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049092.D
Acq On : 12 Jun 2022 15:36
Operator : SY/MD
Sample : N3255-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049092.D
Acq On : 12 Jun 2022 15:36
Operator : SY/MD
Sample : N3255-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc