

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049093.D
 Acq On : 12 Jun 2022 15:59
 Operator : SY/MD
 Sample : N3255-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049093.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	79048	88284	10.46%	1.355%
2	1.900	167	174	184	rBV	65533	83801	9.93%	1.286%
3	2.440	340	342	343	rBV	389	176	0.02%	0.003%
4	2.565	369	381	395	rBV	145946	240245	28.47%	3.686%
5	2.674	413	415	418	rVB2	561	273	0.03%	0.004%
6	2.694	418	421	423	rBV	410	210	0.02%	0.003%
7	2.713	423	427	428	rBV	510	365	0.04%	0.006%
8	2.829	460	463	466	rBV2	644	395	0.05%	0.006%
9	2.922	488	492	497	rBV2	647	718	0.09%	0.011%
10	3.080	539	541	544	rBV	492	298	0.04%	0.005%
11	3.108	544	550	553	rVV2	471	563	0.07%	0.009%
12	3.510	670	675	677	rBV2	649	562	0.07%	0.009%
13	3.559	685	690	693	rBV2	433	378	0.04%	0.006%
14	3.645	714	717	718	rBV	359	202	0.02%	0.003%
15	3.655	718	720	723	rVB	557	291	0.03%	0.004%
16	3.697	727	733	736	rBV2	862	923	0.11%	0.014%
17	3.890	790	793	796	rBV2	878	578	0.07%	0.009%
18	3.909	796	799	803	rVB	451	250	0.03%	0.004%
19	3.948	806	811	815	rBV2	738	773	0.09%	0.012%
20	3.977	816	820	825	rBV2	414	537	0.06%	0.008%
21	4.073	847	850	853	rBV	571	344	0.04%	0.005%
22	4.118	862	864	870	rVB2	518	368	0.04%	0.006%
23	4.144	870	872	874	rBV	407	221	0.03%	0.003%
24	4.173	878	881	887	rVB	947	949	0.11%	0.015%
25	4.211	887	893	895	rBV	1025	890	0.11%	0.014%
26	4.285	913	916	919	rBV2	1029	829	0.10%	0.013%
27	4.350	934	936	939	rVB	651	341	0.04%	0.005%
28	4.481	974	977	980	rBV	749	665	0.08%	0.010%
29	4.539	993	995	998	rVB2	540	259	0.03%	0.004%
30	4.555	998	1000	1003	rBV	677	426	0.05%	0.007%
31	4.620	1007	1020	1043	rBV	110643	270538	32.06%	4.151%
32	4.784	1069	1071	1076	rBV	735	479	0.06%	0.007%
33	4.822	1080	1083	1085	rBV3	711	446	0.05%	0.007%
34	5.063	1142	1158	1180	rBV	165895	361193	42.80%	5.542%
35	5.163	1186	1189	1191	rBV	569	399	0.05%	0.006%
36	5.205	1198	1202	1208	rVB3	1010	1135	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049093.D
 Acq On : 12 Jun 2022 15:59
 Operator : SY/MD
 Sample : N3255-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.240	1208	1213	1215	rBV	844	768	0.09%	0.012%
38	5.282	1223	1226	1229	rBV2	839	742	0.09%	0.011%
39	5.436	1270	1274	1276	rBV	644	467	0.06%	0.007%
40	5.584	1317	1320	1323	rBV	542	392	0.05%	0.006%
41	5.642	1335	1338	1341	rBV	617	518	0.06%	0.008%
42	5.722	1343	1363	1390	rVV2	300546	843903	100.00%	12.948%
43	5.854	1396	1404	1408	rBV3	1317	1933	0.23%	0.030%
44	5.948	1430	1433	1436	rBV2	1530	1137	0.13%	0.017%
45	6.041	1459	1462	1465	rBV	637	503	0.06%	0.008%
46	6.086	1471	1476	1480	rBV	1188	1278	0.15%	0.020%
47	6.131	1486	1490	1494	rBV	761	631	0.07%	0.010%
48	6.182	1503	1506	1508	rBV	353	206	0.02%	0.003%
49	6.195	1508	1510	1512	rBV2	413	210	0.02%	0.003%
50	6.247	1513	1526	1546	rVV	284913	540901	64.10%	8.299%
51	6.578	1627	1629	1630	rBV2	261	105	0.01%	0.002%
52	6.690	1650	1664	1679	rBV2	207406	401055	47.52%	6.153%
53	6.806	1694	1700	1706	rBV3	904	1328	0.16%	0.020%
54	6.903	1727	1730	1732	rBV	325	233	0.03%	0.004%
55	6.999	1758	1760	1762	rBV	396	177	0.02%	0.003%
56	7.038	1766	1772	1775	rBV	838	891	0.11%	0.014%
57	7.153	1805	1808	1809	rBV	518	263	0.03%	0.004%
58	7.269	1841	1844	1848	rBV	539	488	0.06%	0.007%
59	7.446	1896	1899	1901	rVB	422	212	0.03%	0.003%
60	7.475	1905	1908	1910	rBV	633	456	0.05%	0.007%
61	7.565	1920	1936	1952	rBV2	93828	164683	19.51%	2.527%
62	7.771	1997	2000	2003	rBV	875	648	0.08%	0.010%
63	7.819	2008	2015	2020	rBV2	613	896	0.11%	0.014%
64	7.896	2024	2039	2054	rBV	334668	578775	68.58%	8.880%
65	8.179	2116	2127	2143	rBV	67237	111952	13.27%	1.718%
66	8.288	2157	2161	2164	rBV2	780	698	0.08%	0.011%
67	8.501	2225	2227	2231	rBV	400	356	0.04%	0.005%
68	8.578	2246	2251	2253	rBV	978	733	0.09%	0.011%
69	8.632	2257	2268	2299	rVV2	281690	553470	65.58%	8.492%
70	8.938	2360	2363	2364	rBV	442	295	0.03%	0.005%
71	8.999	2379	2382	2384	rBV	373	240	0.03%	0.004%
72	9.050	2395	2398	2401	rBV	507	334	0.04%	0.005%
73	9.327	2479	2484	2487	rBV2	706	787	0.09%	0.012%
74	9.417	2499	2512	2533	rBV	399792	655507	77.68%	10.057%
75	9.845	2639	2645	2651	rBV	976	1235	0.15%	0.019%
76	9.925	2666	2670	2673	rBV	669	660	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
 Data File : VU049093.D
 Acq On : 12 Jun 2022 15:59
 Operator : SY/MD
 Sample : N3255-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

77	10.166	2743	2745	2747	rBV	440	266	0.03%	0.004%
78	10.272	2775	2778	2780	rBV	462	260	0.03%	0.004%
79	10.436	2826	2829	2831	rBV	592	423	0.05%	0.006%
80	10.754	2917	2928	2947	rVB	333478	531149	62.94%	8.149%
81	11.063	3019	3024	3027	rBV	1336	1186	0.14%	0.018%
82	11.234	3074	3077	3080	rBV	633	439	0.05%	0.007%
83	11.388	3122	3125	3129	rBV2	853	685	0.08%	0.011%
84	11.680	3213	3216	3222	rBV2	567	698	0.08%	0.011%
85	11.812	3245	3257	3271	rBV	326542	525455	62.26%	8.062%
86	12.192	3364	3375	3396	rBB	316078	525438	62.26%	8.062%
87	12.561	3487	3490	3493	rBV2	772	584	0.07%	0.009%
88	12.716	3536	3538	3541	rBV2	926	676	0.08%	0.010%
89	13.066	3644	3647	3654	rBV2	928	972	0.12%	0.015%




Sum of corrected areas: 6517601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049093.D
Acq On : 12 Jun 2022 15:59
Operator : SY/MD
Sample : N3255-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

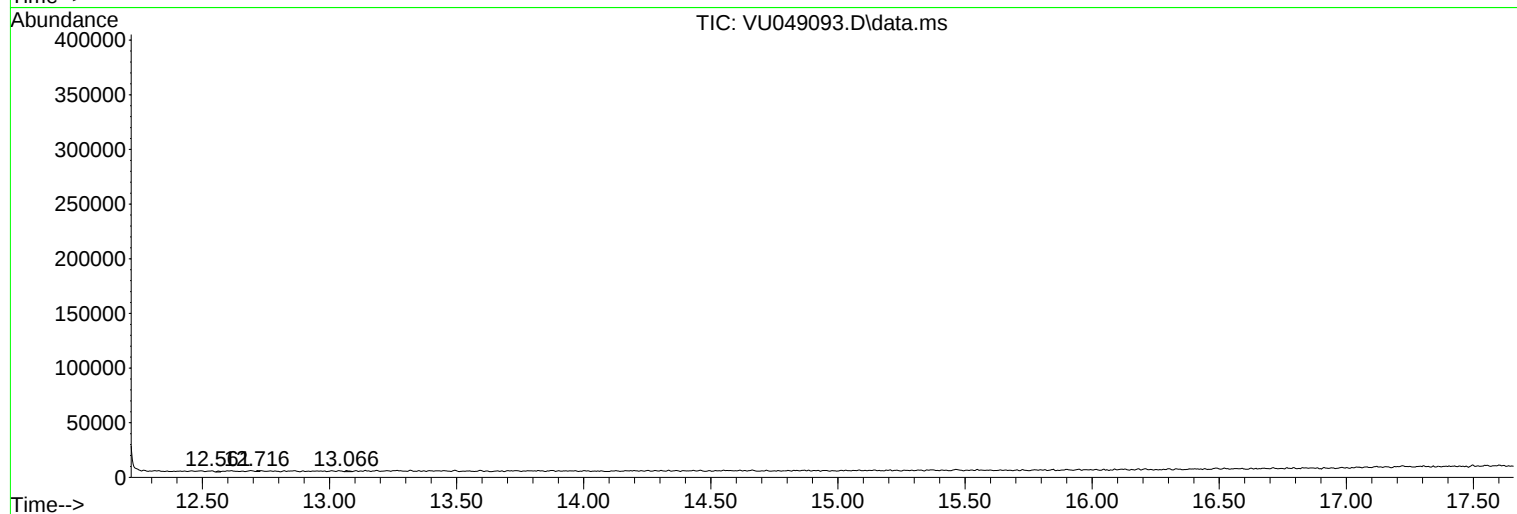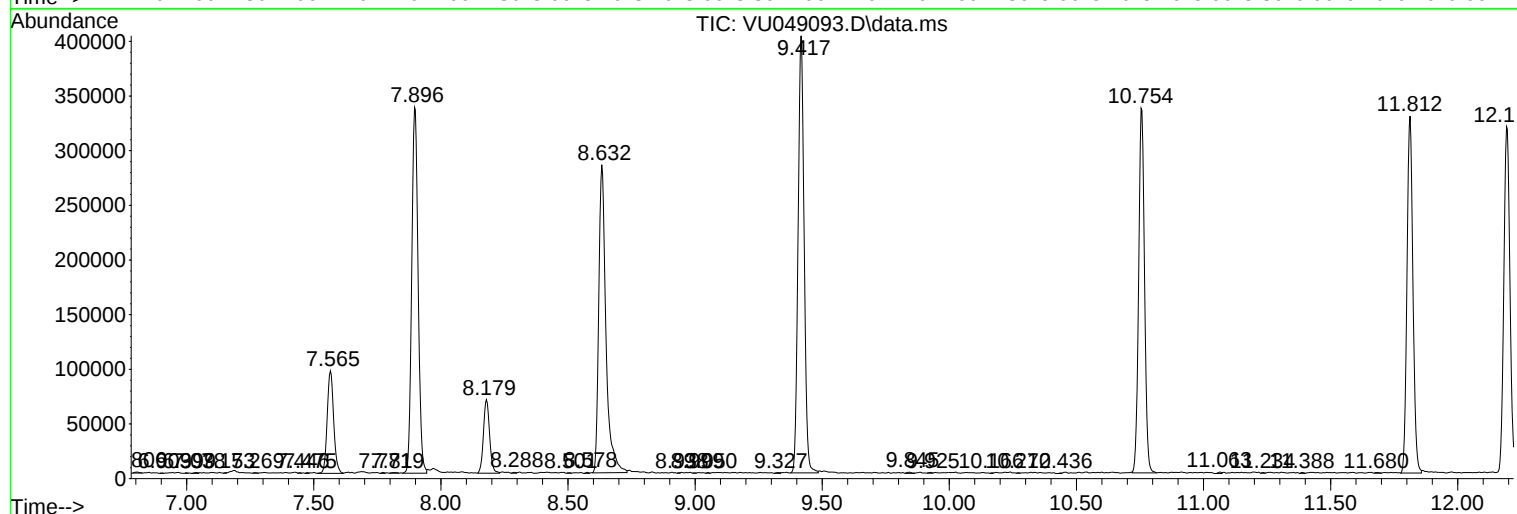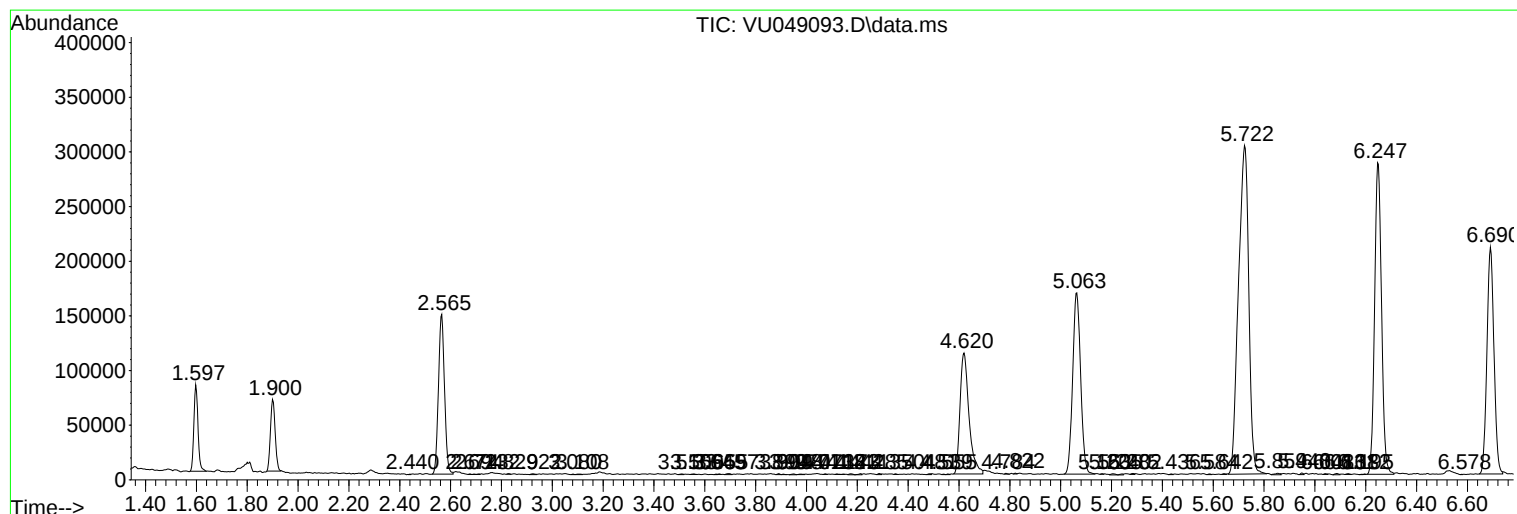

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049093.D
Acq On : 12 Jun 2022 15:59
Operator : SY/MD
Sample : N3255-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061222\
Data File : VU049093.D
Acq On : 12 Jun 2022 15:59
Operator : SY/MD
Sample : N3255-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------